
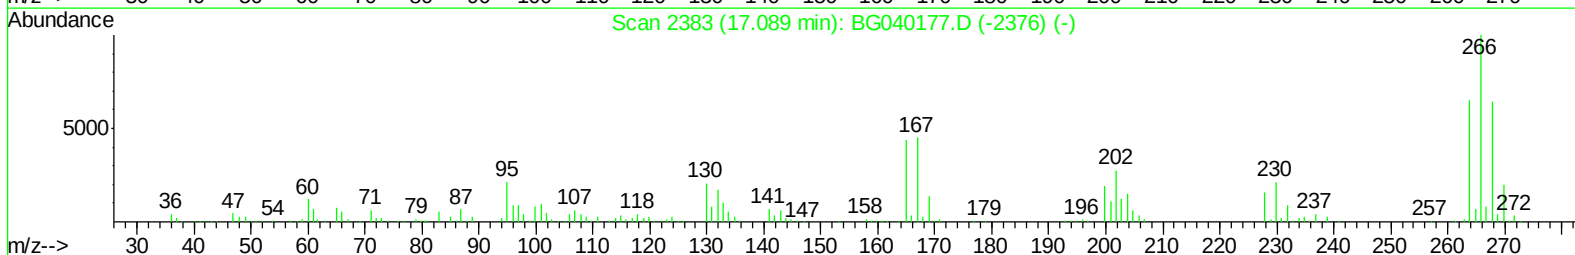
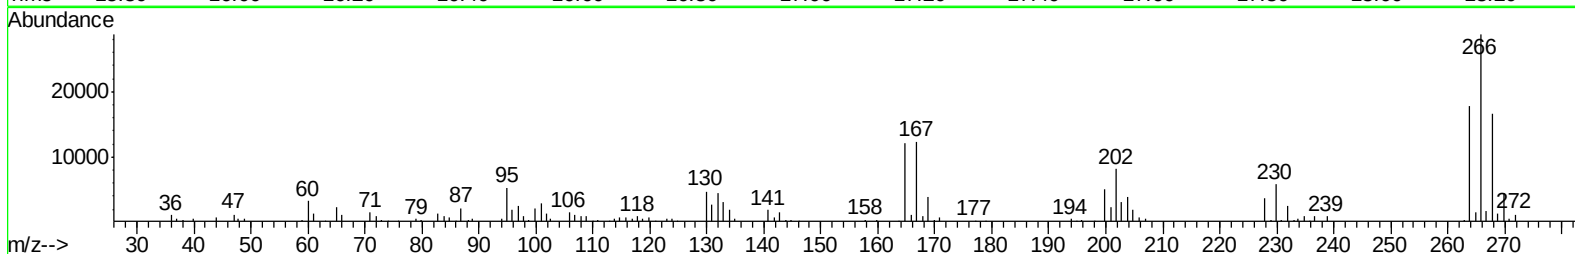


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041619\
 Data File : BG040517.D
 Acq On : 17 Apr 2019 00:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:35:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 13 00:33:11 2019
 Response via : Initial Calibration

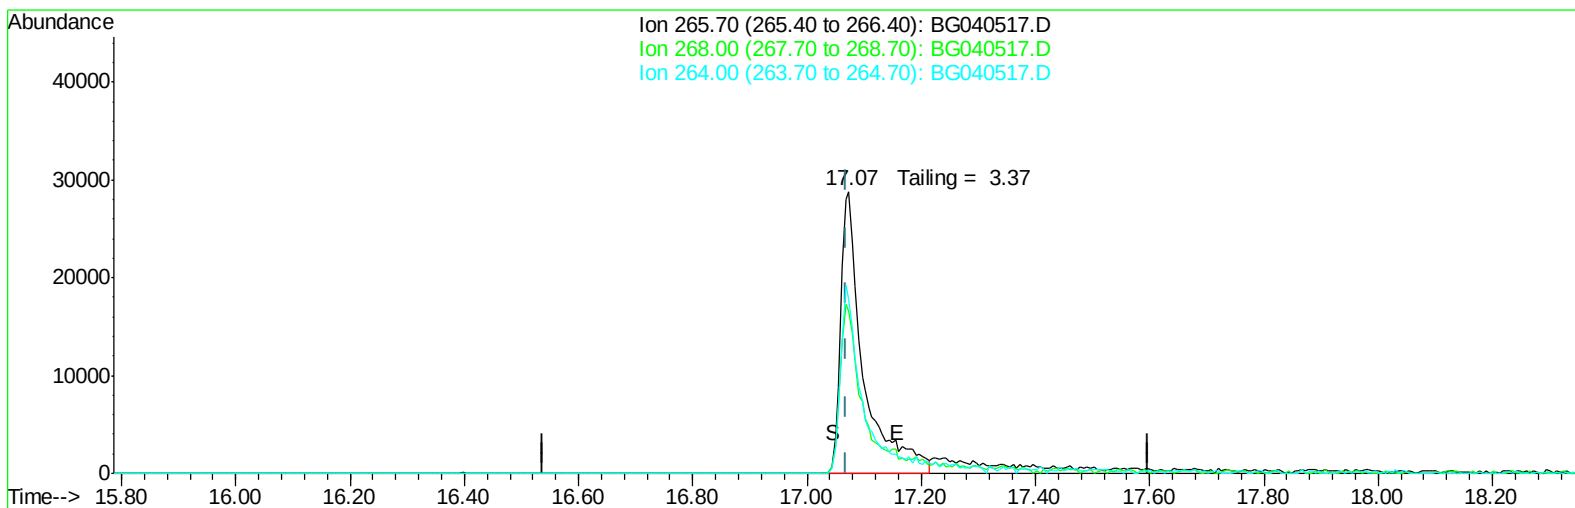

TIC: BG040517.D

(70) Pentachlorophenol (C)




17.073min (+0.004) 25839.92ng

response 79784

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	57.78
264.00	64.80	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041619\
Data File : BG040517.D
Acq On : 17 Apr 2019 00:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:35:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration

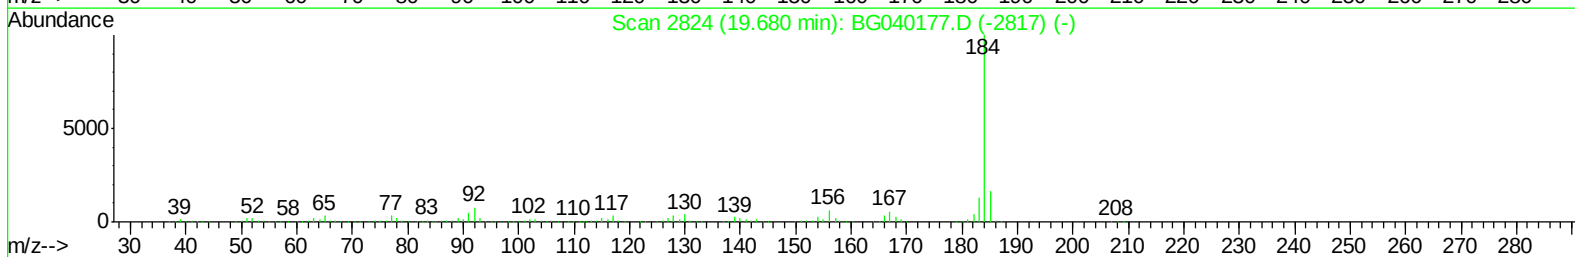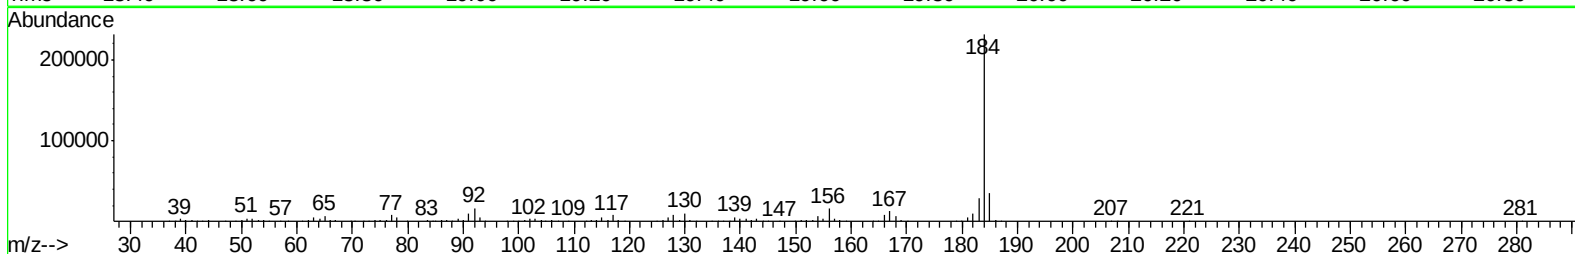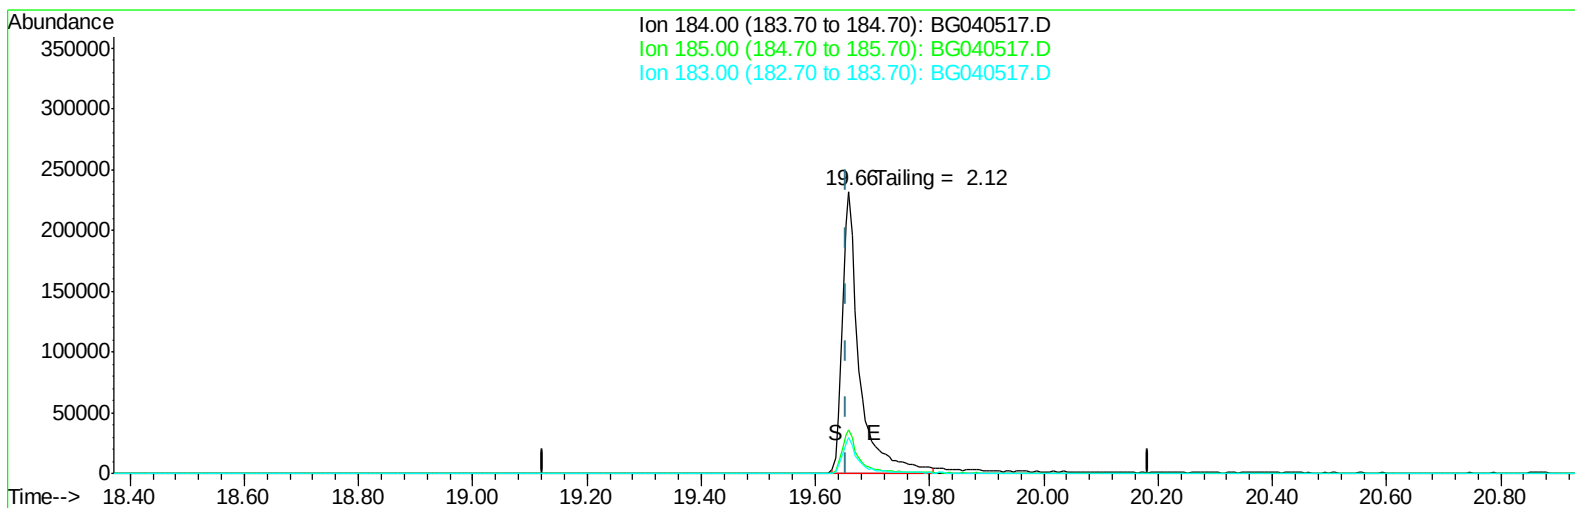

TIC: BG040517.D

(77) Benzidine

19.658min (+0.004) 241919.54ng

response 497951

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	15.31
183.00	12.90	12.64
0.00	0.00	0.00