

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041619\
 Data File : BG040510.D
 Acq On : 16 Apr 2019 19:30
 Operator : JU/SJ
 Sample : K2423-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP2-A

Quant Time: Apr 17 02:33:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	62638	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	248656	20.00	ng	-0.03
39) Acenaphthene-d10	14.67	164	159252	20.00	ng	-0.03
64) Phenanthrene-d10	17.42	188	404907	20.00	ng	-0.03
76) Chrysene-d12	21.69	240	360804	20.00	ng	-0.04
87) Perylene-d12	24.97	264	381217	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	513508	136.28	ng	-0.02
7) Phenol-d6	7.20	99	730360	140.26	ng	-0.02
23) Nitrobenzene-d5	9.22	82	442969	94.69	ng	-0.03
42) 2,4,6-Tribromophenol	16.17	330	257187	149.43	ng	-0.02
45) 2-Fluorobiphenyl	13.29	172	944175	87.85	ng	-0.03
79) Terphenyl-d14	20.02	244	1407679	87.77	ng	-0.03
Target Compounds						
50) Dimethylphthalate	14.12	163	156979	12.595	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041619\
Data File : BG040510.D
Acq On : 16 Apr 2019 19:30
Operator : JU/SJ
Sample : K2423-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP2-A

Quant Time: Apr 17 02:33:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

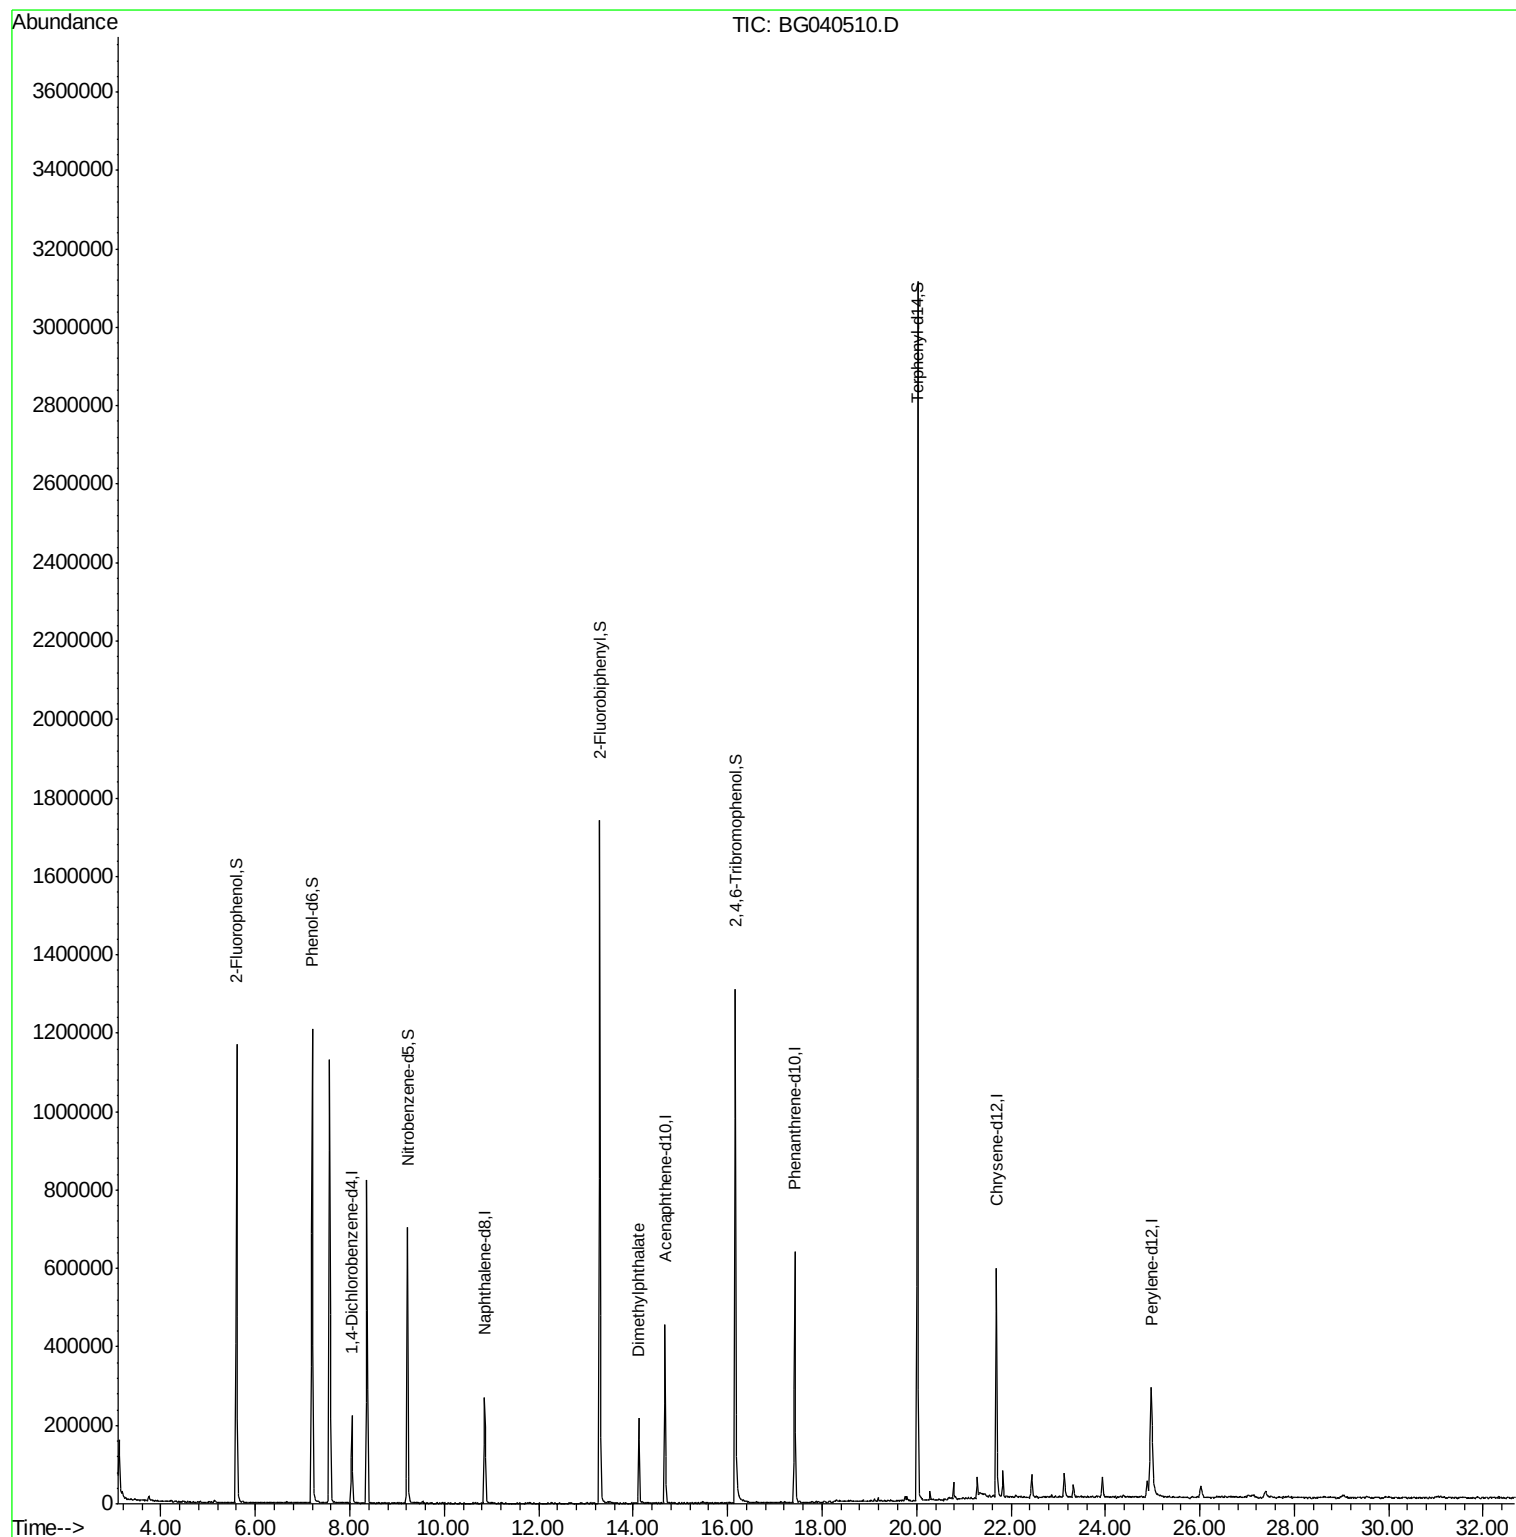

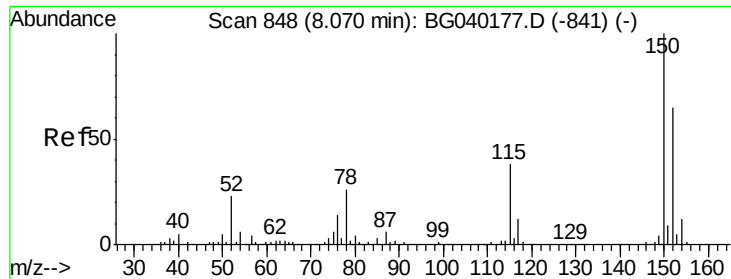


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.02 min
Lab File: BG040510.D
Acq: 16 Apr 2019 19:30

Instrument :
BNA_G
ClientSampleId :
TP2-A

Tgt Ion:152 Resp: 62638
Ion Ratio Lower Upper
152 100
150 149.3 123.7 185.5
115 56.7 46.9 70.3

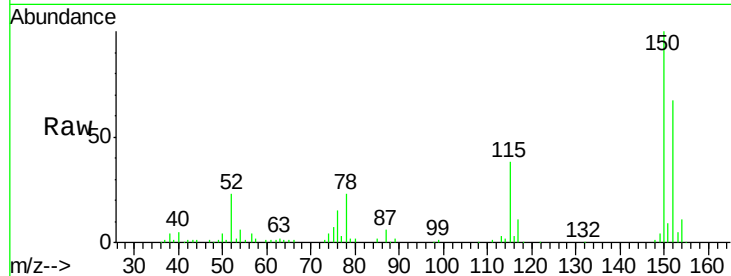


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

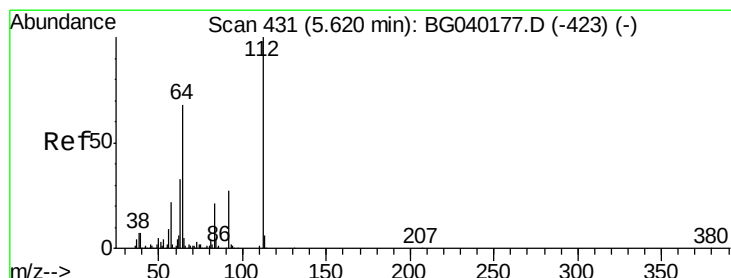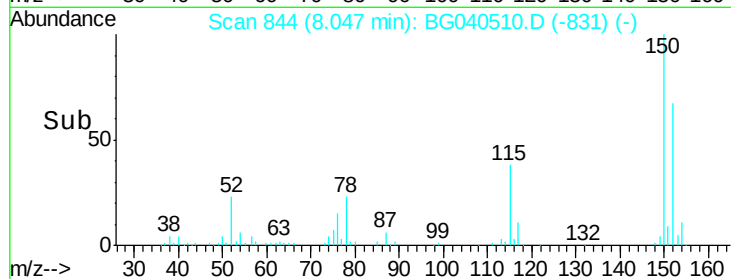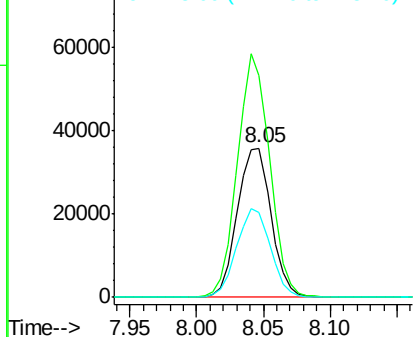



#5


2-Fluorophenol
Concen: 136.285 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.02 min
Lab File: BG040510.D
Acq: 16 Apr 2019 19:30

Tgt Ion:112 Resp: 513508
Ion Ratio Lower Upper
112 100
64 66.4 54.2 81.2
63 33.6 26.4 39.6

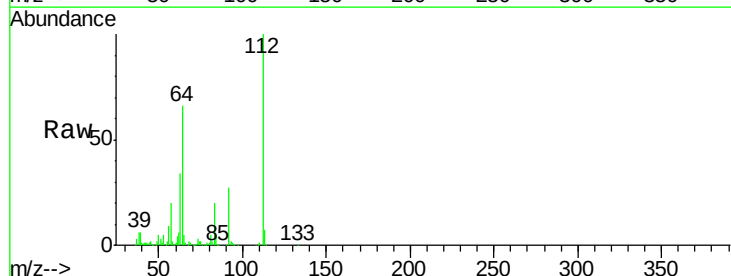

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

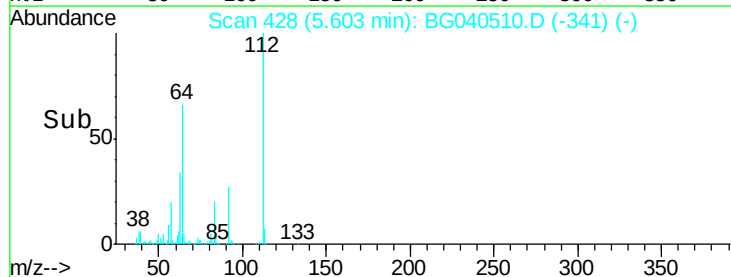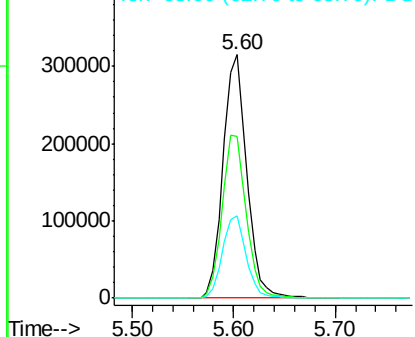

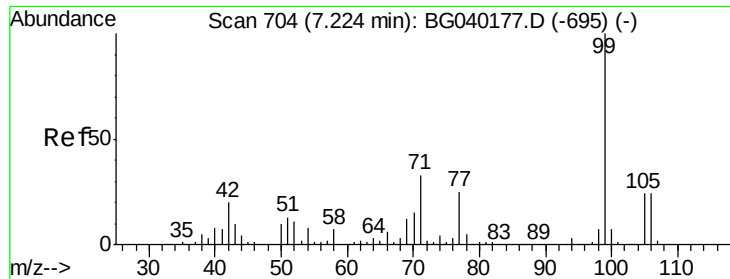

#7

Phenol-d6

Concen: 140.257 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.02 min

Lab File: BG040510.D

Acq: 16 Apr 2019 19:30

Instrument :

BNA_G

ClientSampleId :

TP2-A


Tgt Ion: 99 Resp: 730360

Ion Ratio Lower Upper




99 100

42 19.7 16.2 24.2

71 34.3 26.8 40.2

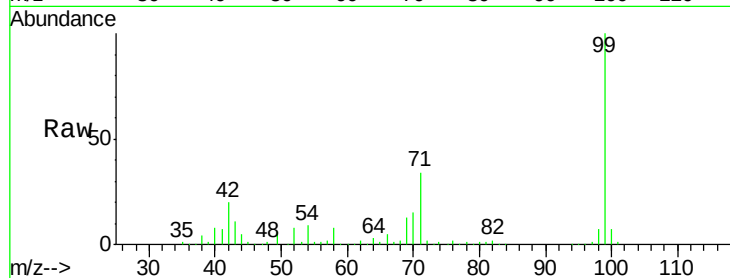

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

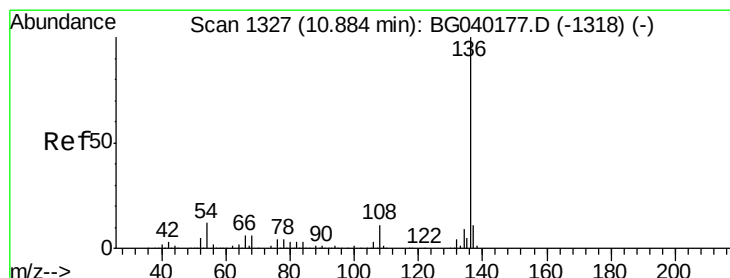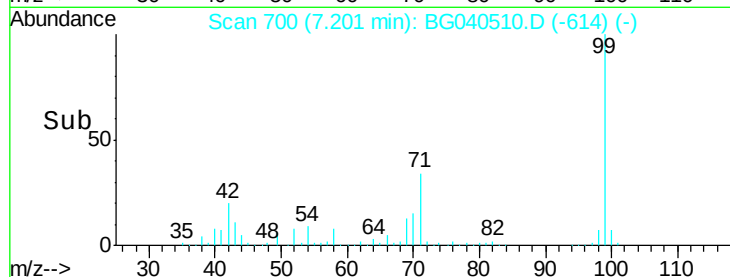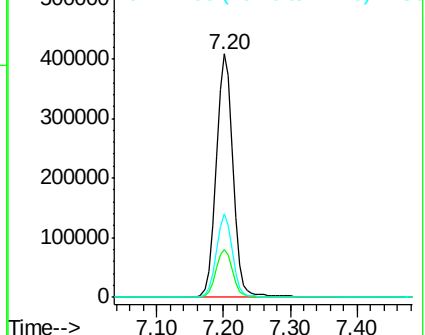

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1322

Delta R.T. -0.03 min

Lab File: BG040510.D

Acq: 16 Apr 2019 19:30

Tgt Ion: 136 Resp: 248656


Ion Ratio Lower Upper

136 100



137 11.2 8.9 13.3


54 10.7 9.6 14.4

68 6.9 5.1 7.7

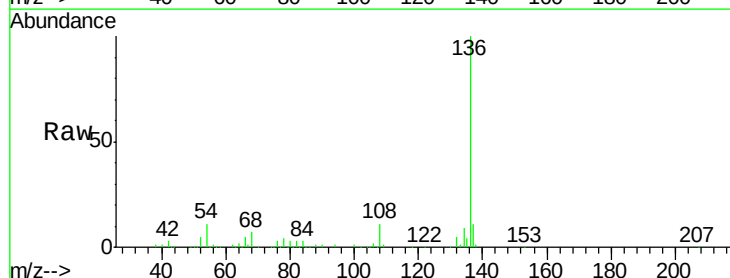

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

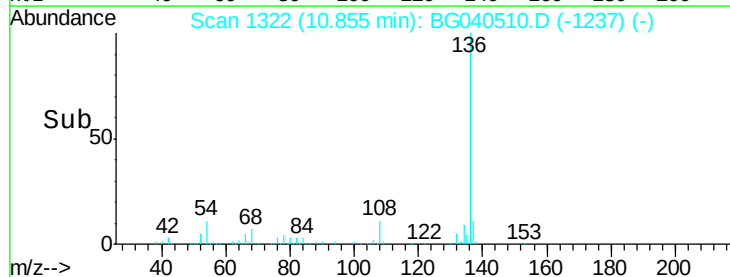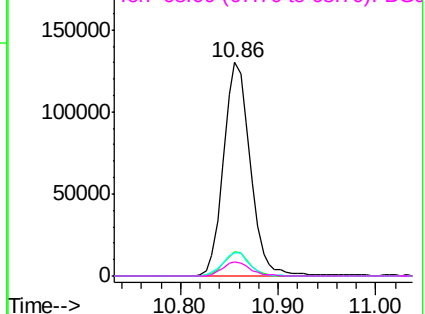


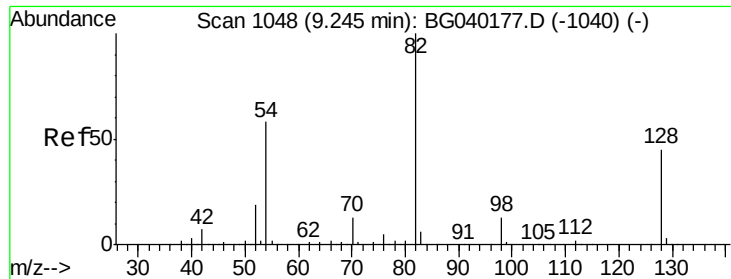




#23
Nitrobenzene-d5
Concen: 94.690 ng
RT: 9.22 min Scan# 1043
Delta R.T. -0.03 min
Lab File: BG040510.D
Acq: 16 Apr 2019 19:30

Instrument :
BNA_G
ClientSampleId :
TP2-A

Tgt Ion: 82 Resp: 442969
Ion Ratio Lower Upper
82 100
128 42.7 35.8 53.8
54 55.9 46.2 69.2

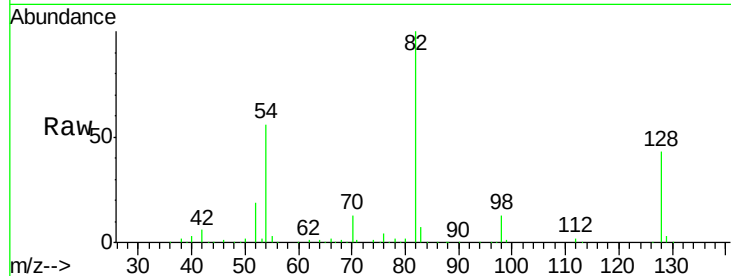


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

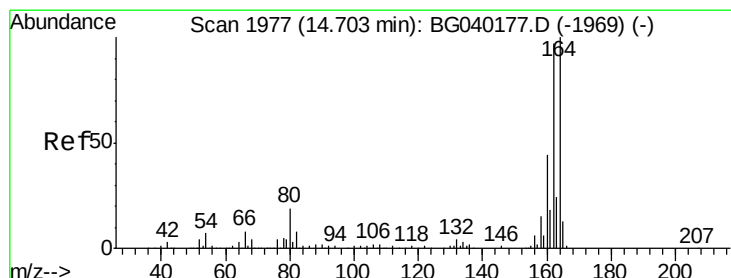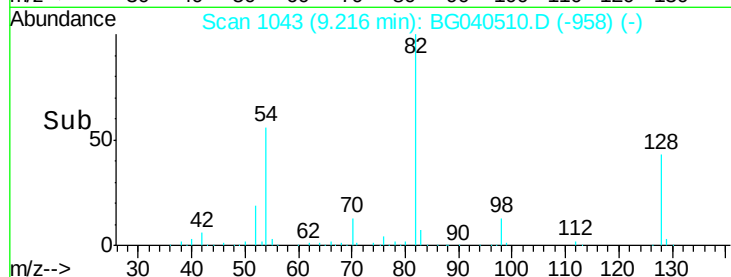
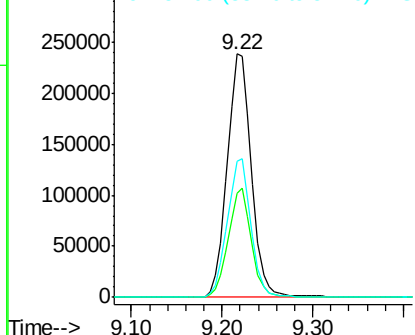



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1972
Delta R.T. -0.03 min
Lab File: BG040510.D
Acq: 16 Apr 2019 19:30

Tgt Ion: 164 Resp: 159252
Ion Ratio Lower Upper
164 100
162 102.6 77.4 116.2
160 46.4 35.3 52.9

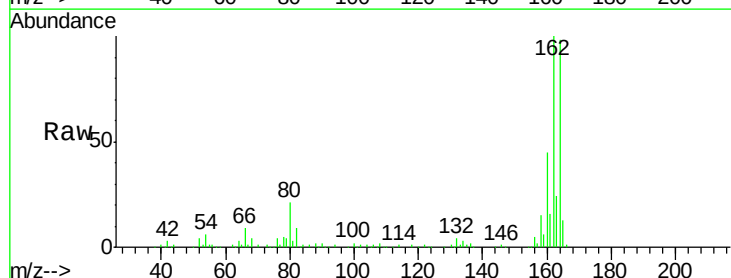

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

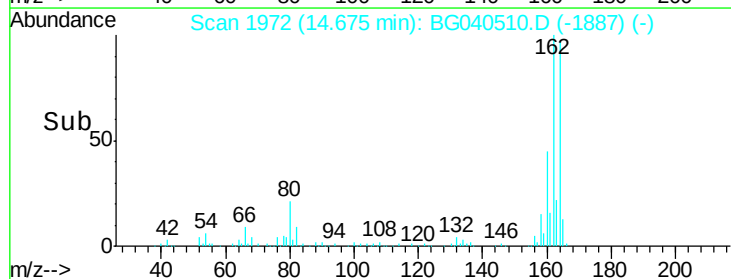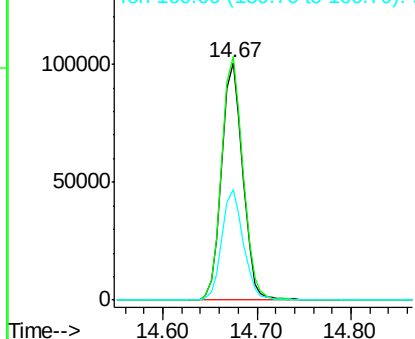

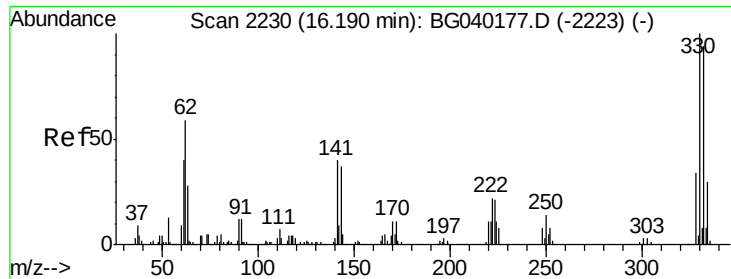

#42

2,4,6-Tribromophenol

Concen: 149.432 ng

RT: 16.17 min Scan# 2226

Delta R.T. -0.02 min

Lab File: BG040510.D

Acq: 16 Apr 2019 19:30

Instrument :

BNA_G

ClientSampleId :

TP2-A


Tgt Ion:330 Resp: 257187

Ion Ratio Lower Upper

330 100

332 94.4 76.6 115.0




141 40.0 32.6 48.8

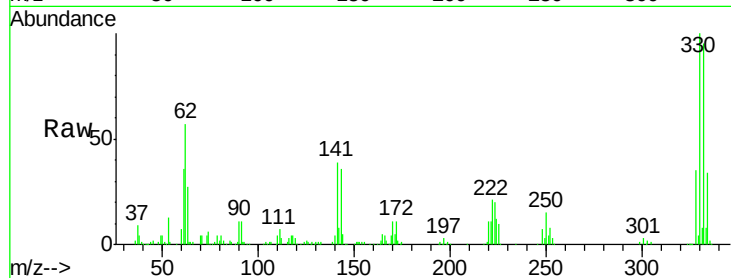

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

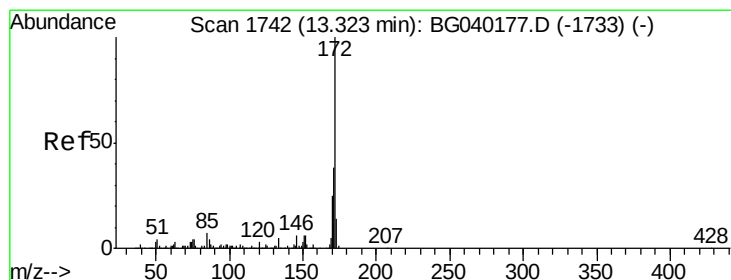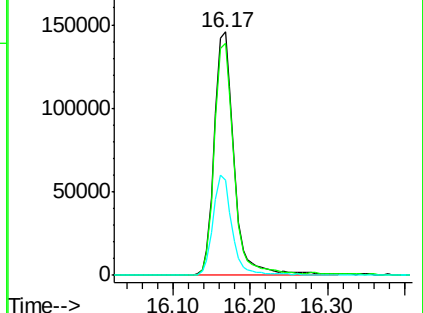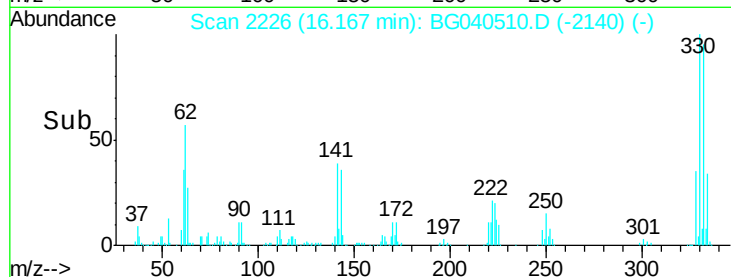

#45

2-Fluorobiphenyl

Concen: 87.851 ng

RT: 13.29 min Scan# 1737

Delta R.T. -0.03 min

Lab File: BG040510.D

Acq: 16 Apr 2019 19:30


Tgt Ion:172 Resp: 944175

Ion Ratio Lower Upper

172 100

171 37.7 30.5 45.7



170 24.6 20.1 30.1

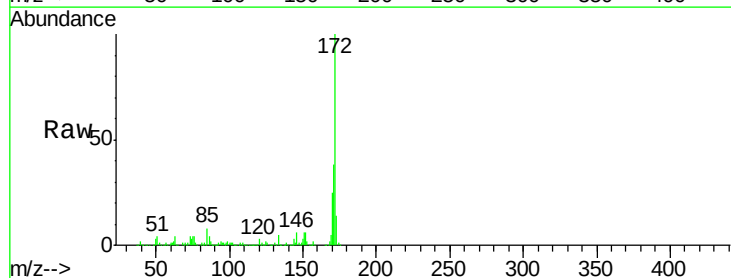


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

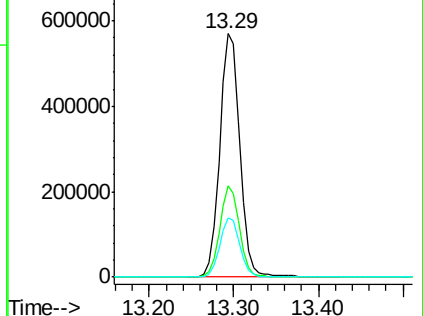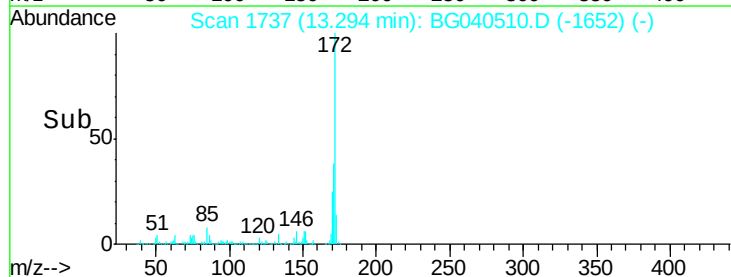

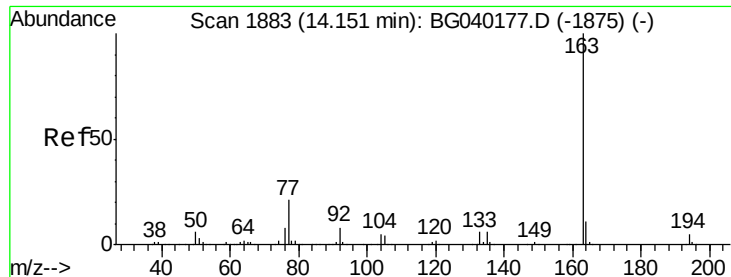

#50

Dimethylphthalate

Concen: 12.595 ng

RT: 14.12 min Scan# 1878

Delta R.T. -0.03 min

Lab File: BG040510.D

Acq: 16 Apr 2019 19:30

Instrument :

BNA_G

ClientSampleId :

TP2-A


Tgt Ion:163 Resp: 156979

Ion Ratio Lower Upper

163 100

194 4.4 4.1 6.1




164 9.2 8.6 13.0

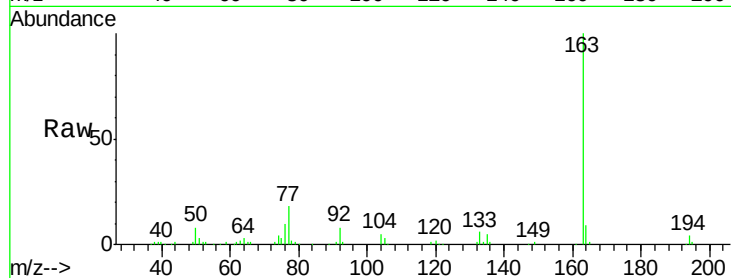

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

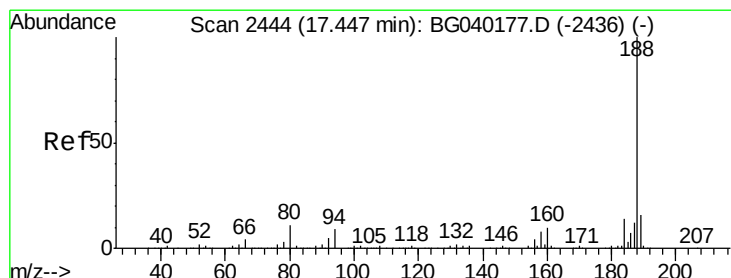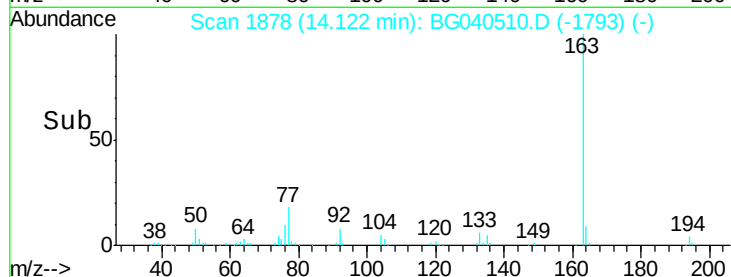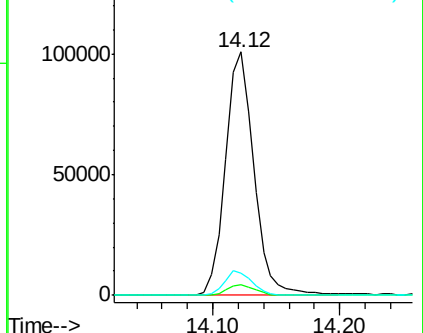

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2439

Delta R.T. -0.03 min

Lab File: BG040510.D

Acq: 16 Apr 2019 19:30


Tgt Ion:188 Resp: 404907

Ion Ratio Lower Upper

188 100

94 9.5 7.0 10.4



80 10.1 8.6 13.0

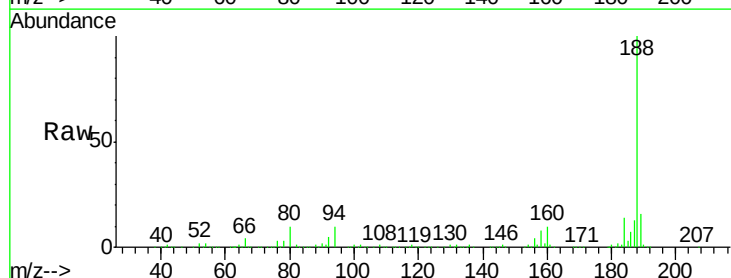


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0



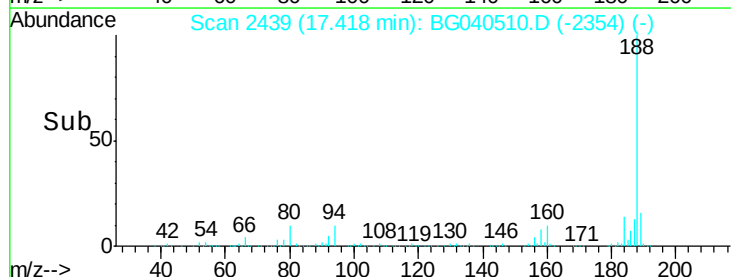
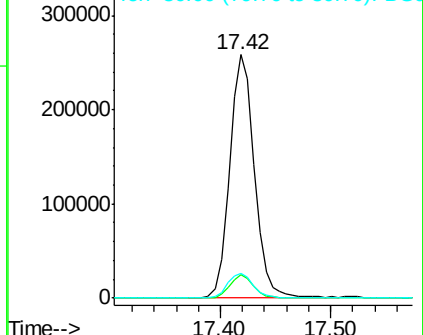


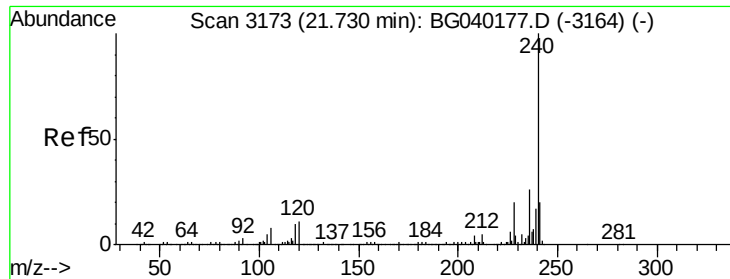

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.69 min Scan# 3166
Delta R.T. -0.04 min
Lab File: BG040510.D
Acq: 16 Apr 2019 19:30




Instrument :
BNA_G
ClientSampleId :
TP2-A




Tgt Ion:240 Resp: 360804
Ion Ratio Lower Upper
240 100
120 11.5 8.4 12.6
236 27.2 20.8 31.2

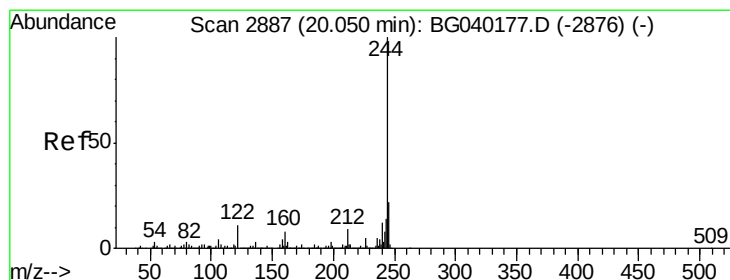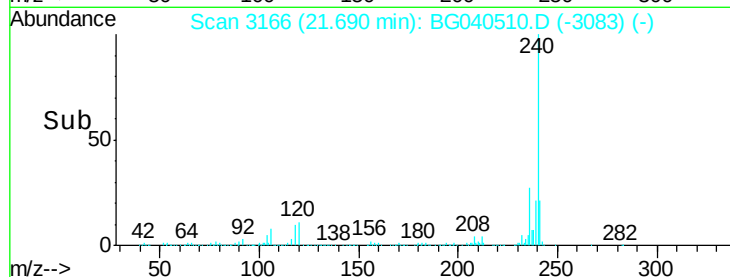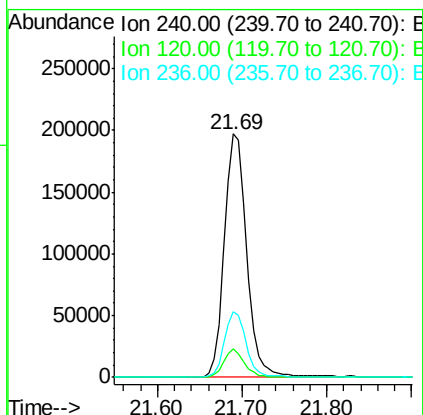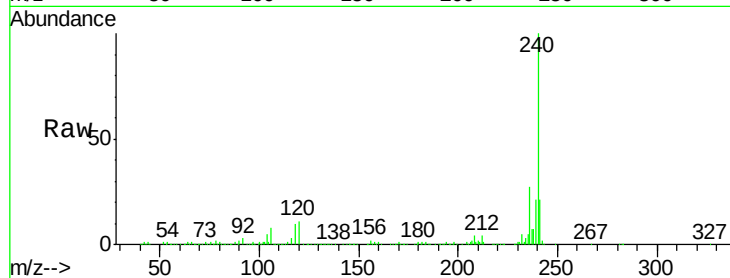

#79
Terphenyl-d14
Concen: 87.770 ng
RT: 20.02 min Scan# 2882
Delta R.T. -0.03 min
Lab File: BG040510.D
Acq: 16 Apr 2019 19:30

Tgt Ion:244 Resp: 1407679
Ion Ratio Lower Upper
244 100
212 9.2 7.0 10.6
122 11.9 8.5 12.7

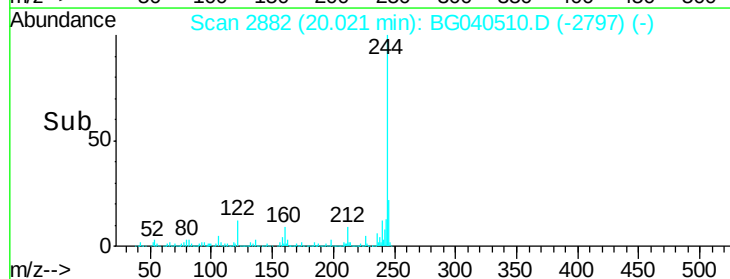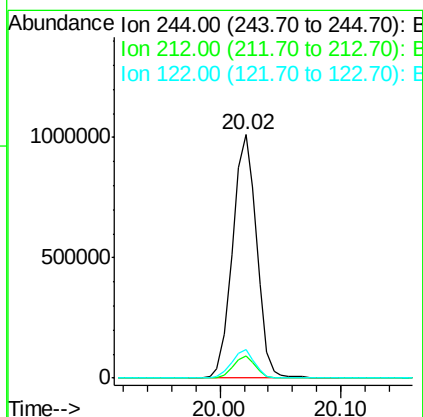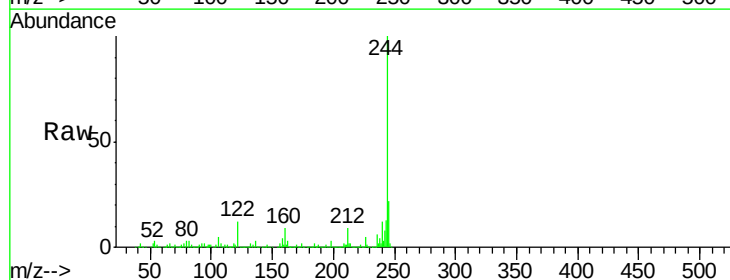

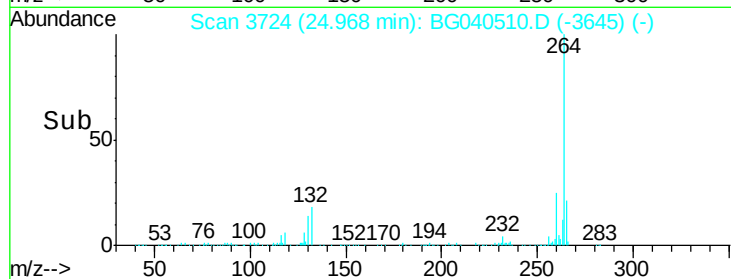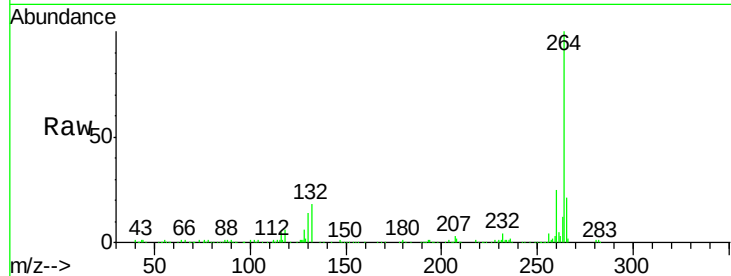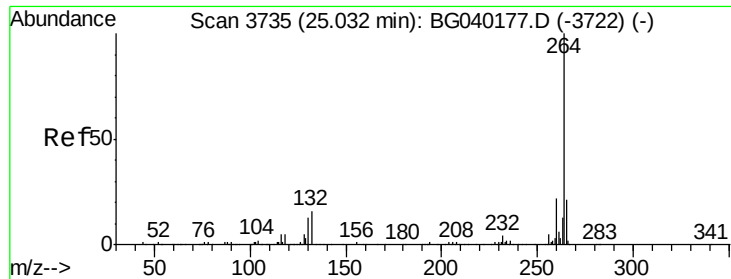

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.97 min Scan# 3724

Delta R.T. -0.06 min

Lab File: BG040510.D

Acq: 16 Apr 2019 19:30

Instrument :

BNA_G

ClientSampleId :

TP2-A

Tgt Ion:264 Resp: 381217

Ion Ratio Lower Upper

264 100

260 25.0 17.9 26.9

265 21.1 16.8 25.2

