

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041619\
 Data File : BG040508.D
 Acq On : 16 Apr 2019 18:09
 Operator : JU/SJ
 Sample : K2423-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP1-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.602	421	428	440	rBV	1133886	1853956	47.37%	8.127%
2	7.200	692	700	716	rBV	1129442	2036523	52.03%	8.928%
3	7.576	755	764	779	rBV	1109225	1944435	49.68%	8.524%
4	8.040	835	843	854	rBV	213075	370415	9.46%	1.624%
5	8.363	889	898	908	rBV	801541	1410854	36.04%	6.185%
6	9.221	1036	1044	1057	rBV	651492	1235040	31.55%	5.414%
7	10.855	1315	1322	1336	rBV	253030	495901	12.67%	2.174%
8	13.293	1729	1737	1752	rBV	1610078	2591574	66.21%	11.361%
9	14.121	1873	1878	1891	rBV	187416	294990	7.54%	1.293%
10	14.674	1965	1972	1984	rBV2	444955	715159	18.27%	3.135%
11	16.166	2219	2226	2252	rBV	1302819	2236157	57.13%	9.803%
12	17.423	2433	2440	2453	rBV	614714	1015187	25.94%	4.450%
13	20.020	2876	2882	2900	rBV	2985727	3914171	100.00%	17.159%
14	20.784	3007	3012	3016	rBV2	34697	40757	1.04%	0.179%
15	21.284	3093	3097	3101	rBV	38575	52822	1.35%	0.232%
16	21.689	3160	3166	3179	rBV2	594605	1057470	27.02%	4.636%
17	21.830	3185	3190	3194	rBV2	47719	67530	1.73%	0.296%
18	22.435	3288	3293	3301	rBV	48017	79418	2.03%	0.348%
19	23.129	3405	3411	3420	rVB2	47861	94181	2.41%	0.413%
20	23.939	3541	3549	3556	rBV3	44887	97903	2.50%	0.429%
21	24.891	3702	3711	3715	rBV2	39730	93264	2.38%	0.409%
22	24.973	3715	3725	3747	rVB3	297674	991708	25.34%	4.347%
23	26.025	3897	3904	3914	rVB5	25974	74890	1.91%	0.328%
24	27.382	4127	4135	4146	rBV8	13828	47001	1.20%	0.206%


Sum of corrected areas: 22811306

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041619\
Data File : BG040508.D
Acq On : 16 Apr 2019 18:09
Operator : JU/SJ
Sample : K2423-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP1-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

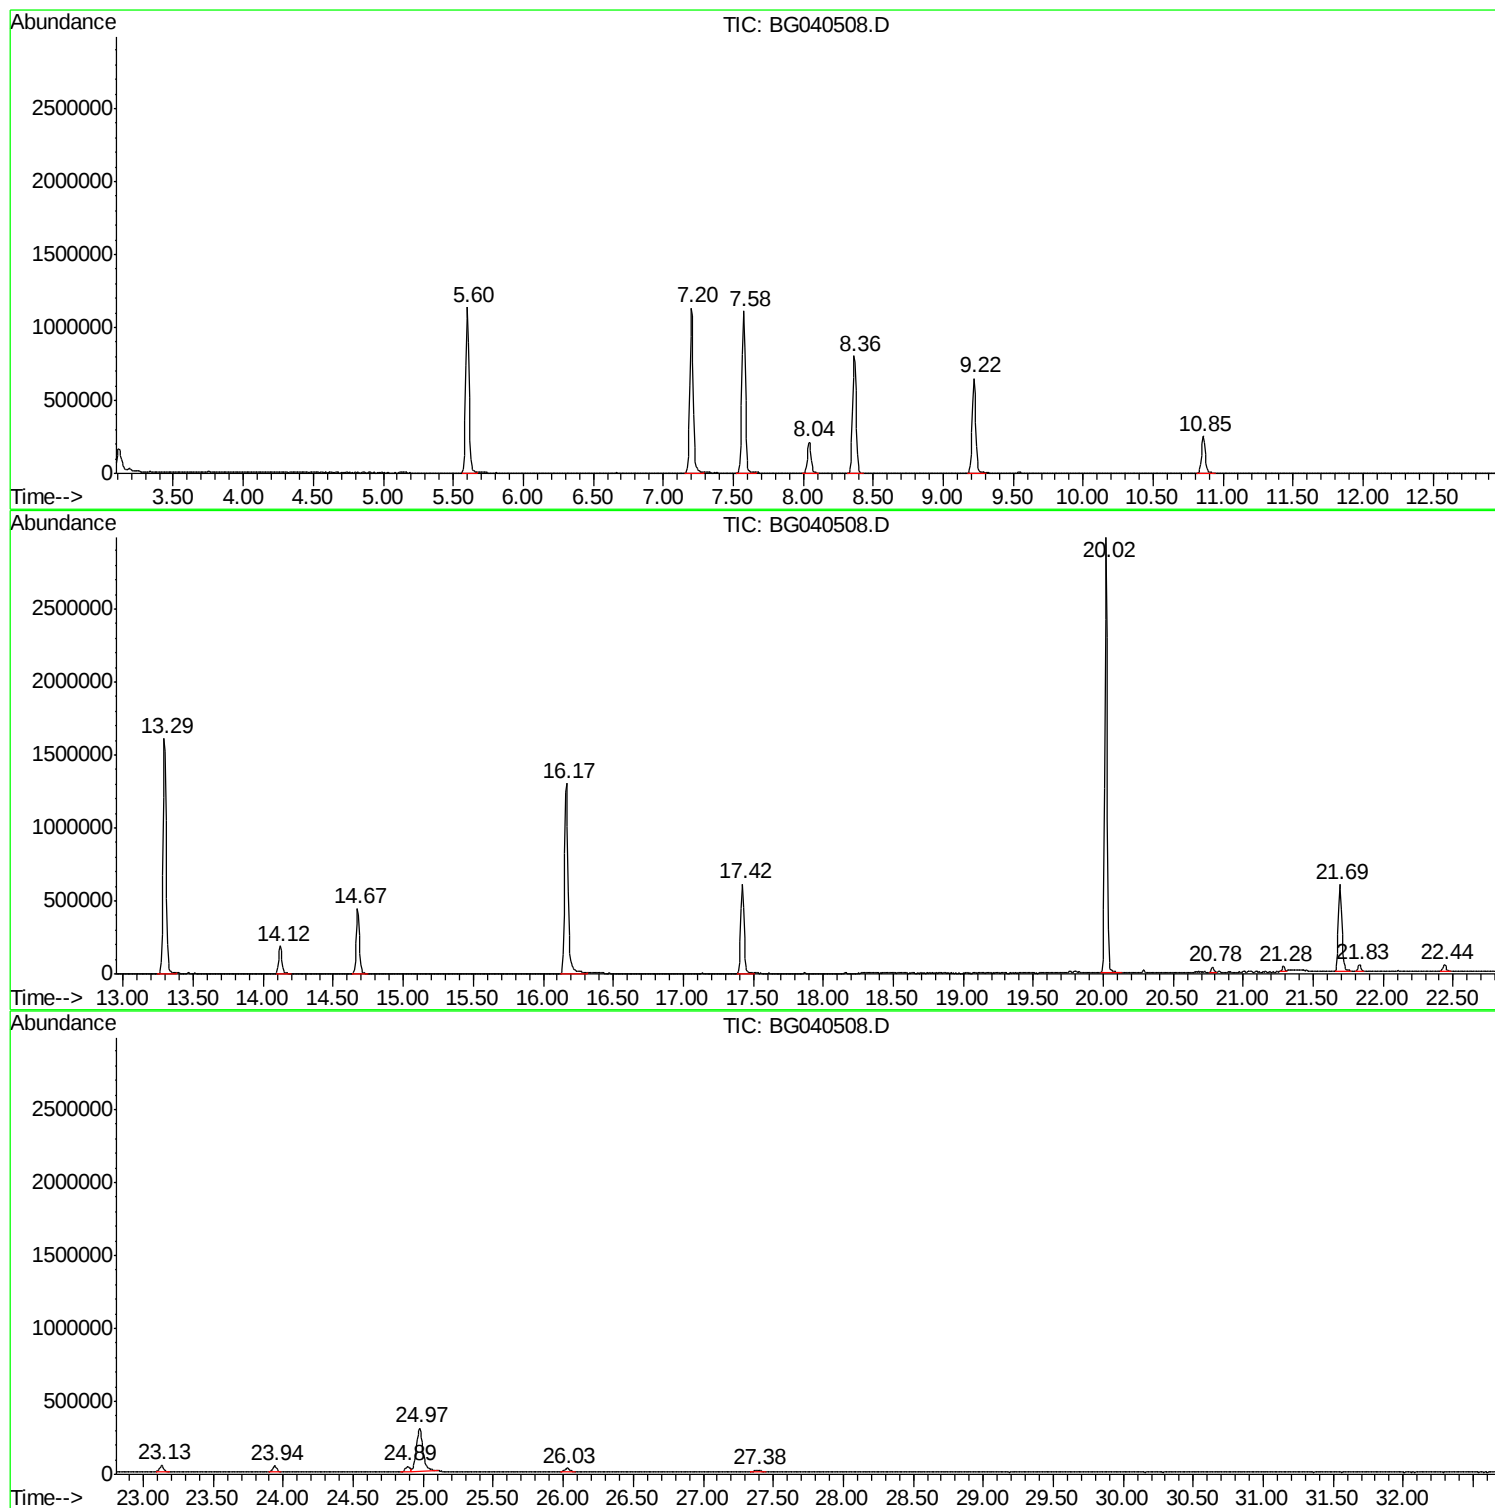

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041619\
Data File : BG040508.D
Acq On : 16 Apr 2019 18:09
Operator : JU/SJ
Sample : K2423-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP1-A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	104.99 ng	1944440	1,4-Dichlorobenzene-d4	8.04

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

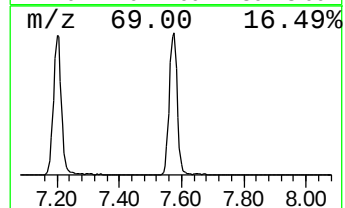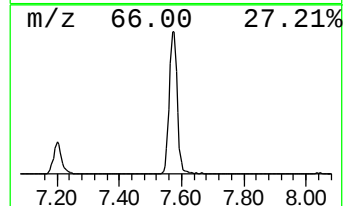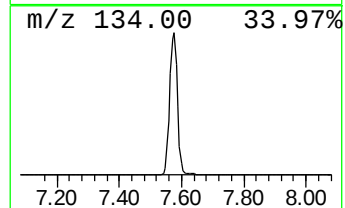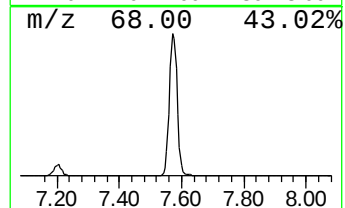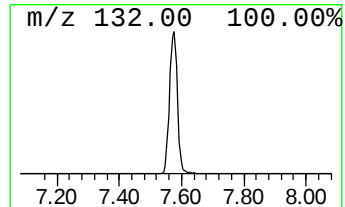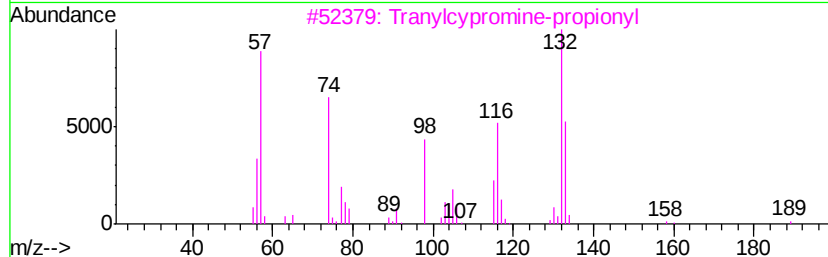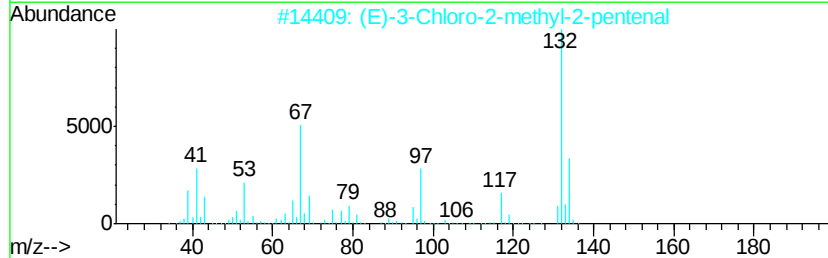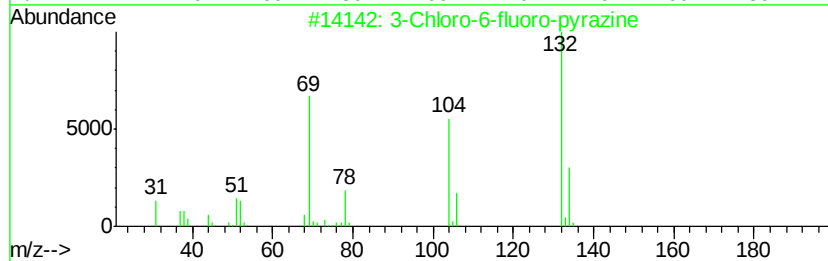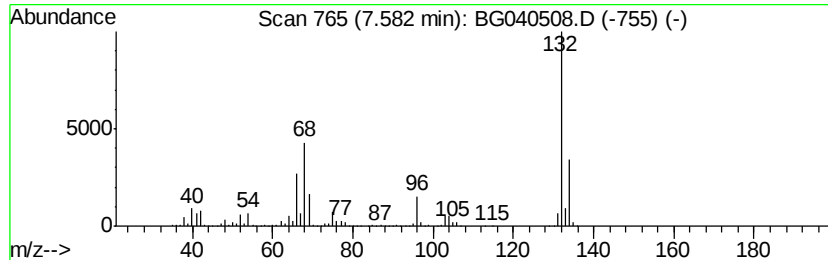

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041619\
Data File : BG040508.D
Acq On : 16 Apr 2019 18:09
Operator : JU/SJ
Sample : K2423-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP1-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.58	7.58	105.0	ng	1944440	1	8.04	370415	20.0