


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041619\
Data File : BG040499.D
Acq On : 16 Apr 2019 11:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Apr 13 00:33:11 2019

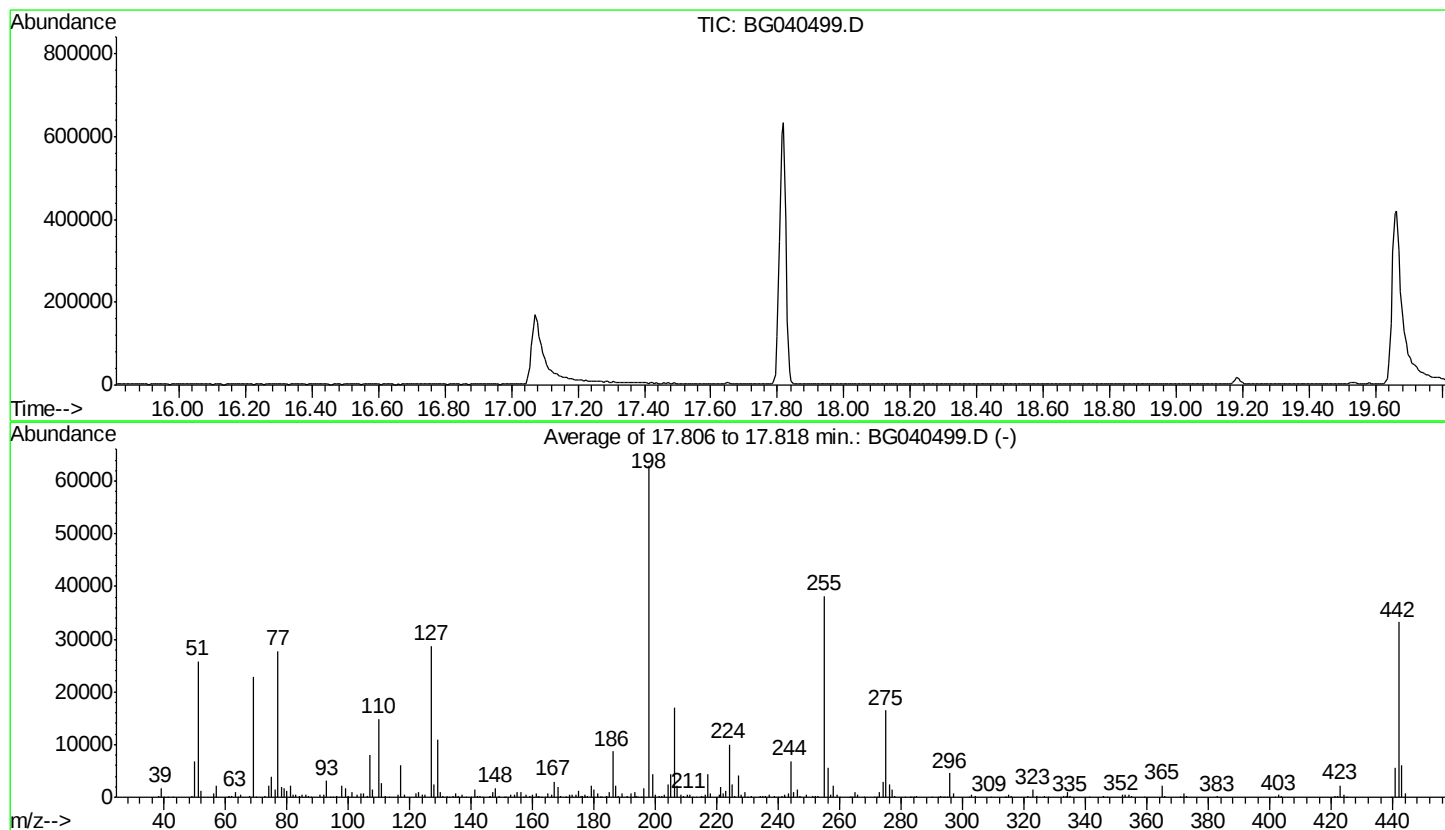

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	25812	PASS
68	69	0.00	2	1.1	254	PASS
69	198	0.00	100	36.2	22805	PASS
70	69	0.00	2	0.6	126	PASS
127	198	10	80	45.7	28760	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62936	PASS
199	198	5	9	7.1	4476	PASS
275	198	10	60	26.2	16466	PASS
365	198	1	100	3.6	2259	PASS
441	198	0.01	100	8.8	5508	PASS
442	198	50	100	52.9	33272	PASS
443	442	15	24	18.5	6166	PASS