

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041620\
 Data File : BG045018.D
 Acq On : 16 Apr 2020 22:50
 Operator : CG/JU
 Sample : L2281-12 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-37-38-45-46

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.593	419	426	433	rBV	218201	372480	31.85%	3.244%
2	7.185	689	697	706	rBV	266227	471018	40.28%	4.102%
3	8.031	834	841	850	rVB	254853	440865	37.70%	3.839%
4	8.260	872	880	885	rBV6	22017	37252	3.19%	0.324%
5	8.354	889	896	903	rBV	233564	412062	35.24%	3.589%
6	8.788	964	970	977	rVB	47183	86231	7.37%	0.751%
7	9.182	1027	1037	1045	rBV	182686	343750	29.40%	2.994%
8	10.838	1311	1319	1324	rBV	374637	687132	58.76%	5.984%
9	10.891	1324	1328	1334	rVB3	44313	82109	7.02%	0.715%
10	12.712	1632	1638	1644	rBV3	18490	39692	3.39%	0.346%
11	13.288	1729	1736	1742	rVB	590552	924539	79.06%	8.052%
12	13.993	1850	1856	1859	rBV5	23194	36950	3.16%	0.322%
13	14.105	1871	1875	1882	rVB	53304	84046	7.19%	0.732%
14	14.663	1963	1970	1977	rBV2	583046	997207	85.28%	8.684%
15	14.733	1977	1982	1987	rVB2	88615	149986	12.83%	1.306%
16	15.062	2034	2038	2044	rBV2	51964	88491	7.57%	0.771%
17	15.708	2145	2148	2155	rVB2	107801	165610	14.16%	1.442%
18	16.149	2218	2223	2232	rBV2	398350	610049	52.17%	5.313%
19	17.412	2433	2438	2441	rBV	593074	956637	81.81%	8.331%
20	17.453	2441	2445	2451	rVB	721952	1112386	95.13%	9.687%
21	17.541	2457	2460	2465	rVB	203543	270923	23.17%	2.359%
22	19.456	2783	2786	2793	rVB	818079	1169376	100.00%	10.184%
23	19.820	2845	2848	2854	rVB	716683	1046896	89.53%	9.117%
24	20.014	2879	2881	2885	rVB	822398	897065	76.71%	7.812%


Sum of corrected areas: 11482752

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041620\
Data File : BG045018.D
Acq On : 16 Apr 2020 22:50
Operator : CG/JU
Sample : L2281-12 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-37-38-45-46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

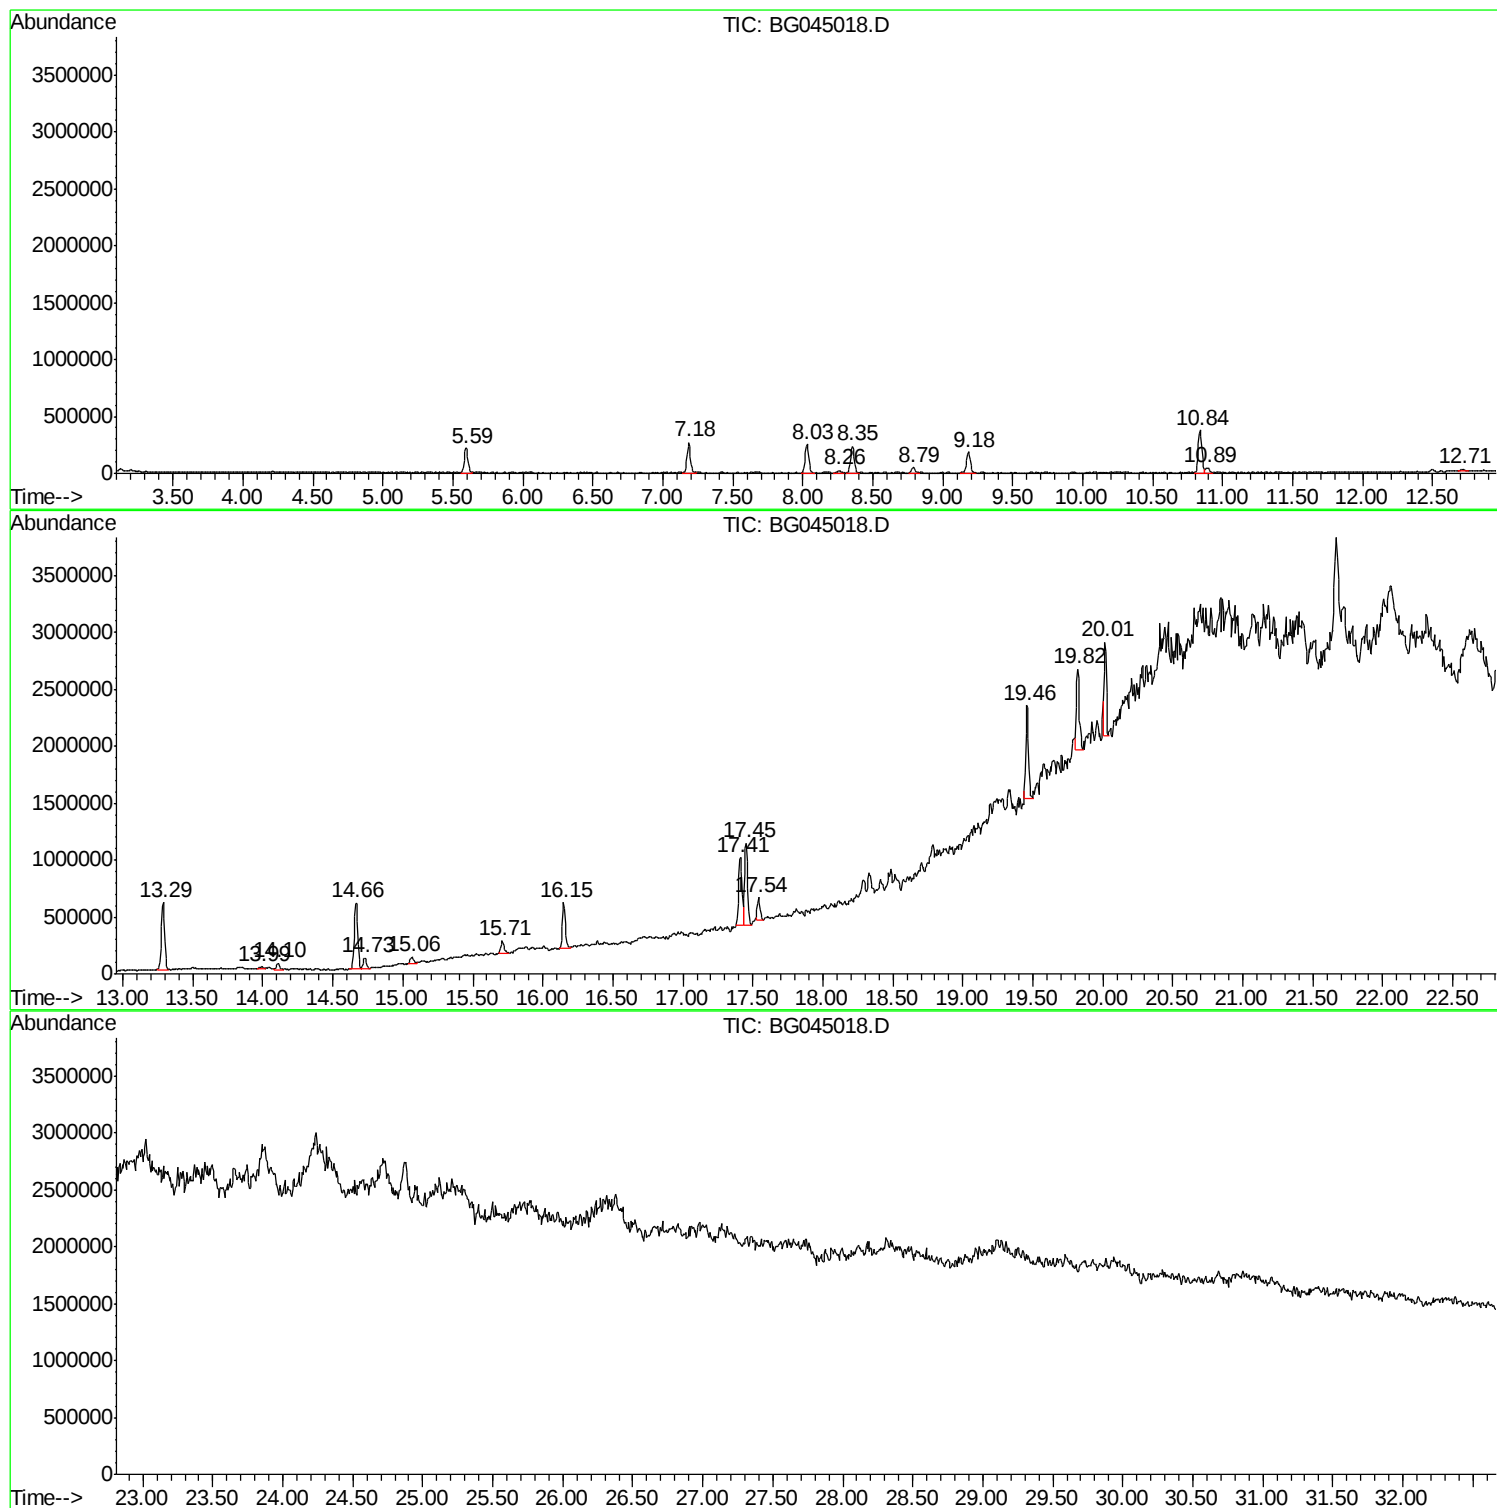

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041620\
Data File : BG045018.D
Acq On : 16 Apr 2020 22:50
Operator : CG/JU
Sample : L2281-12 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-37-38-45-46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041620\
Data File : BG045018.D
Acq On : 16 Apr 2020 22:50
Operator : CG/JU
Sample : L2281-12 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-37-38-45-46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc