

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041620\
 Data File : BG045019.D
 Acq On : 16 Apr 2020 23:29
 Operator : CG/JU
 Sample : L2281-09 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-35-36-43-44

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	14	rVB4	22396	36705	3.53%	0.417%
2	5.590	420	426	434	rVB	192765	324216	31.21%	3.682%
3	7.182	690	697	707	rVB	236057	411813	39.65%	4.677%
4	8.027	832	841	850	rBV	246098	431904	41.58%	4.905%
5	8.351	888	896	903	rBV	195706	351279	33.82%	3.990%
6	9.179	1030	1037	1048	rVB	150456	286274	27.56%	3.251%
7	10.835	1307	1319	1332	rBV	360783	706126	67.98%	8.020%
8	13.279	1729	1735	1744	rVB	529091	835635	80.45%	9.491%
9	14.108	1871	1876	1881	rBV	50299	78070	7.52%	0.887%
10	14.660	1963	1970	1977	rBV	638042	1033742	99.52%	11.741%
11	14.718	1977	1980	1985	rVB	19915	32324	3.11%	0.367%
12	15.053	2034	2037	2044	rVB4	14158	24899	2.40%	0.283%
13	15.705	2142	2148	2153	rBV2	30390	52262	5.03%	0.594%
14	16.146	2216	2223	2231	rBV	373835	616383	59.34%	7.000%
15	17.403	2432	2437	2441	rBV	678034	1038742	100.00%	11.797%
16	17.444	2441	2444	2451	rVB	244026	348923	33.59%	3.963%
17	17.532	2457	2459	2466	rVB	61946	90678	8.73%	1.030%
18	19.453	2781	2786	2790	rBV	496188	773405	74.46%	8.784%
19	19.812	2844	2847	2853	rVB	373104	510366	49.13%	5.796%
20	20.011	2878	2881	2888	rVB	674110	821121	79.05%	9.326%


Sum of corrected areas: 8804867

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041620\
Data File : BG045019.D
Acq On : 16 Apr 2020 23:29
Operator : CG/JU
Sample : L2281-09 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-35-36-43-44

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

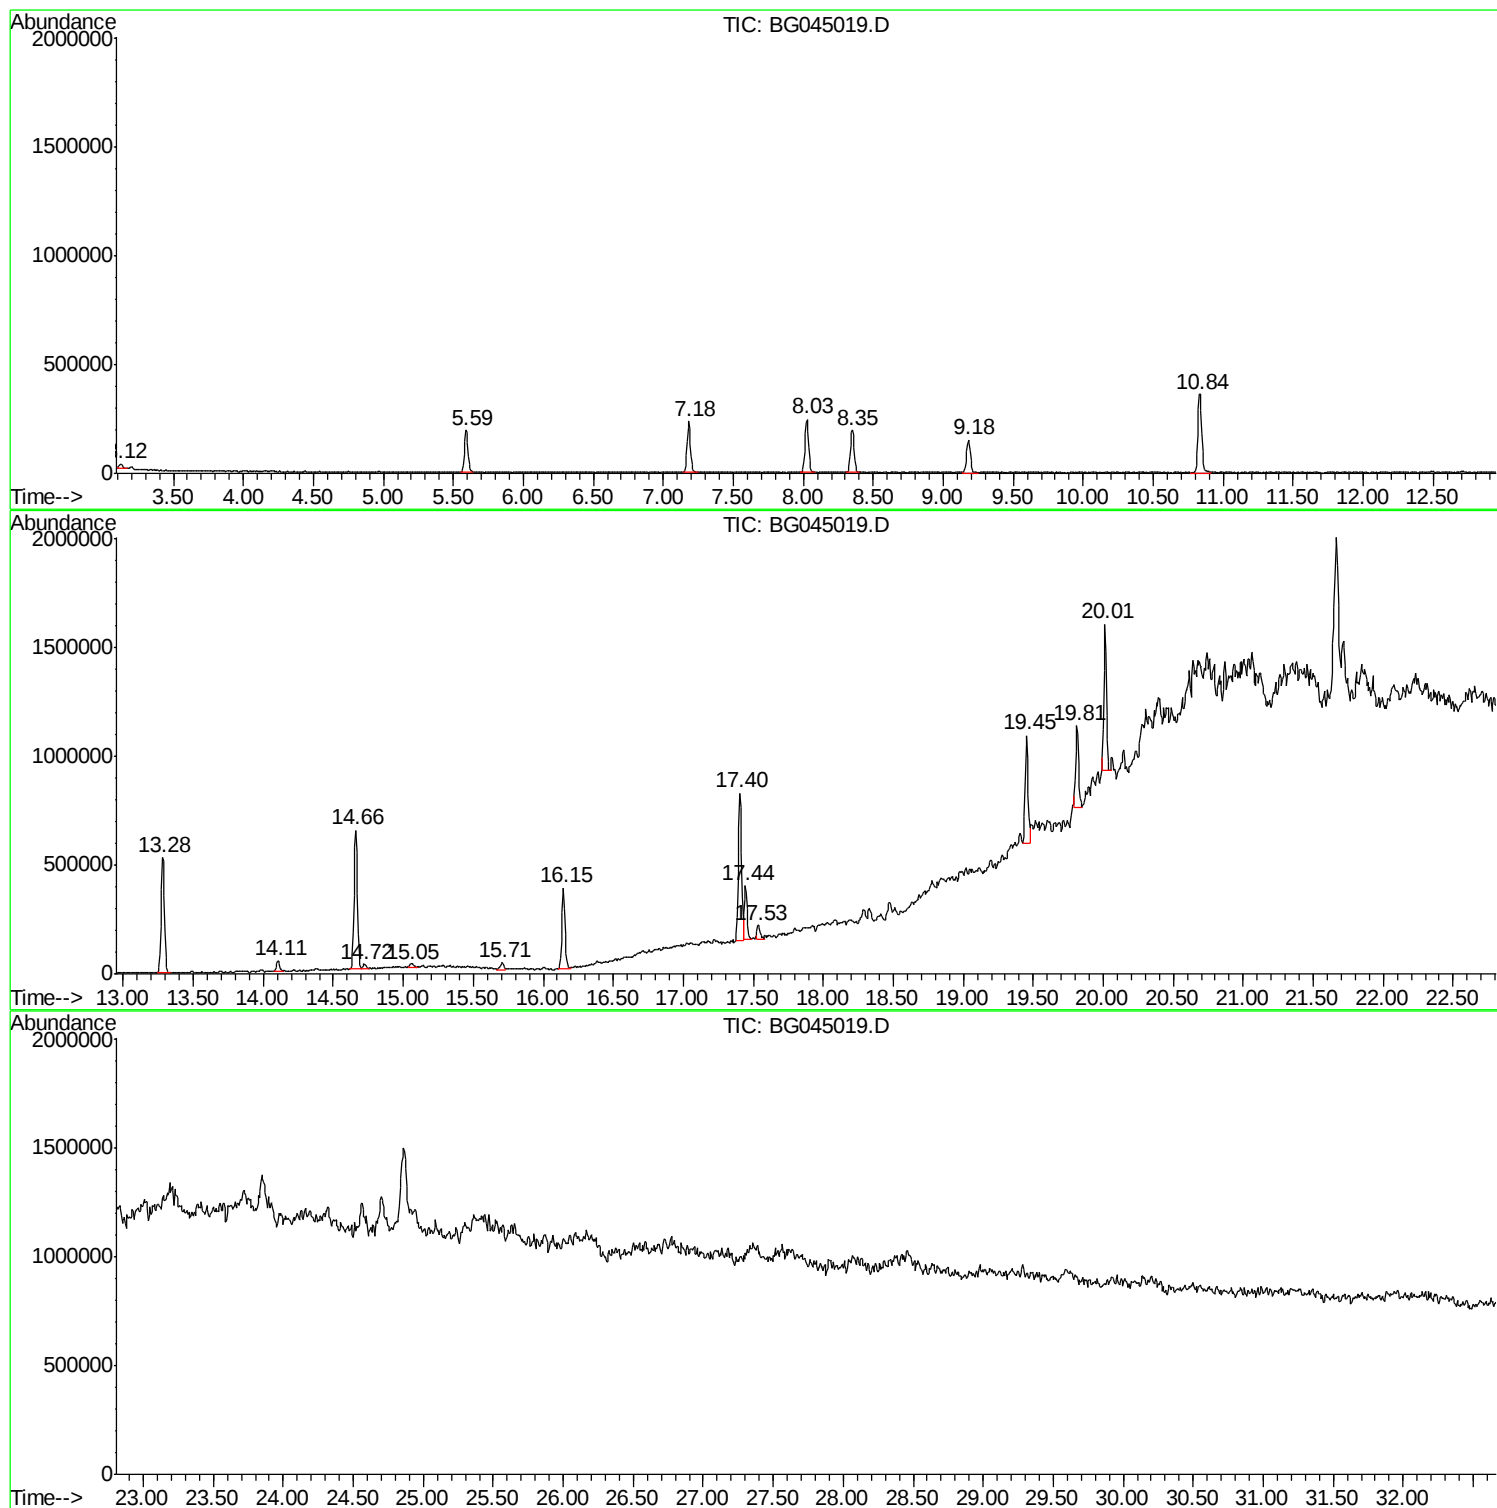

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041620\
Data File : BG045019.D
Acq On : 16 Apr 2020 23:29
Operator : CG/JU
Sample : L2281-09 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-35-36-43-44

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041620\
Data File : BG045019.D
Acq On : 16 Apr 2020 23:29
Operator : CG/JU
Sample : L2281-09 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-35-36-43-44

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc