

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041620\
 Data File : BG045023.D
 Acq On : 17 Apr 2020 2:08
 Operator : CG/JU
 Sample : L2284-18 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-16-B-SA

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	13	rVB5	20418	36503	2.86%	0.405%
2	5.590	419	426	434	rBV2	139085	232995	18.24%	2.586%
3	7.182	688	697	705	rBV	160595	296669	23.23%	3.292%
4	8.022	831	840	851	rBV	271281	464054	36.33%	5.150%
5	8.346	889	895	904	rVB	147138	258513	20.24%	2.869%
6	9.174	1029	1036	1044	rBV	110167	205007	16.05%	2.275%
7	10.830	1309	1318	1326	rBV	390121	718552	56.25%	7.974%
8	13.280	1727	1735	1742	rBV	392551	607461	47.56%	6.741%
9	14.102	1870	1875	1881	rVB2	33276	53307	4.17%	0.592%
10	14.655	1961	1969	1977	rBV	696939	1133945	88.77%	12.583%
11	16.141	2214	2222	2229	rBV2	260816	434367	34.01%	4.820%
12	17.398	2430	2436	2442	rBV	806306	1277331	100.00%	14.174%
13	17.439	2442	2443	2448	rVB	50350	51255	4.01%	0.569%
14	17.533	2456	2459	2465	rVB2	10636	15110	1.18%	0.168%
15	18.291	2583	2588	2591	rBV7	10185	18368	1.44%	0.204%
16	18.473	2614	2619	2623	rBV8	15957	29577	2.32%	0.328%
17	18.773	2667	2670	2674	rBV6	12175	17225	1.35%	0.191%
18	19.448	2781	2785	2792	rBV	80123	128947	10.10%	1.431%
19	19.807	2842	2846	2853	rVB	67069	103990	8.14%	1.154%
20	20.012	2876	2881	2886	rVB	555907	759792	59.48%	8.431%
21	21.663	3156	3162	3168	rBV	683664	1144594	89.61%	12.701%
22	24.853	3697	3705	3714	rBV2	381817	1024016	80.17%	11.363%


Sum of corrected areas: 9011578

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041620\
Data File : BG045023.D
Acq On : 17 Apr 2020 2:08
Operator : CG/JU
Sample : L2284-18 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-16-B-SA

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

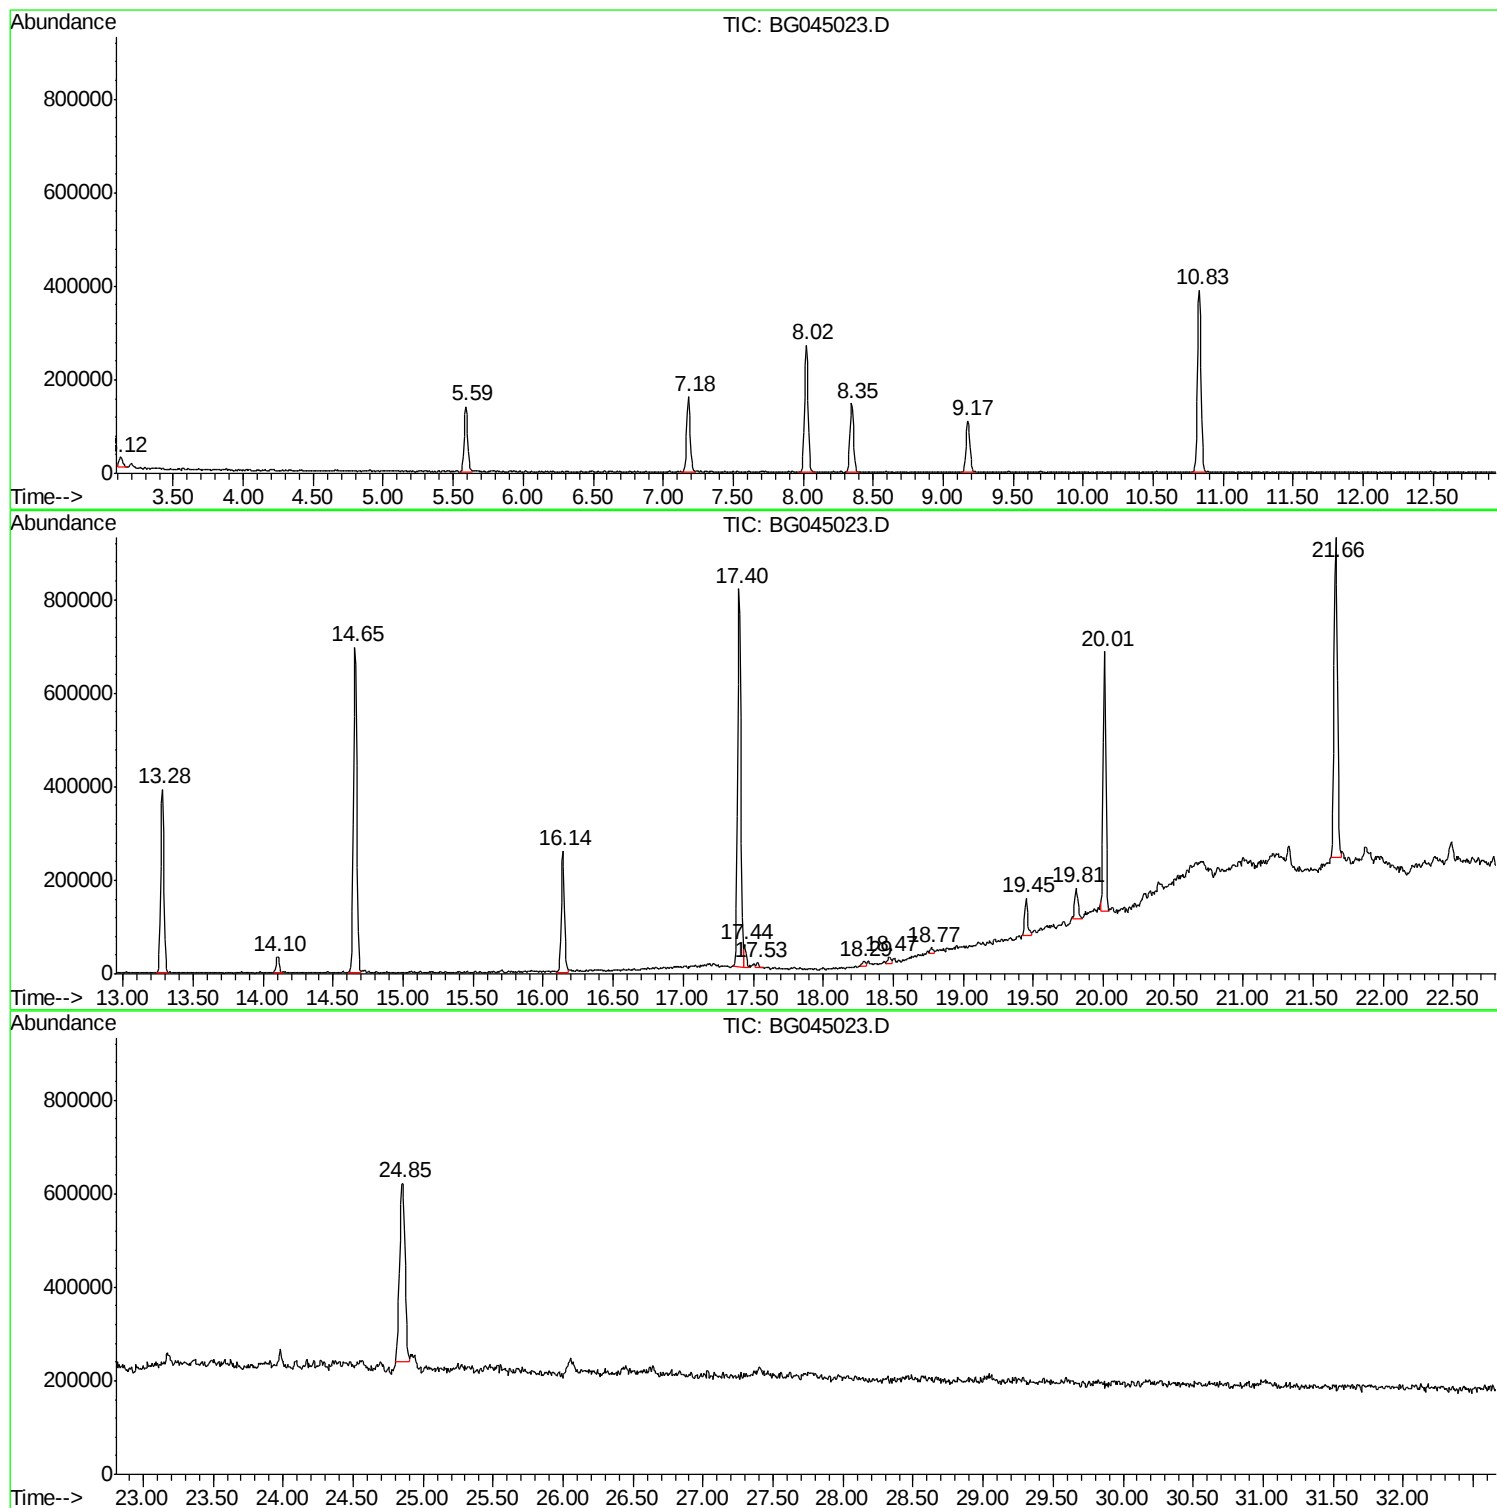

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041620\
Data File : BG045023.D
Acq On : 17 Apr 2020 2:08
Operator : CG/JU
Sample : L2284-18 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-16-B-SA

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041620\
Data File : BG045023.D
Acq On : 17 Apr 2020 2:08
Operator : CG/JU
Sample : L2284-18 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-16-B-SA

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc