


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG041620\
 Data File : BG045006.D
 Acq On : 16 Apr 2020 14:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 11:08:29 2020

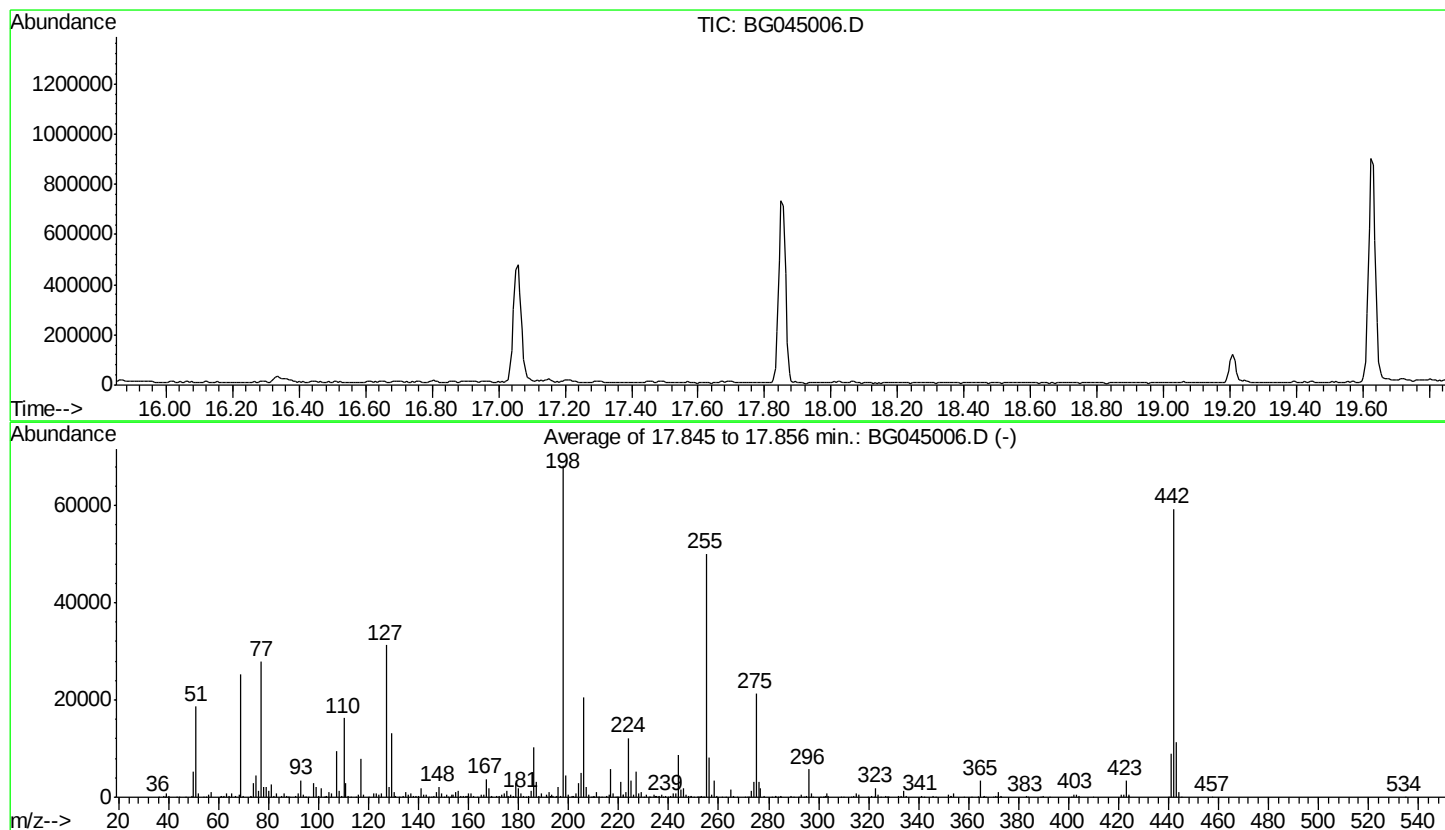

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	18660	PASS
68	69	0.00	2	1.6	416	PASS
69	198	0.00	100	37.1	25316	PASS
70	69	0.00	2	1.0	243	PASS
127	198	10	80	45.8	31253	PASS
197	198	0.00	2	0.4	248	PASS
198	198	100	100	100.0	68178	PASS
199	198	5	9	6.8	4609	PASS
275	198	10	60	31.2	21300	PASS
365	198	1	100	4.9	3307	PASS
441	198	0.01	100	13.2	8998	PASS
442	198	50	100	86.9	59280	PASS
443	442	15	24	19.3	11454	PASS