
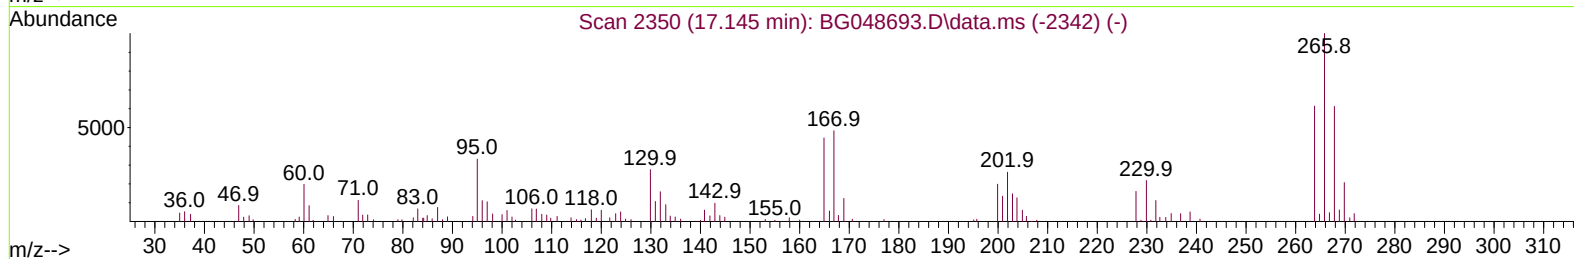
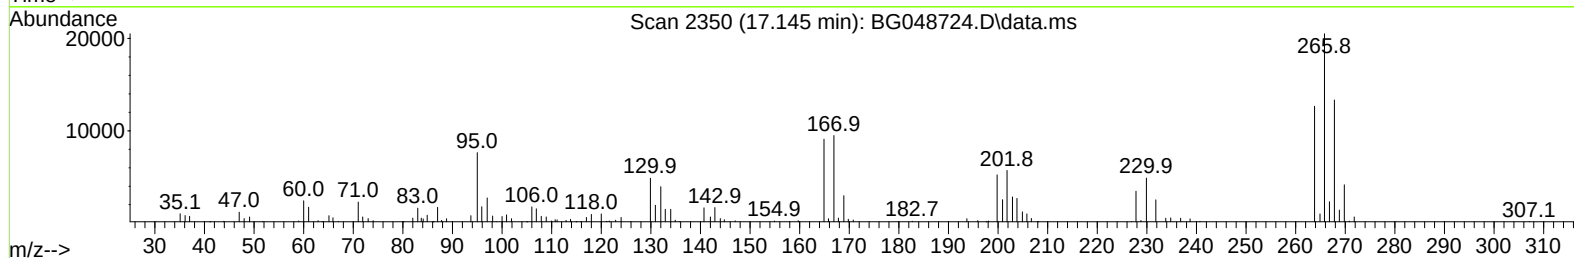


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
Data File : BG048724.D
Acq On : 16 Apr 2021 14:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 00:43:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 15:59:00 2021
Response via : Initial Calibration

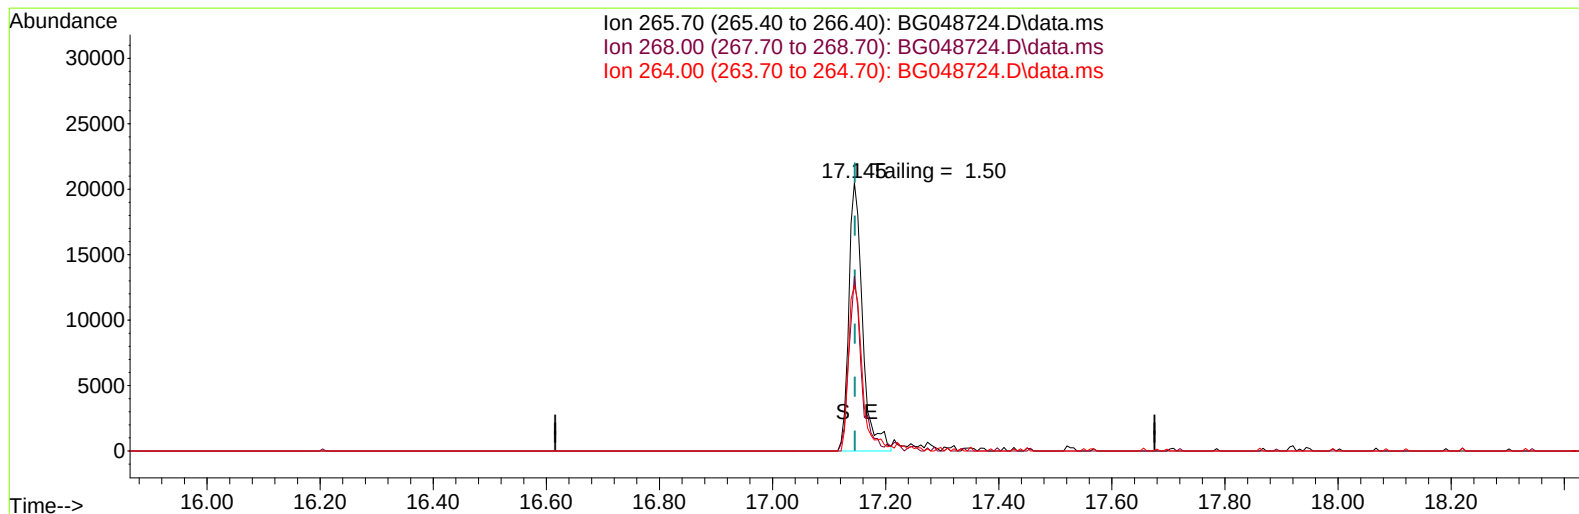

TIC: BG048724.D\data.ms

(70) Pentachlorophenol (C)




17.145min (-0.001) 21655.15 ng

response 34708

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.02
264.00	61.30	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
 Data File : BG048724.D
 Acq On : 16 Apr 2021 14:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 00:43:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 15:59:00 2021
 Response via : Initial Calibration

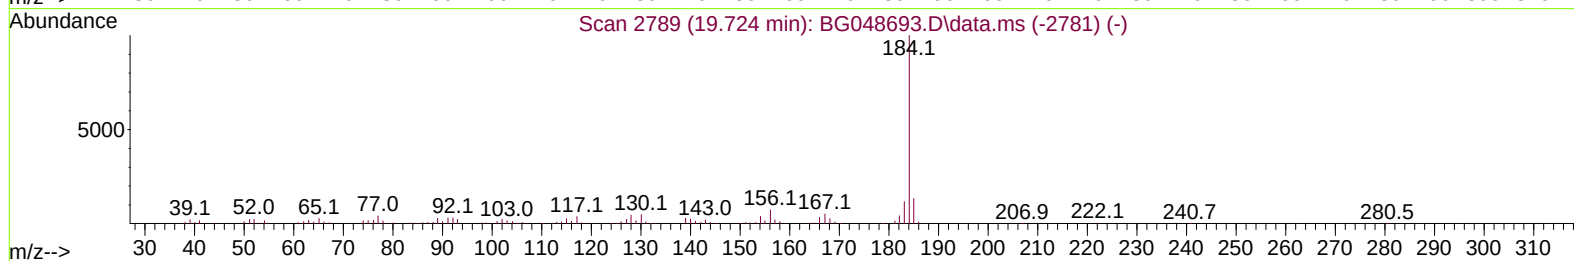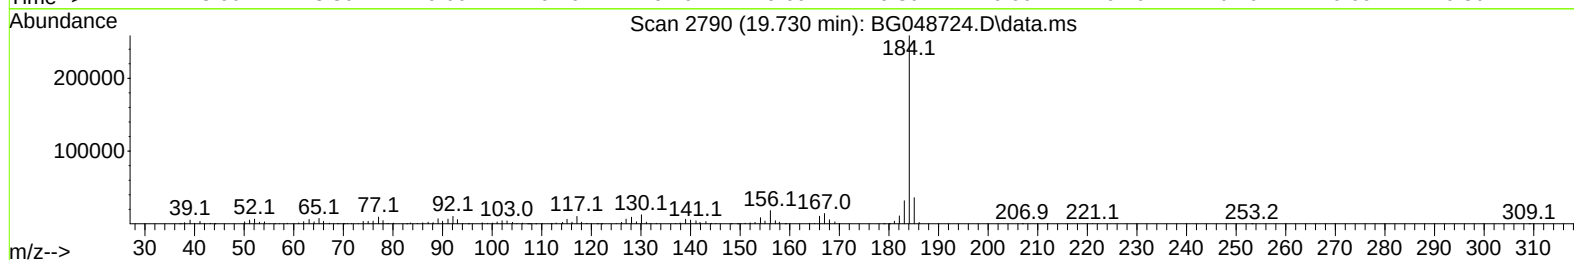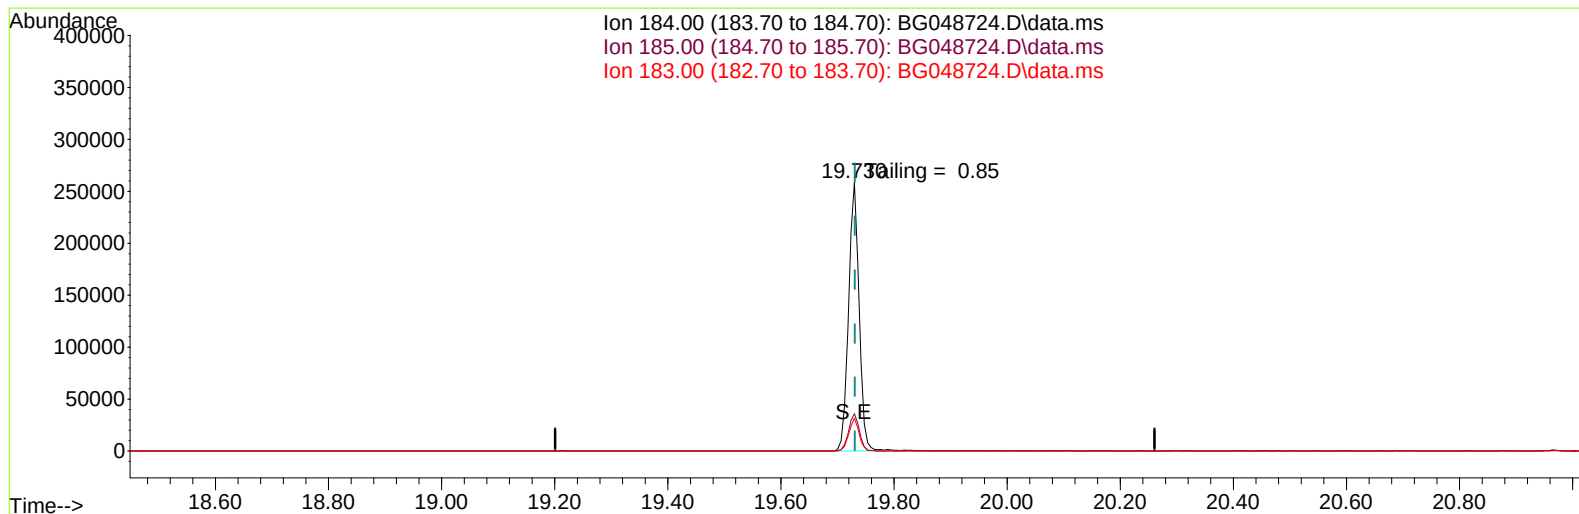

TIC: BG048724.D\data.ms

(77) Benzidine

19.730min (-0.001) 232087.67 ng

response 334040

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.90
183.00	11.70	12.32
0.00	0.00	0.00