
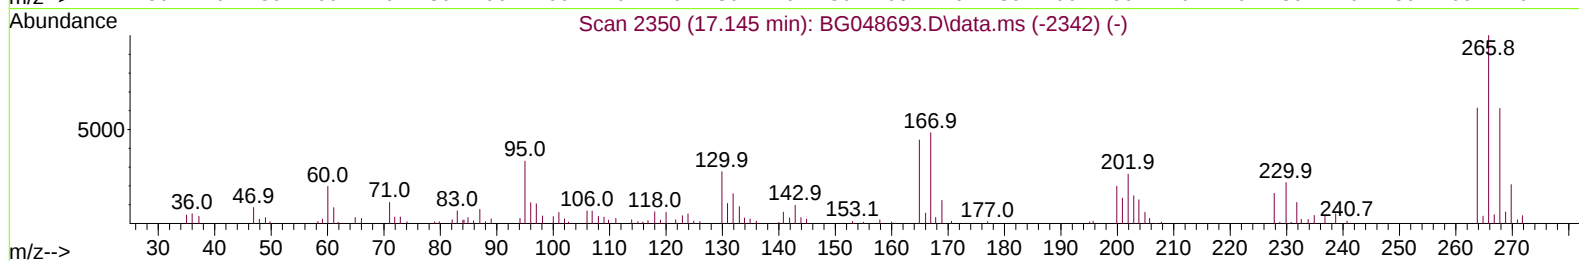
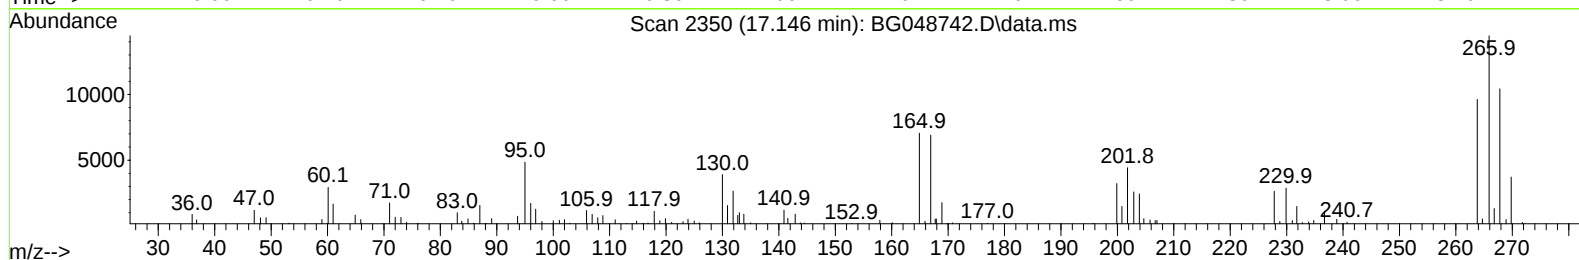


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\  
Data File : BG048742.D  
Acq On    : 17 Apr 2021    4:54  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 17 05:37:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 15:59:00 2021
Response via : Initial Calibration

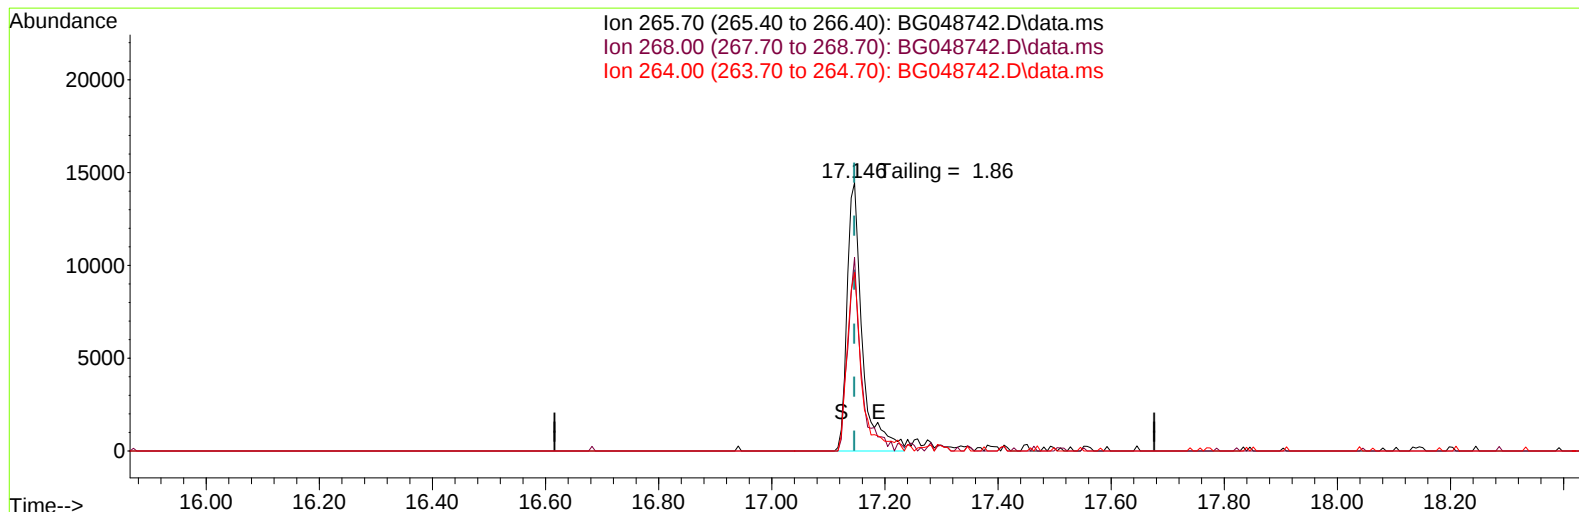

TIC: BG048742.D\data.ms

(70) Pentachlorophenol (C)




17.146min (+ 0.000) 12724.32 ng

response **27113**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	72.06
264.00	61.30	70.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
Data File : BG048742.D
Acq On : 17 Apr 2021 4:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:37:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 15:59:00 2021
Response via : Initial Calibration

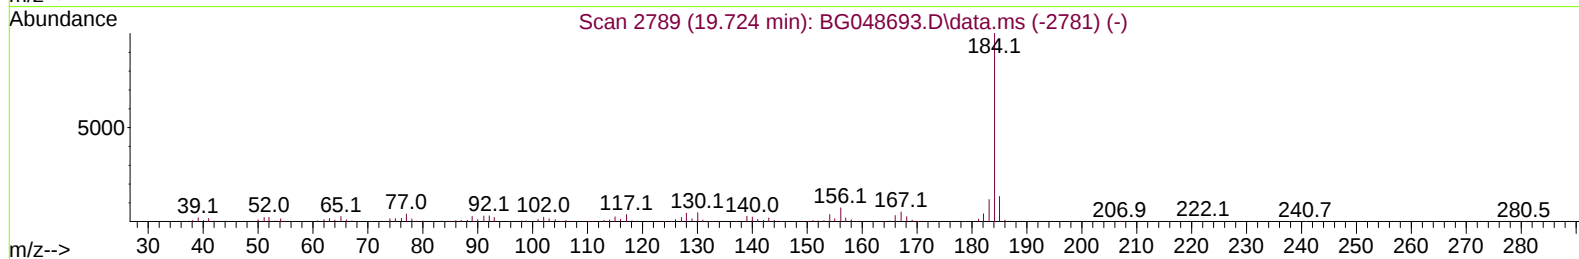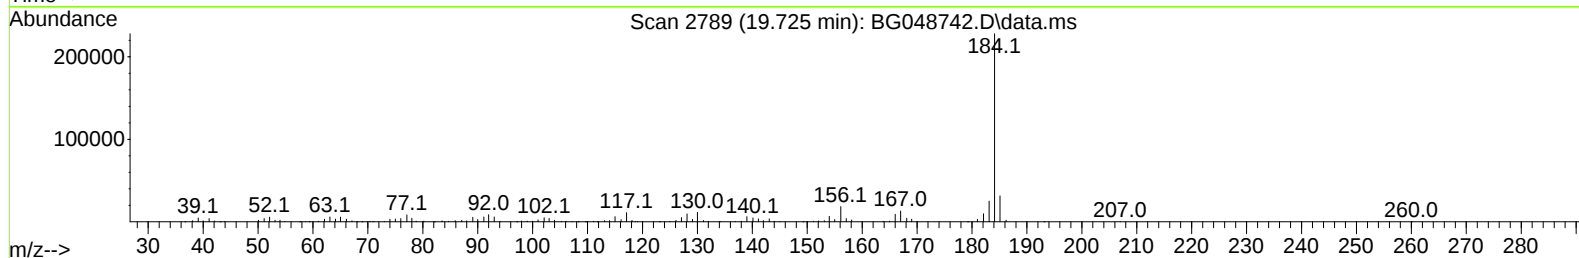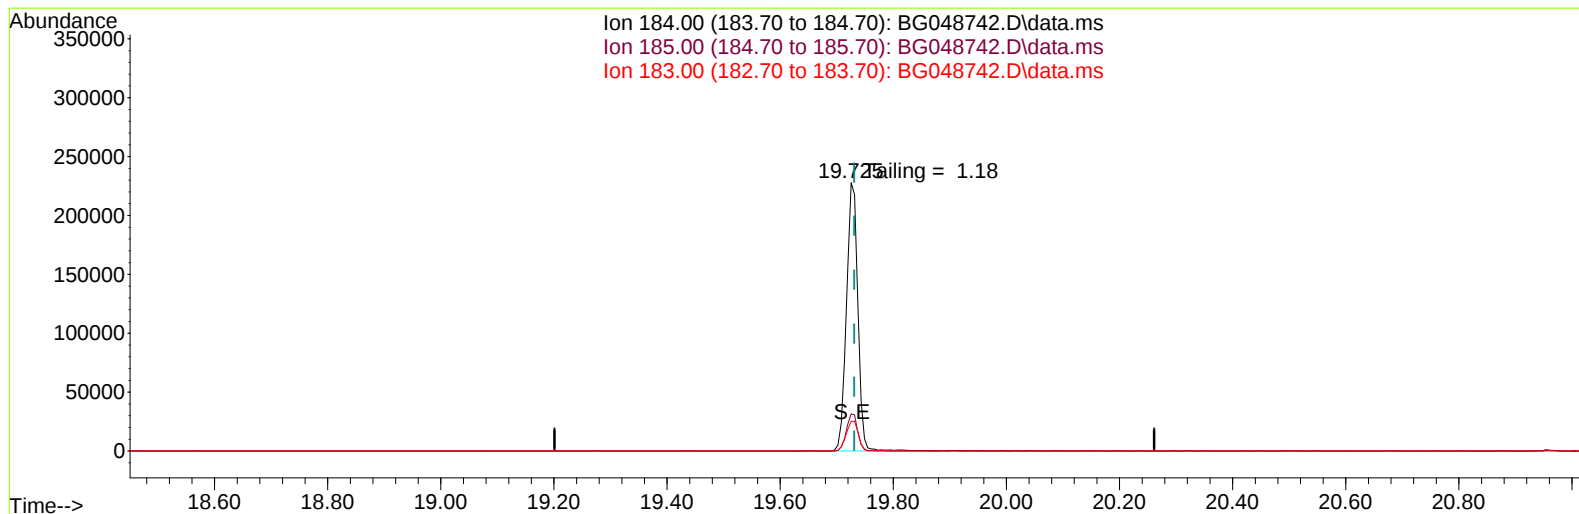

TIC: BG048742.D\data.ms

(77) Benzidine**19.725min (-0.006) 216479.37 ng****response 317454**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.85
183.00	11.70	11.06
0.00	0.00	0.00