
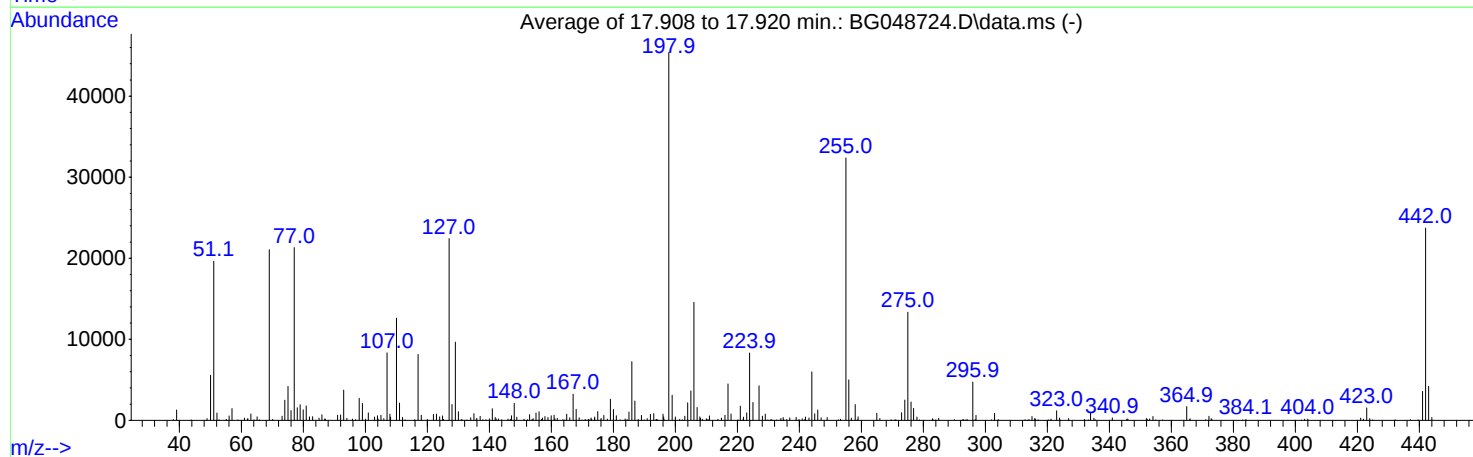


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
 Data File : BG048724.D
 Acq On : 16 Apr 2021 14:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 15:59:00 2021

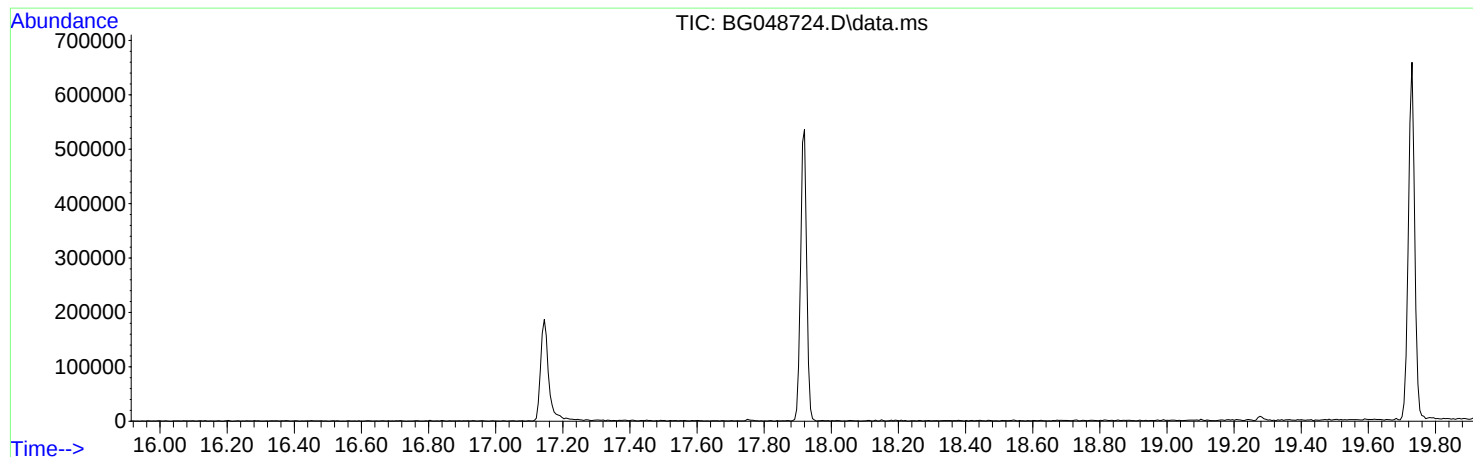




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	19633	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.4	21074	PASS
70	69	0.00	2	0.6	119	PASS
127	198	10	80	49.4	22427	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45387	PASS
199	198	5	9	6.8	3096	PASS
275	198	10	60	29.4	13339	PASS
365	198	1	100	3.7	1702	PASS
441	198	0.01	100	7.9	3580	PASS
442	198	50	100	52.3	23728	PASS
443	442	15	24	17.6	4178	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
Data File : BG048724.D
Acq On : 16 Apr 2021 14:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 00:43:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 15:59:00 2021
Response via : Initial Calibration

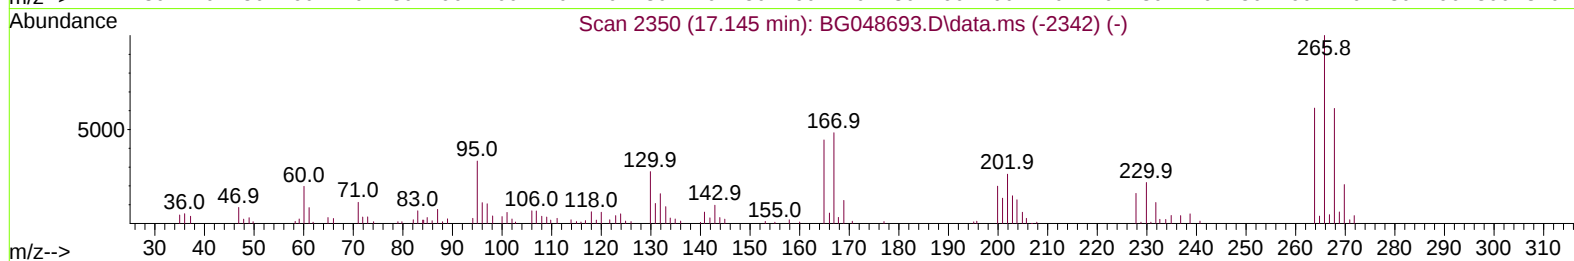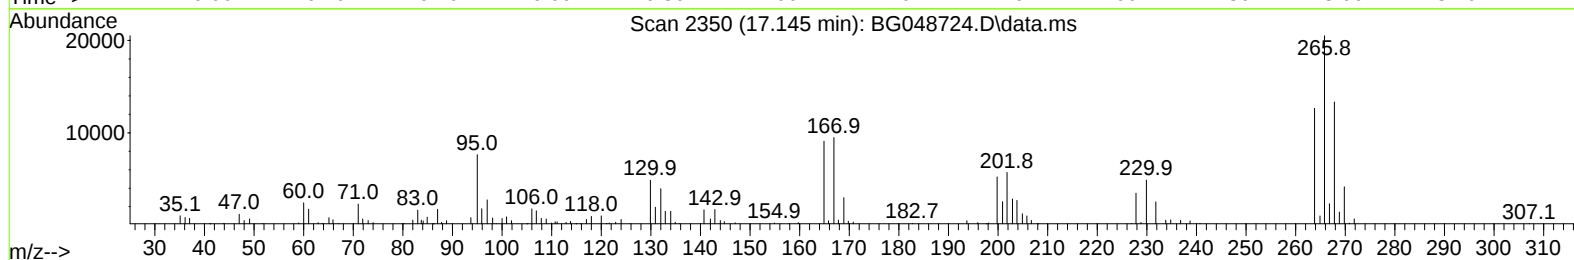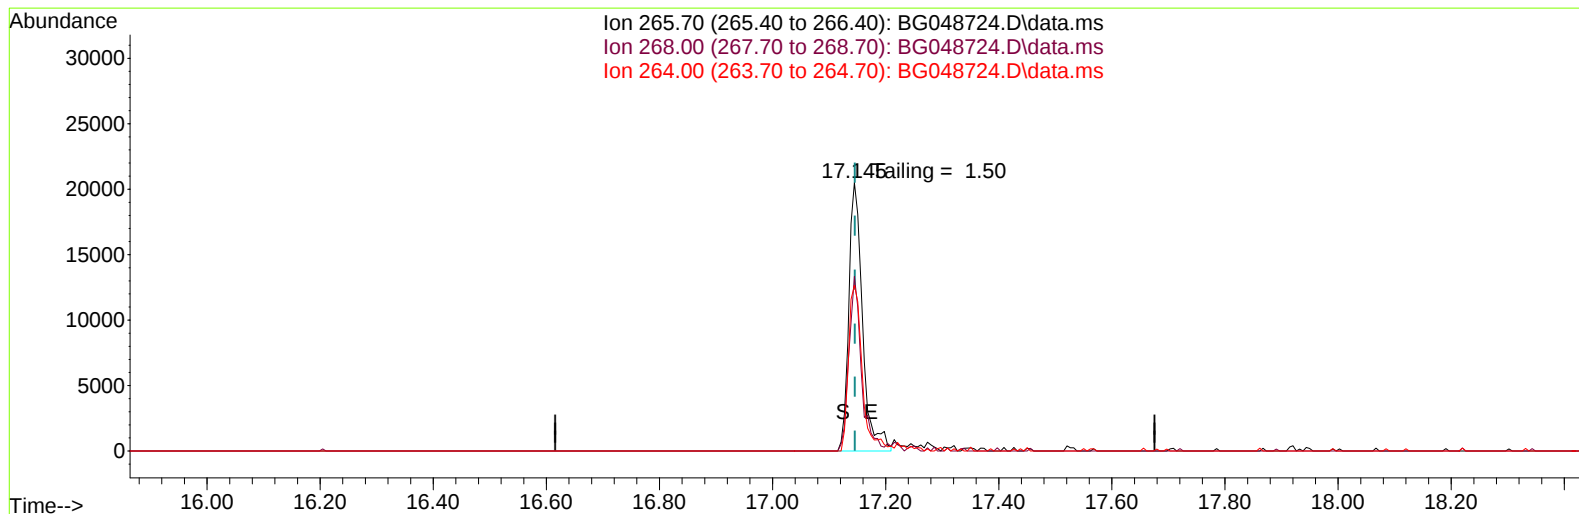

TIC: BG048724.D\data.ms

(70) Pentachlorophenol (C)

17.145min (-0.001) 21655.15 ng




response 34708

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.02
264.00	61.30	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
Data File : BG048724.D
Acq On : 16 Apr 2021 14:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 00:43:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 15:59:00 2021
Response via : Initial Calibration

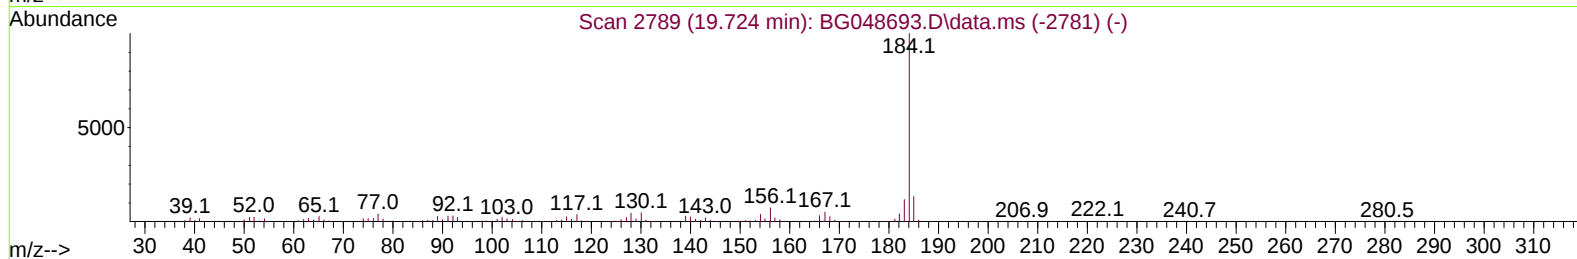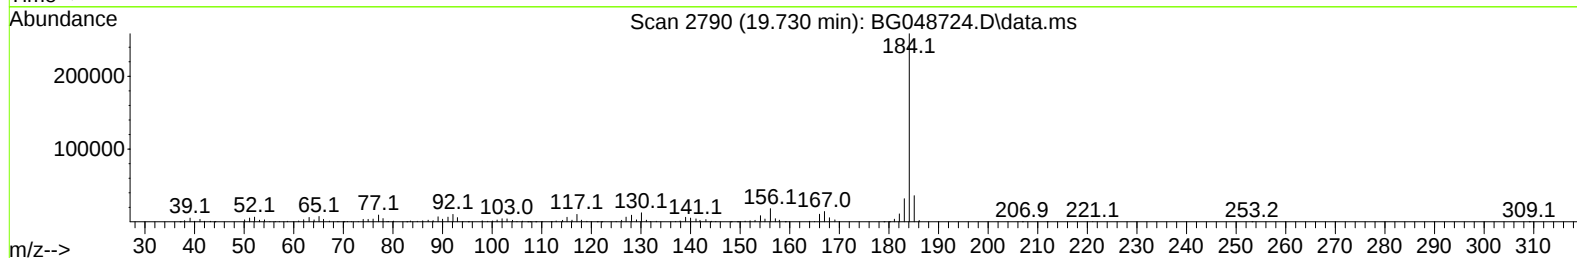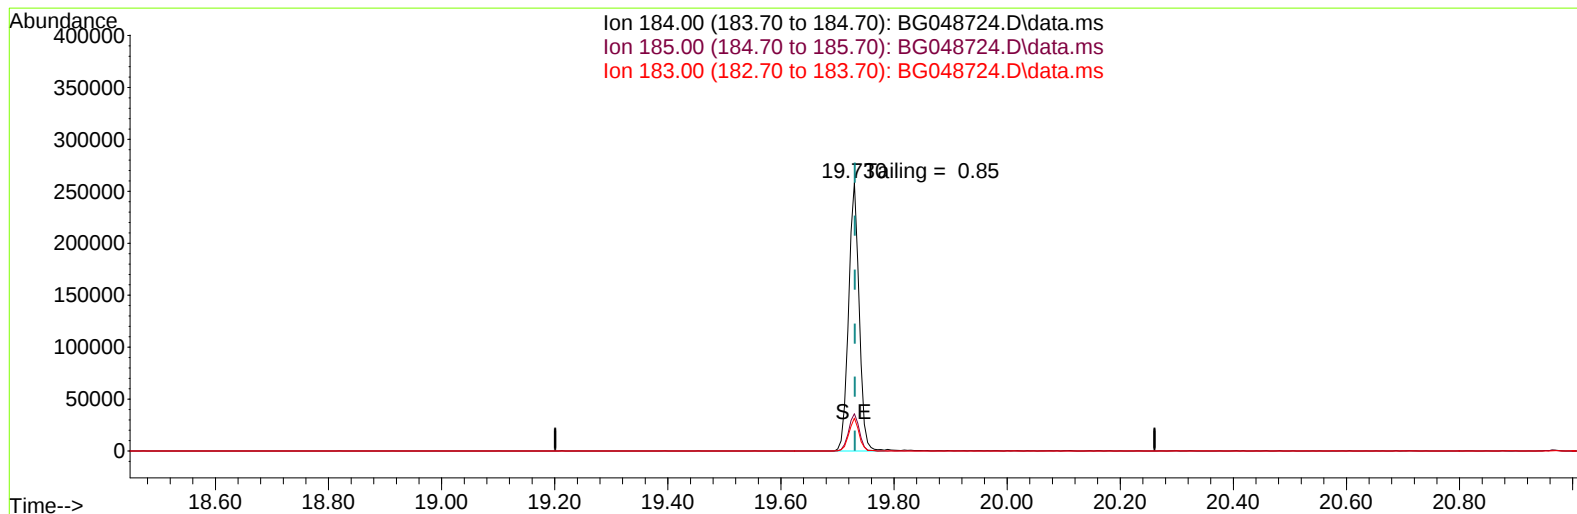

TIC: BG048724.D\data.ms

(77) Benzidine

19.730min (-0.001) 232087.67 ng

response 334040

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.90
183.00	11.70	12.32
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_G
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/16/2021	BNA_G	BG048724.D
Compound Name	Response	Retention Time
DDT	165223	20.964
DDD	7069	20.517
DDE	758	20.012
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7827	173050	4.52

Instrument :
BNA_G
ClientSampleId :
DFTPP