
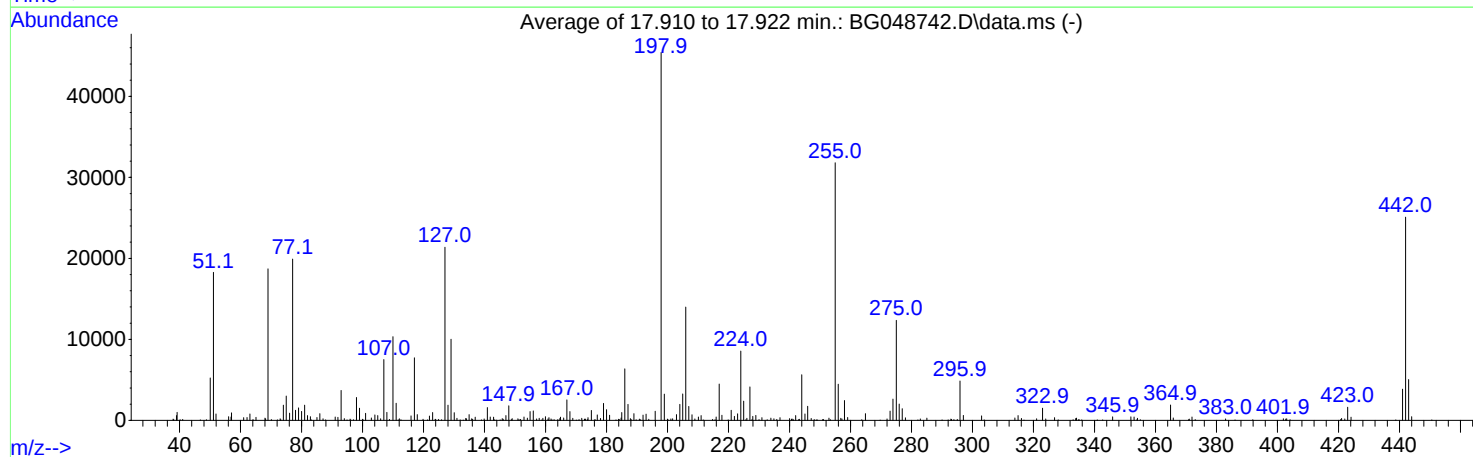


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
 Data File : BG048742.D
 Acq On : 17 Apr 2021 4:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 15:59:00 2021

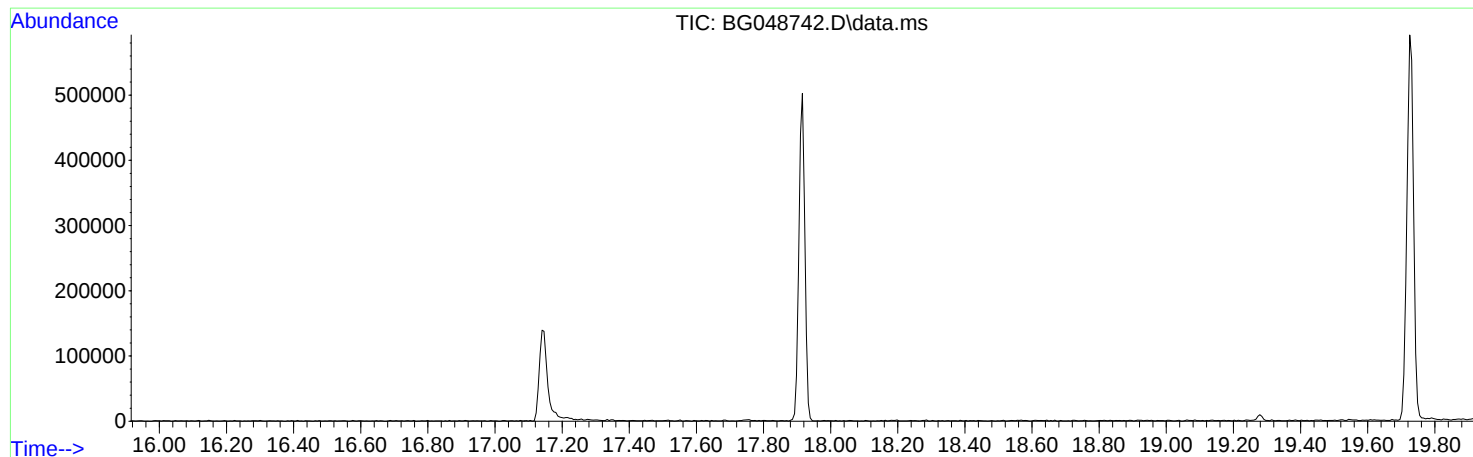




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	18265	PASS
68	69	0.00	2	1.4	270	PASS
69	198	0.00	100	41.2	18712	PASS
70	69	0.00	2	0.5	95	PASS
127	198	10	80	47.1	21376	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45413	PASS
199	198	5	9	7.1	3245	PASS
275	198	10	60	27.2	12357	PASS
365	198	1	100	4.2	1905	PASS
441	198	0.01	100	8.5	3856	PASS
442	198	50	100	55.2	25080	PASS
443	442	15	24	20.1	5033	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041621\
 Data File : BG048742.D
 Acq On : 17 Apr 2021 4:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 17 05:37:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 15:59:00 2021
 Response via : Initial Calibration

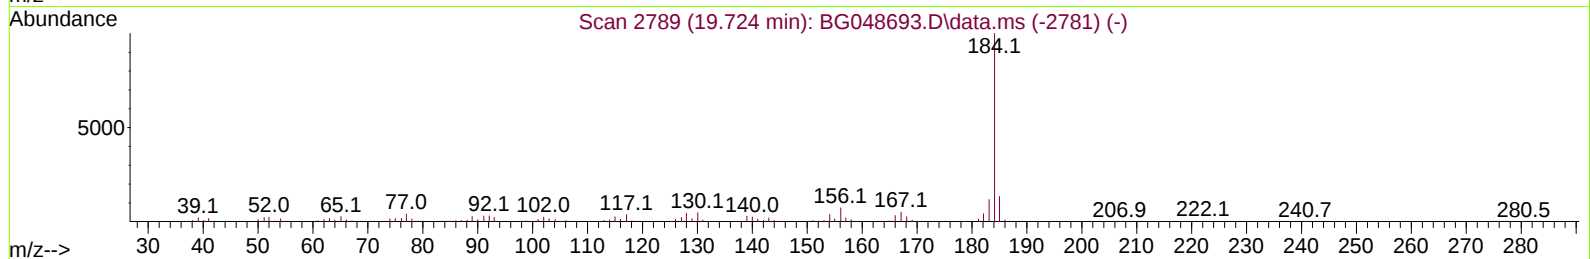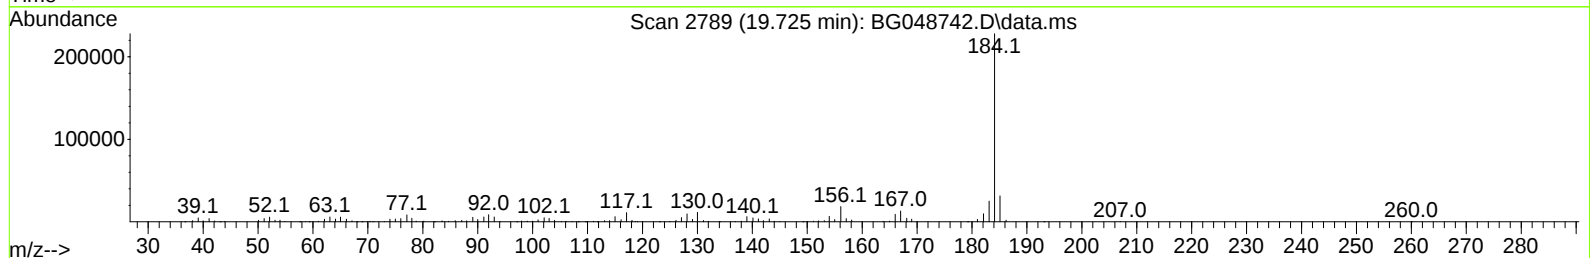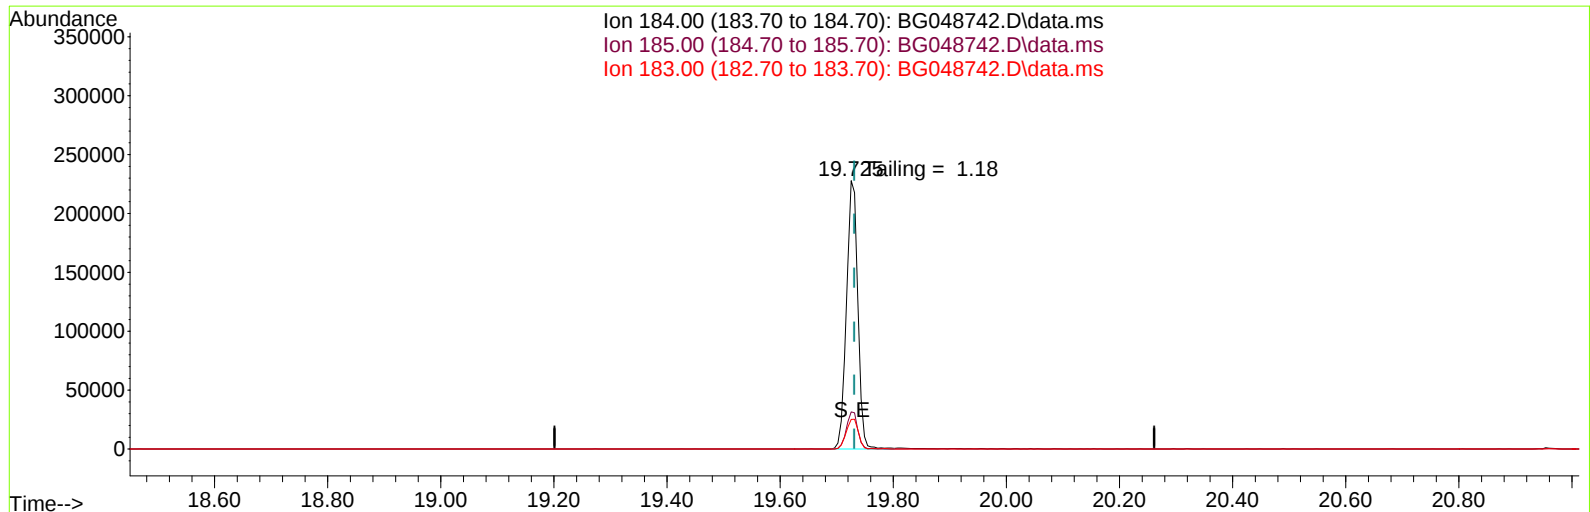

TIC: BG048742.D\data.ms

(77) Benzidine

19.725min (-0.006) 216479.37 ng

response 317454

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.85
183.00	11.70	11.06
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_G
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/16/2021	BNA_G	BG048742.D
Compound Name	Response	Retention Time
DDT	128382	20.959
DDD	23397	20.513
DDE	1054	20.007
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24451	152833	16.00

Instrument :
BNA_G
ClientSampleId :
DFTPP