
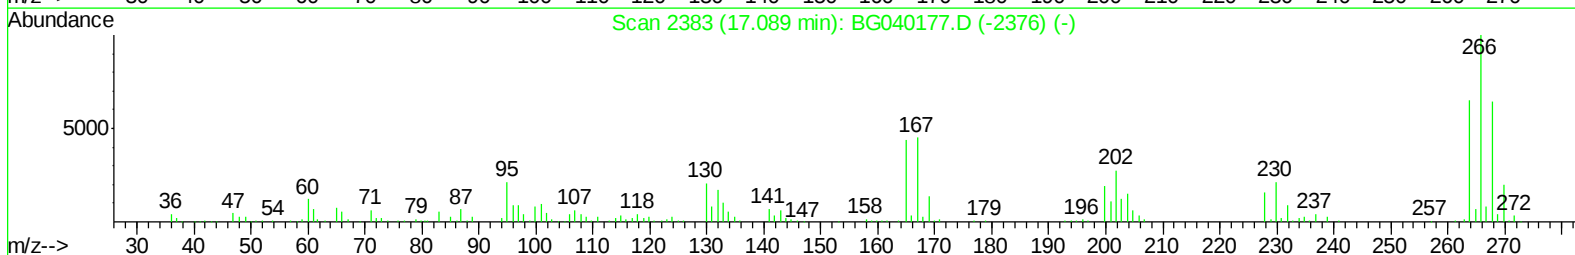
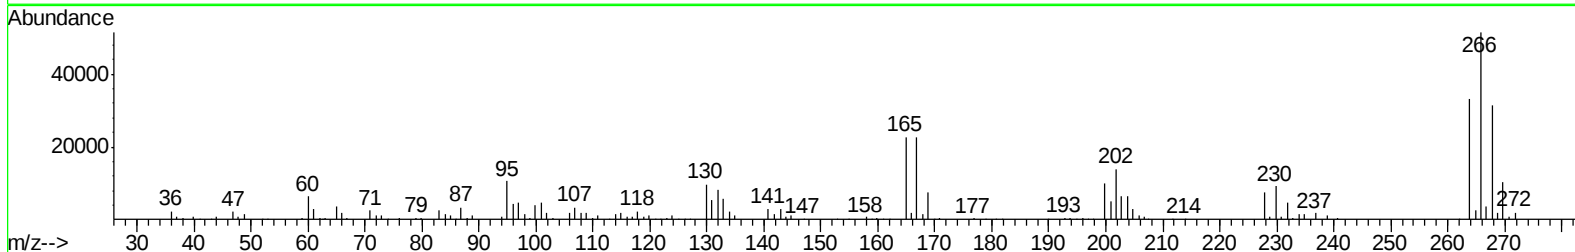


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041719\
Data File : BG040528.D
Acq On : 17 Apr 2019 13:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 05:05:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration

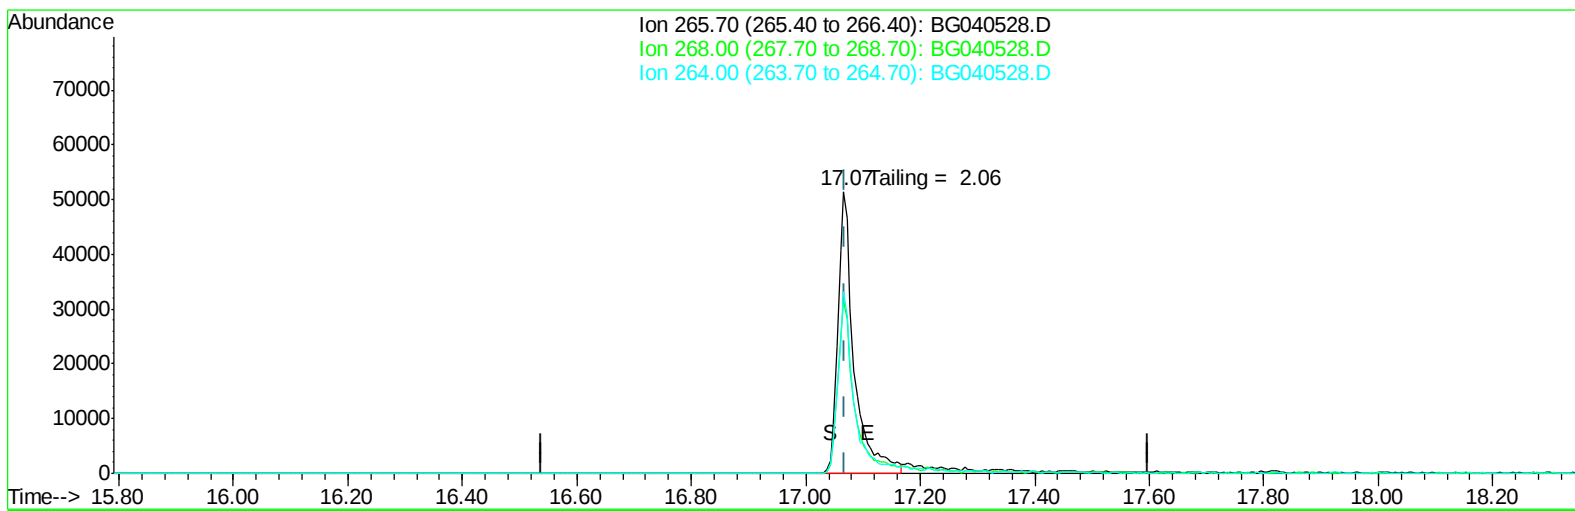

TIC: BG040528.D

(70) Pentachlorophenol (C)




17.066min (-0.003) 25133.37ng m

response 101771

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	61.18
264.00	64.80	64.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041719\
 Data File : BG040528.D
 Acq On : 17 Apr 2019 13:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 05:05:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 13 00:33:11 2019
 Response via : Initial Calibration

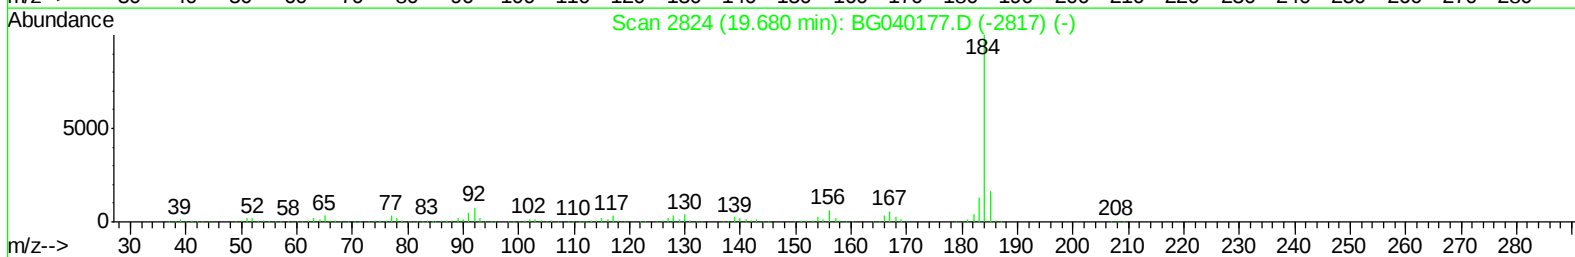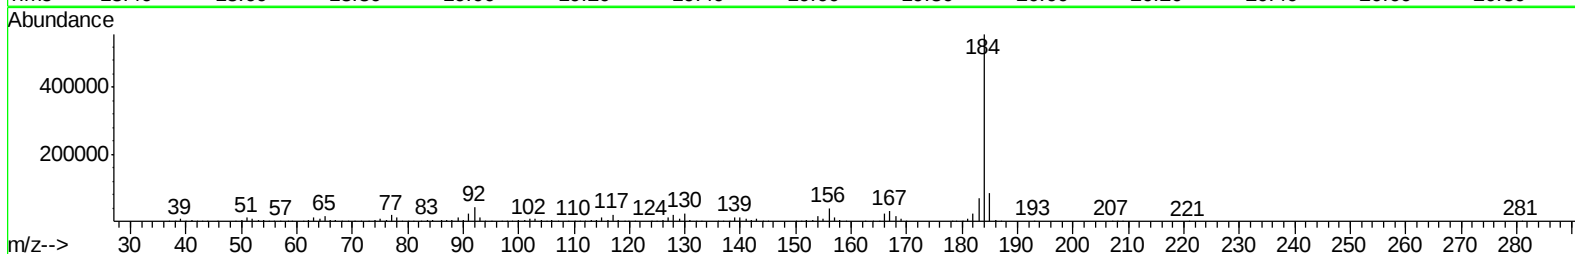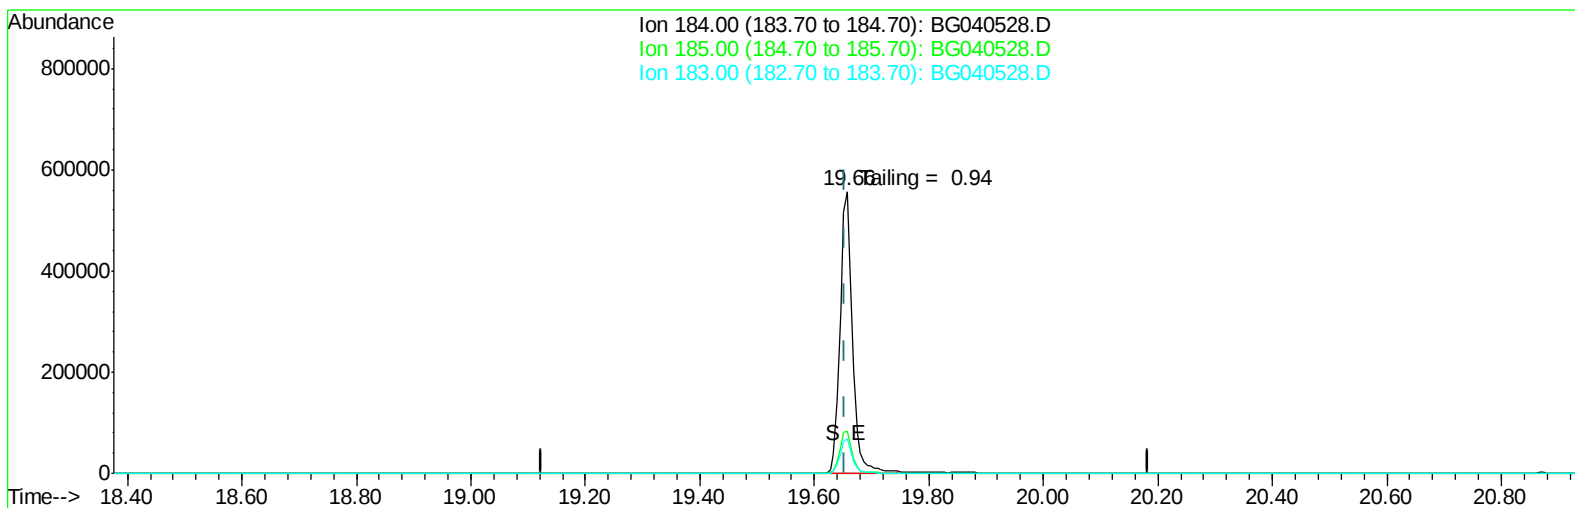

TIC: BG040528.D

(77) Benzidine

19.657min (+0.003) 327795.40ng

response 864105

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	15.20
183.00	12.90	12.24
0.00	0.00	0.00