
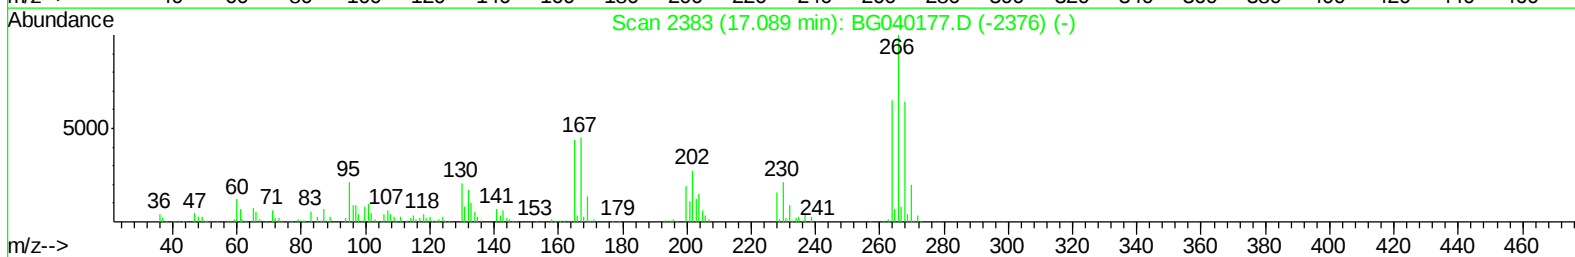
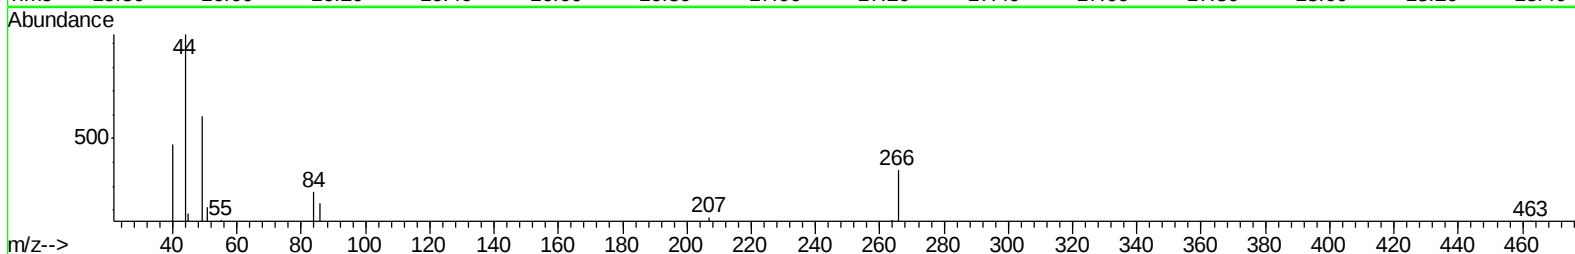


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041719\
Data File : BG040546.D
Acq On : 18 Apr 2019 1:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 05:06:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration

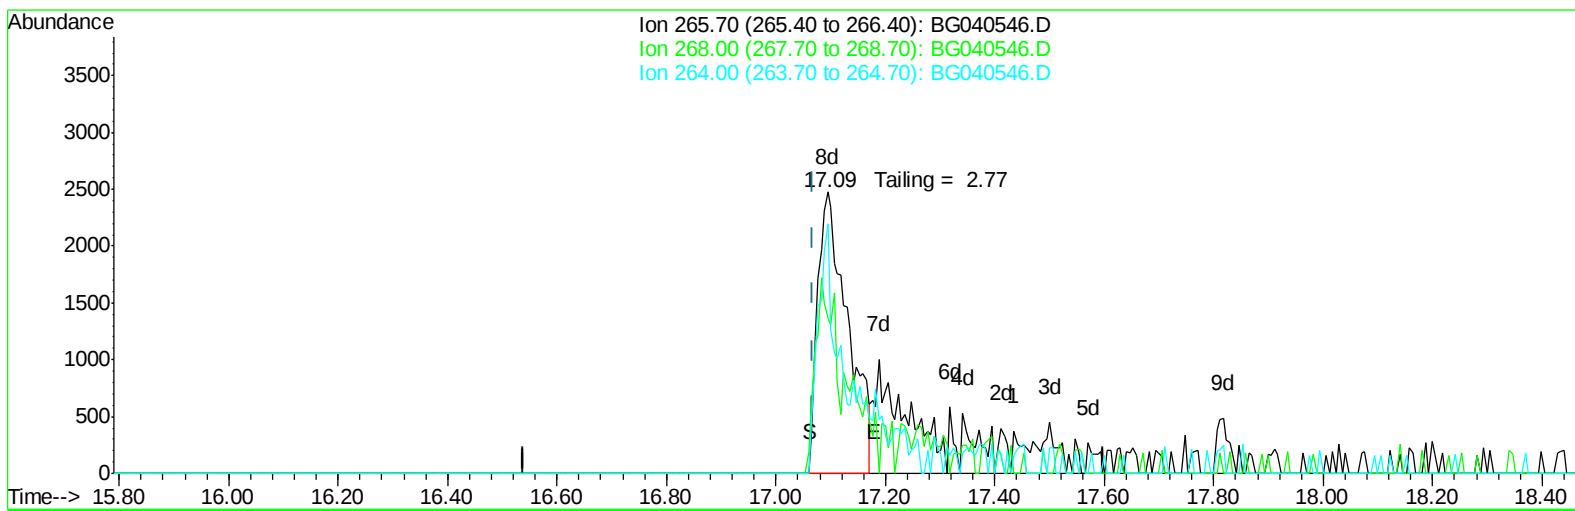

TIC: BG040546.D

(70) Pentachlorophenol (C)




17.435min (+0.366) 132.70ng

response 533

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	0.00#
264.00	64.80	43.60#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041719\
Data File : BG040546.D
Acq On : 18 Apr 2019 1:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 05:06:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration

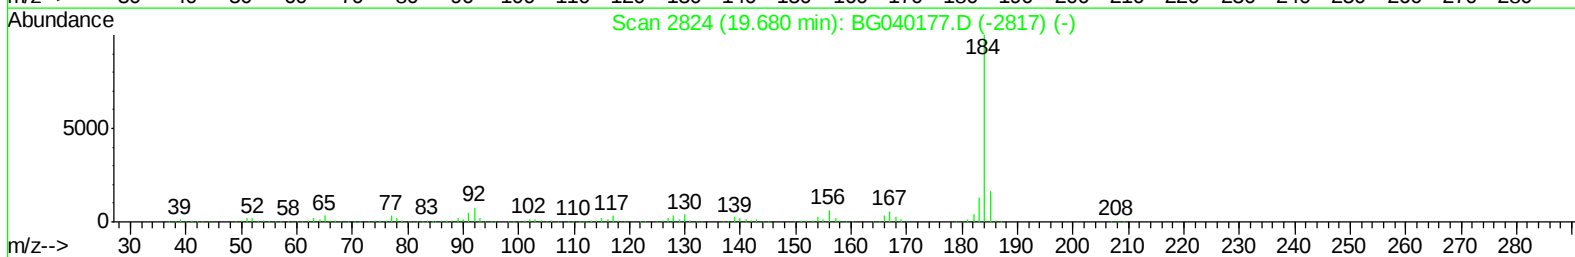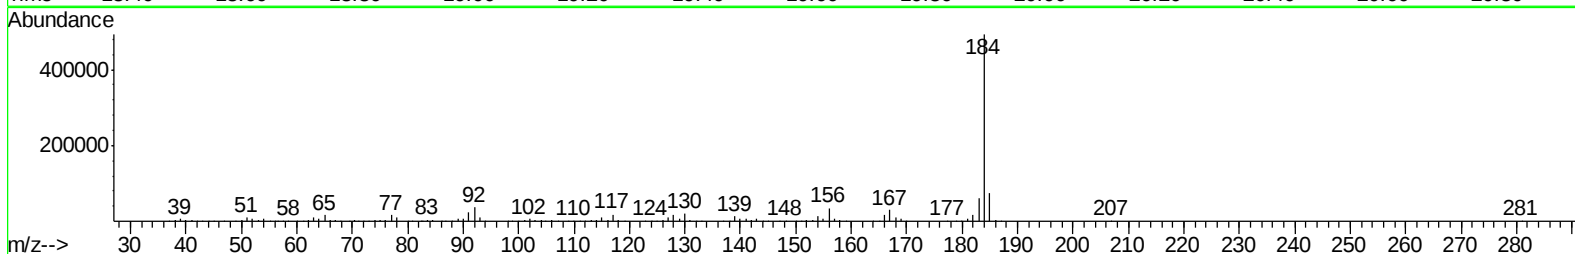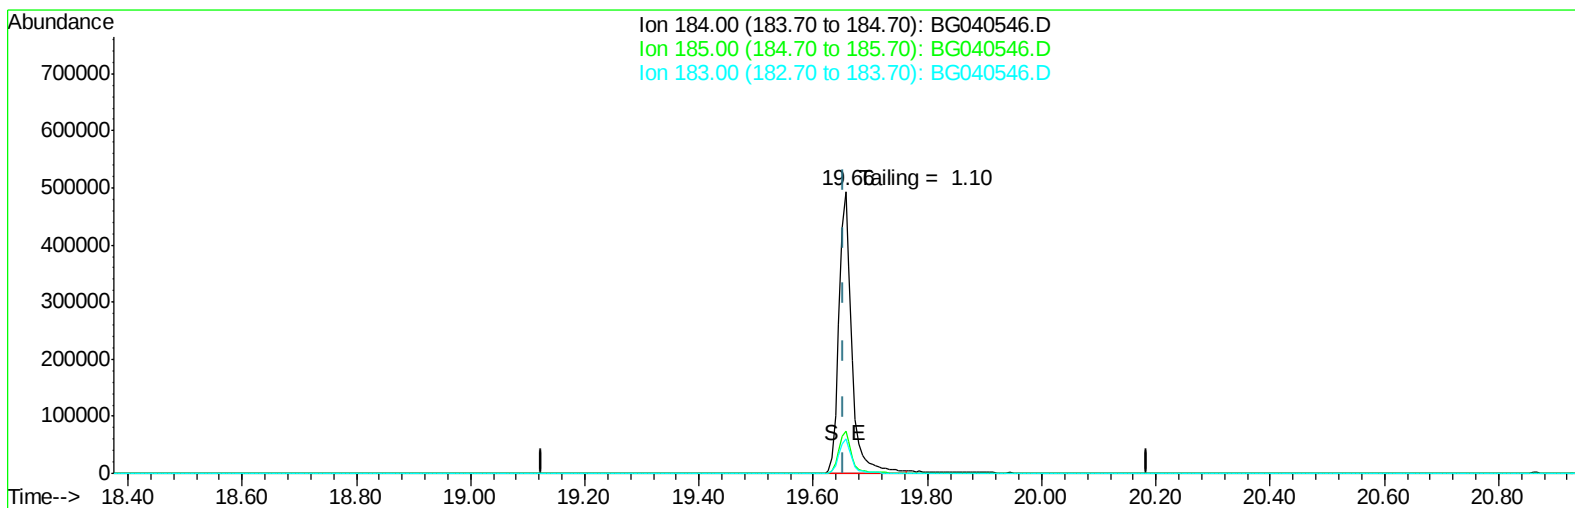

TIC: BG040546.D

(77) Benzidine

19.656min (+0.002) 0.00ng

response 781884

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	14.91
183.00	12.90	12.44
0.00	0.00	0.00