


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041719\
 Data File : BG040528.D
 Acq On : 17 Apr 2019 13:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Apr 13 00:33:11 2019

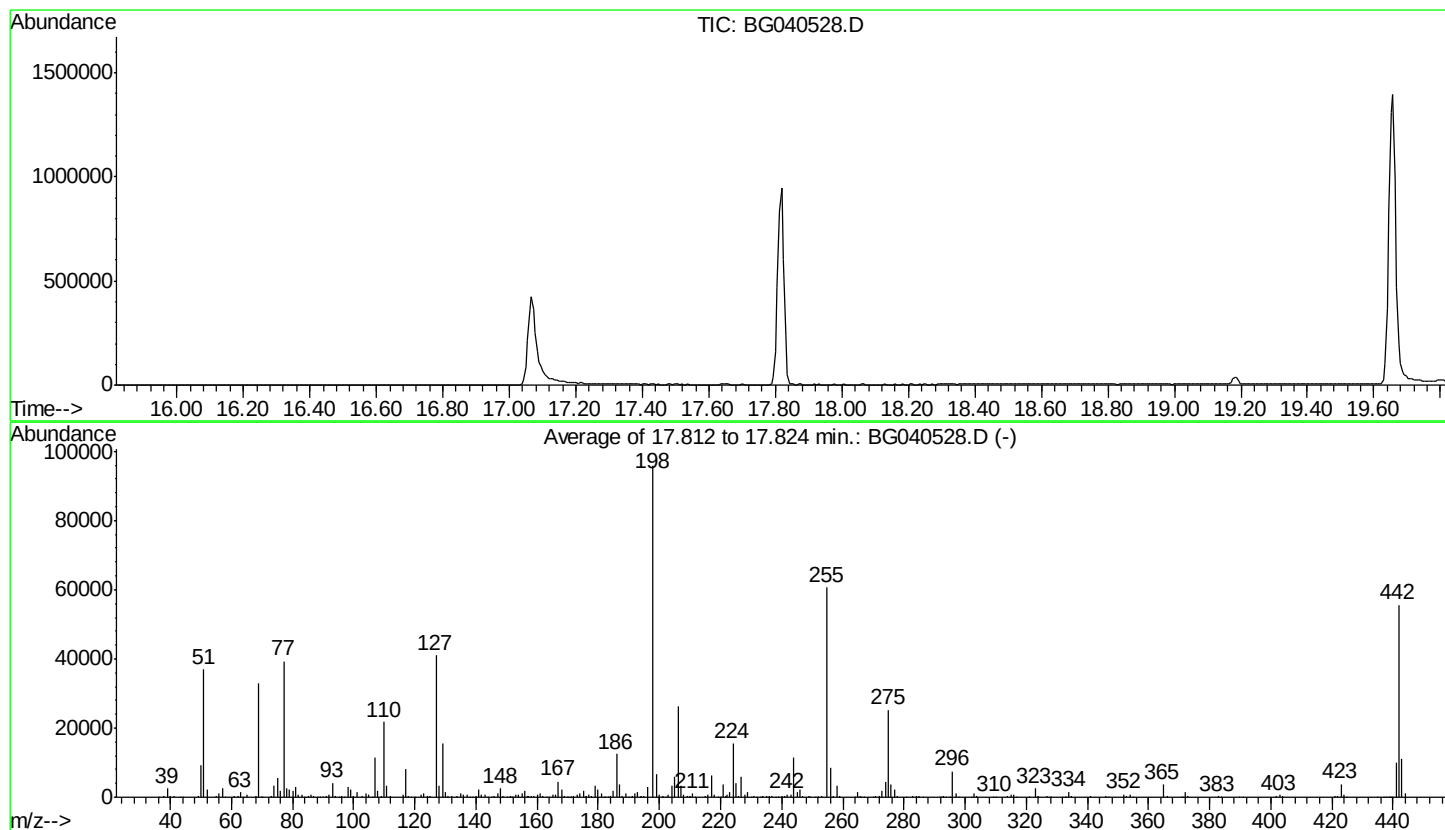

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	36837	PASS
68	69	0.00	2	1.1	373	PASS
69	198	0.00	100	34.3	32858	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	42.8	41008	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95858	PASS
199	198	5	9	6.8	6500	PASS
275	198	10	60	26.4	25349	PASS
365	198	1	100	3.7	3528	PASS
441	198	0.01	100	10.3	9902	PASS
442	198	50	100	58.0	55642	PASS
443	442	15	24	20.1	11158	PASS