


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041719\
 Data File : BG040546.D
 Acq On : 18 Apr 2019 1:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Apr 13 00:33:11 2019

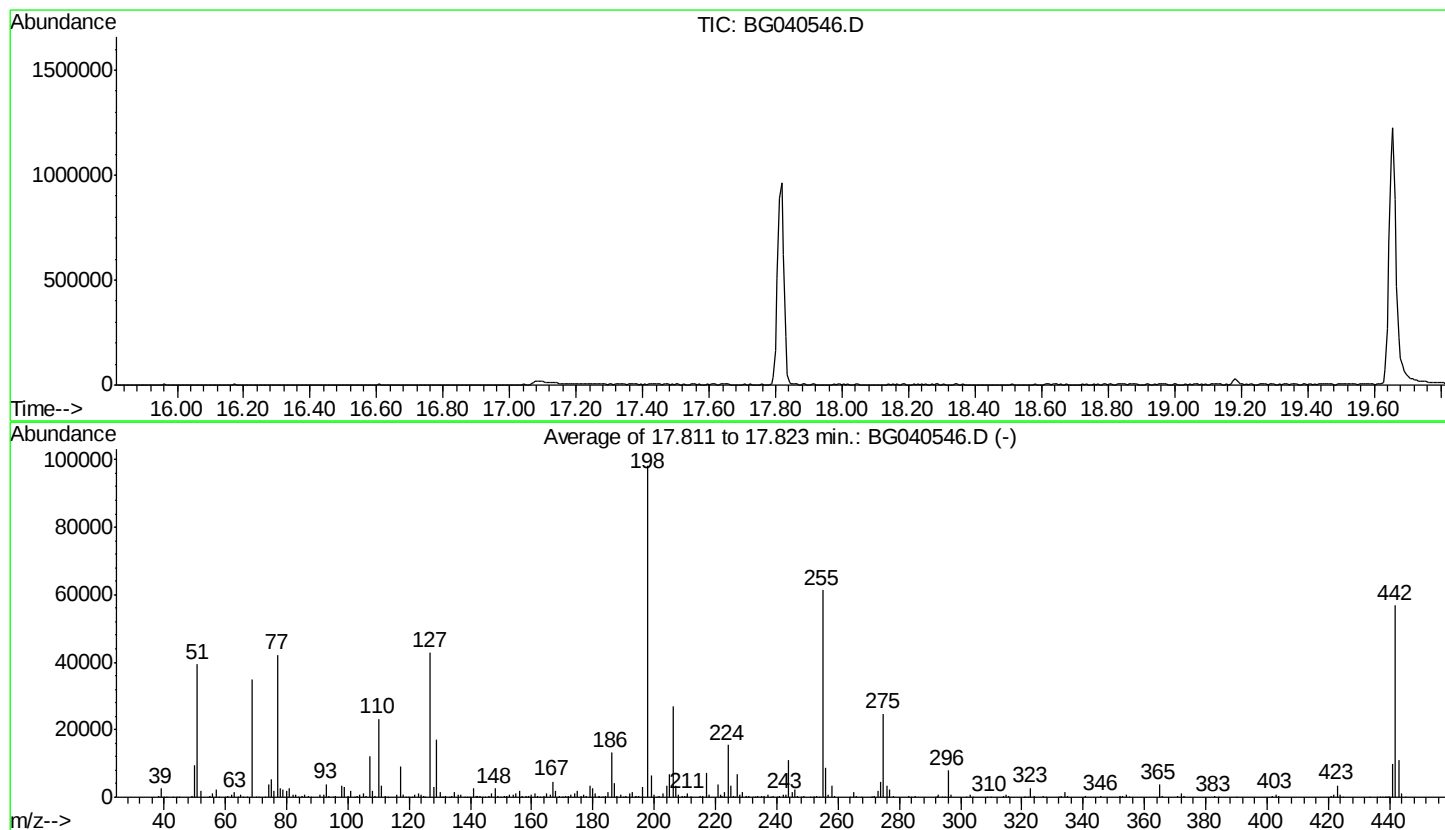

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	39362	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	34949	PASS
70	69	0.00	2	0.3	111	PASS
127	198	10	80	43.6	42792	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98250	PASS
199	198	5	9	6.5	6415	PASS
275	198	10	60	25.2	24768	PASS
365	198	1	100	3.8	3750	PASS
441	198	0.01	100	9.9	9755	PASS
442	198	50	100	57.8	56792	PASS
443	442	15	24	19.7	11198	PASS