

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041720\
 Data File : BG045043.D
 Acq On : 17 Apr 2020 23:07
 Operator : CG/JU
 Sample : PB128298BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB128298BL

Quant Time: Apr 18 02:25:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 17 11:08:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	60645	20.00	ng	0.00
21) Naphthalene-d8	10.83	136	270178	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	217614	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	523822	20.00	ng	0.00
76) Chrysene-d12	21.66	240	513252	20.00	ng	0.00
87) Perylene-d12	24.85	264	532736	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.59	112	489450	133.24	ng	0.00
7) Phenol-d6	7.18	99	749184	137.27	ng	0.00
23) Nitrobenzene-d5	9.18	82	566933	95.75	ng	0.00
42) 2,4,6-Tribromophenol	16.15	330	490421	145.88	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	1410400	95.04	ng	0.00
79) Terphenyl-d14	20.01	244	2389022	101.45	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	7.18	77	1328	Below Cal	#	4
19) n-Nitroso-di-n-propylamine	9.18	70	74815	19.384	ng	# 81
32) Benzoic acid	10.01	122	77	6.394	ng	# 1
51) 2,6-Dinitrotoluene	14.65	165	27450	6.926	ng	# 27
57) 2,4-Dinitrotoluene	14.65	165	27450	4.739	ng	# 24
67) 4-Bromophenyl-phenylether	16.14	248	32503	4.810	ng	# 1
69) Atrazine	16.41	200	66	Below Cal	#	35
74) Di-n-butylphthalate	18.44	149	68	Below Cal	#	76
75) Fluoranthene	19.45	202	61	Below Cal	#	62
77) Benzidine	20.01	184	47673	Below Cal	#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041720\
Data File : BG045043.D
Acq On : 17 Apr 2020 23:07
Operator : CG/JU
Sample : PB128298BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB128298BL

Quant Time: Apr 18 02:25:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 11:08:29 2020
Response via : Initial Calibration

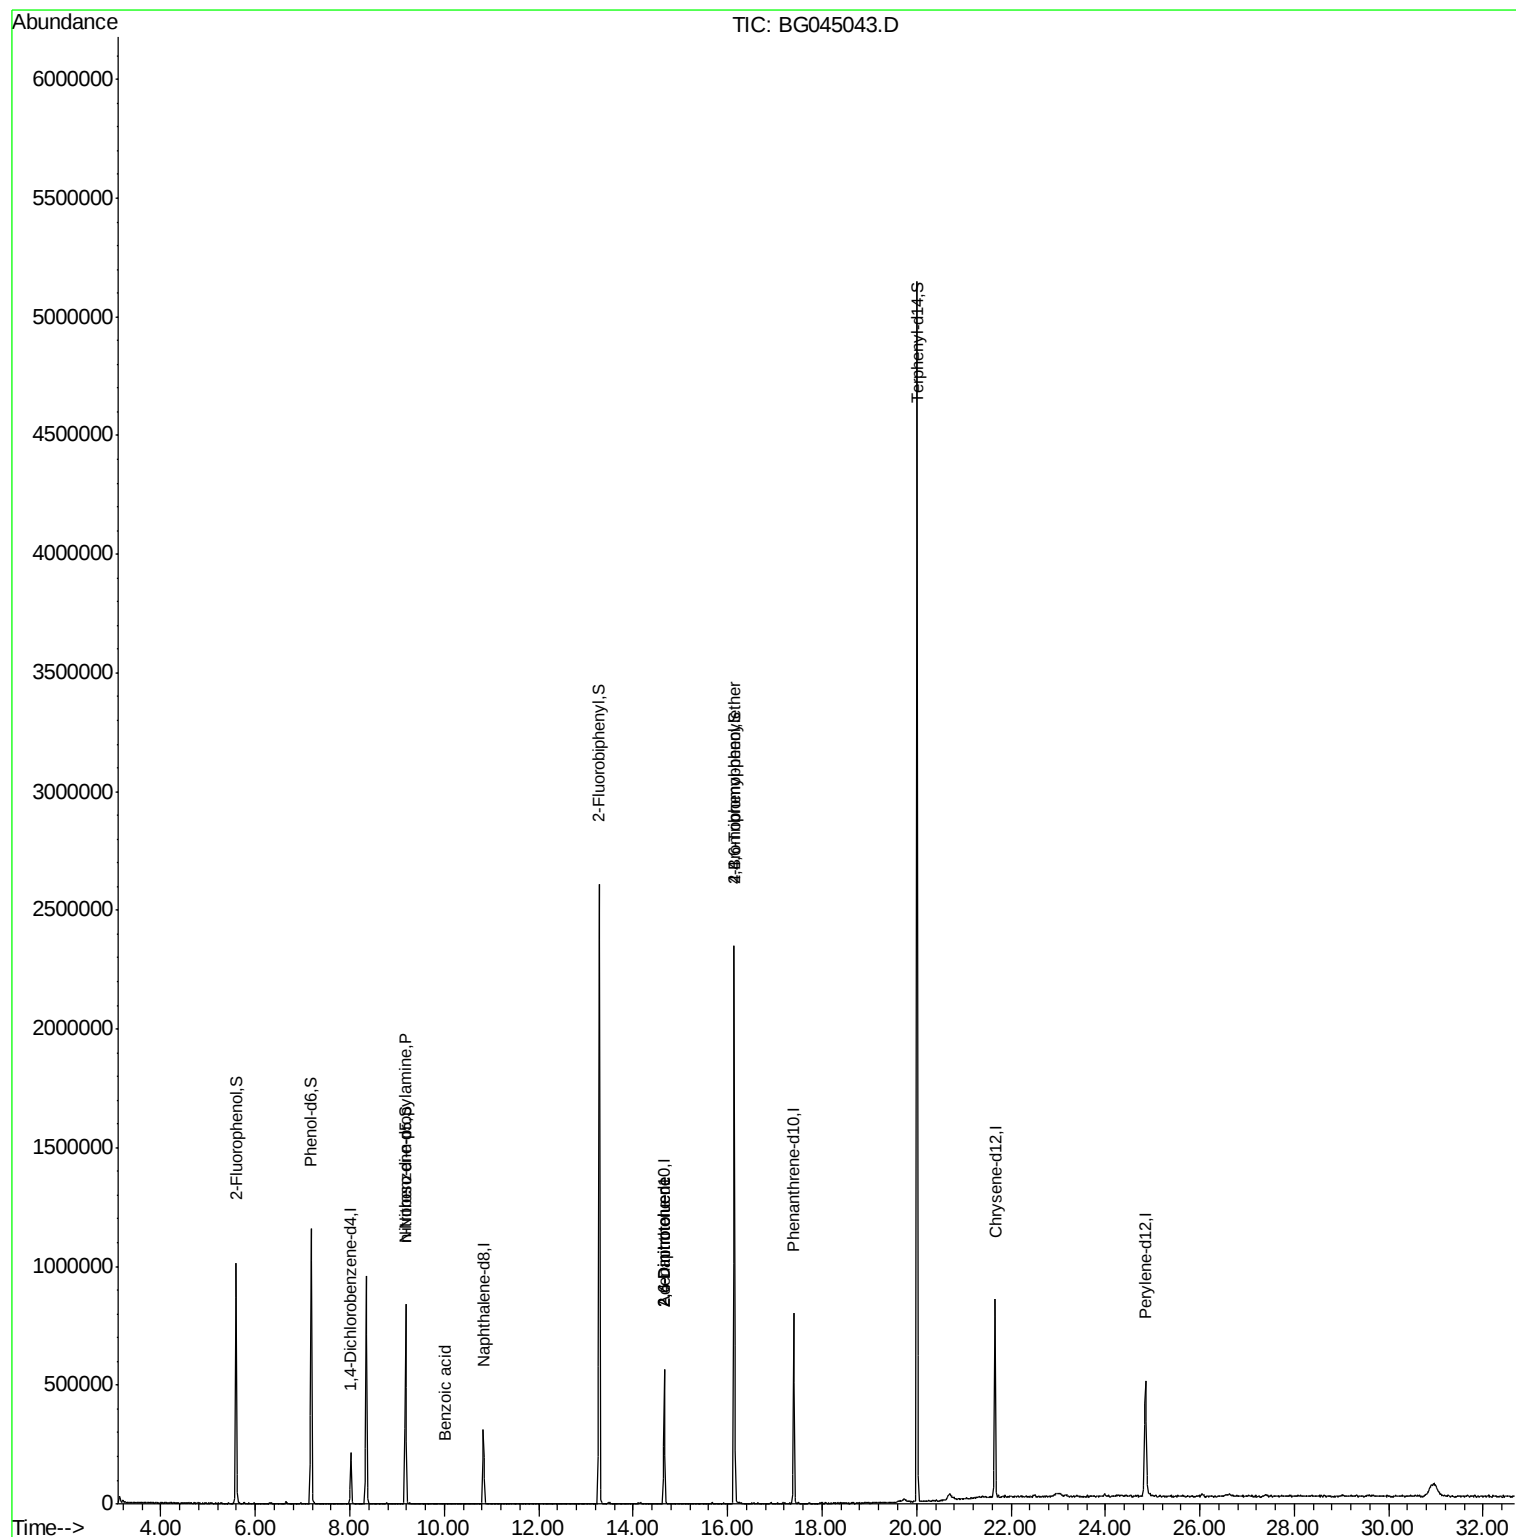






#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.02 min Scan# 840
Delta R.T. -0.00 min
Lab File: BG045043.D
Acq: 17 Apr 2020 23:07

Instrument :
BNA_G
ClientSampleId :
PB128298BL




Tot Ion	Ratio	Lower	Upper
152	100		
150	164.3	123.6	185.4
115	60.8	49.1	73.7

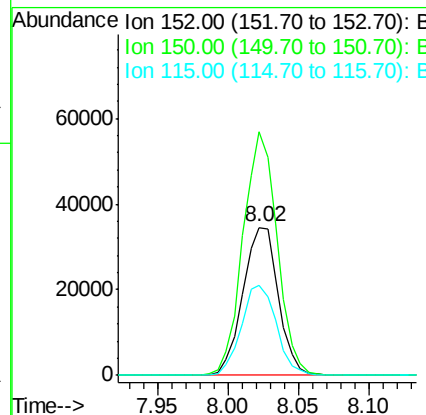
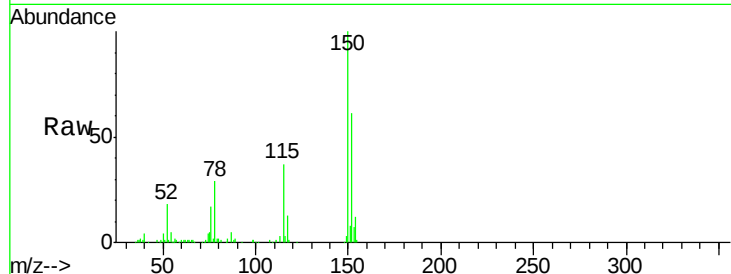


#5

2-Fluorophenol
Concen: 133.244 ng
RT: 5.59 min Scan# 426
Delta R.T. -0.00 min
Lab File: BG045043.D
Acq: 17 Apr 2020 23:07

Tgt Ion	Ratio	Lower	Upper
112	100		
64	54.0	42.4	63.6
63	31.4	23.1	34.7

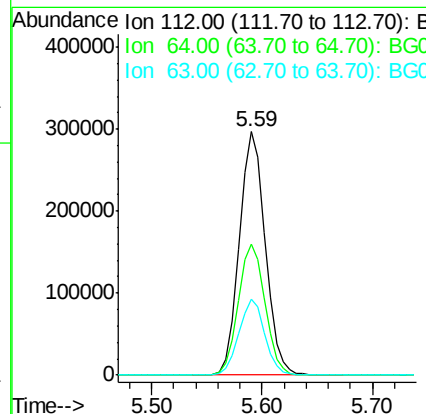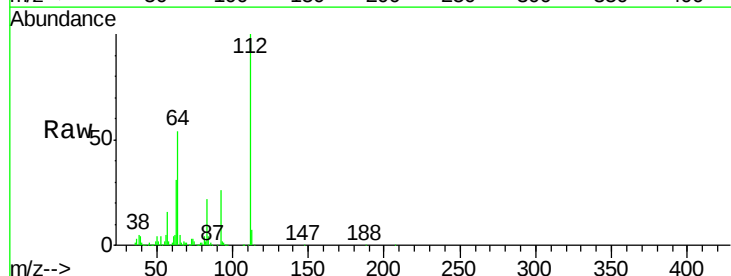

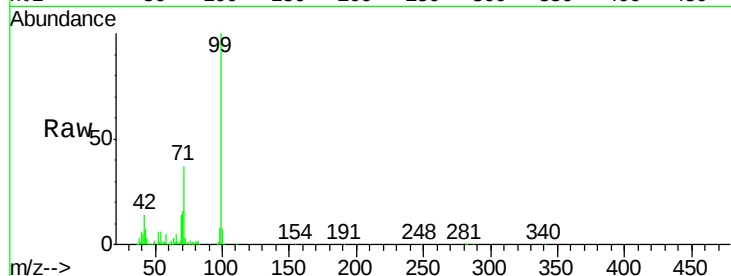

#7

Phenol-d6

Concen: 137.272 ng

RT: 7.18 min Scan# 697

Delta R.T. -0.00 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07

Instrument :

BNA_G

ClientSampleId :

PB128298BL





Tot Ion: 99 Resp: 749184

Ion Ratio Lower Upper

99 100

42 13.5 11.3 16.9

71 37.3 28.3 42.5

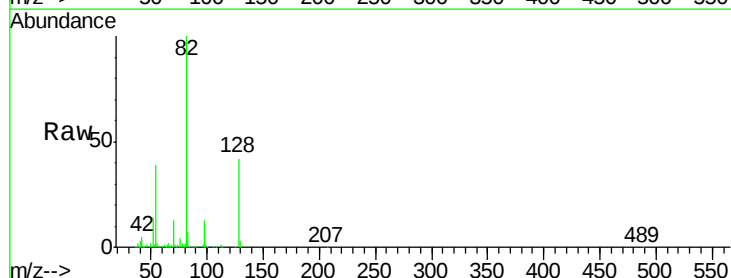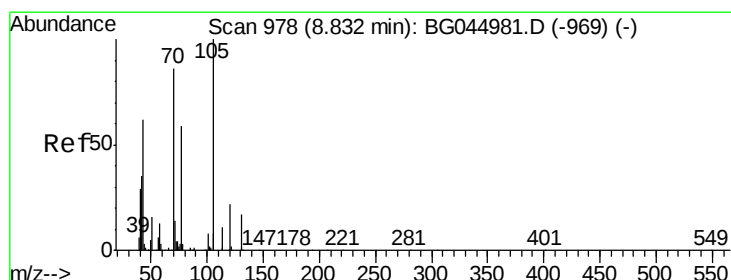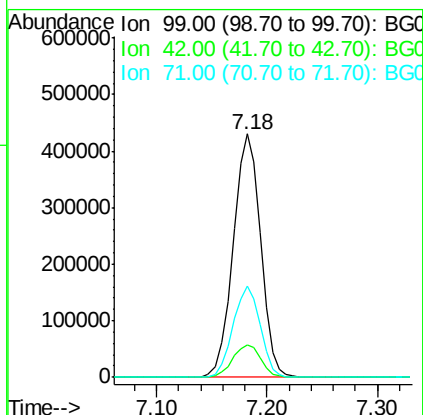

#19

n-Nitroso-di-n-propylamine

Concen: 19.384 ng

RT: 9.18 min Scan# 1037

Delta R.T. 0.35 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07

Tgt Ion: 70 Resp: 74815


Ion Ratio Lower Upper


70 100

42 37.4 33.3 49.9

101 0.0 7.8 11.8#

130 1.5 15.8 23.6#




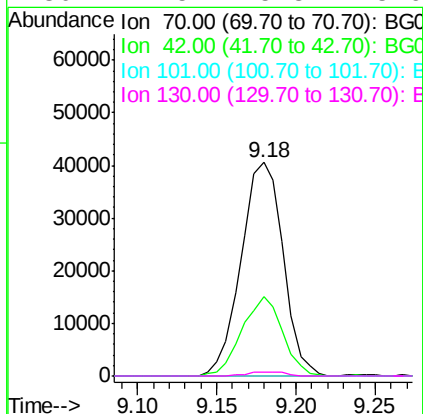


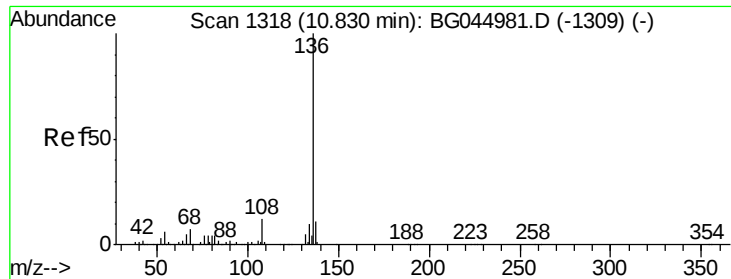

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.83 min Scan# 1318
Delta R.T. -0.00 min
Lab File: BG045043.D
Acq: 17 Apr 2020 23:07




Instrument :
BNA_G
ClientSampleId :
PB128298BL


Tot Ion:136	Resp: 270178
Ion Ratio	Lower Upper
136 100	
137 9.9	8.6 13.0
54 6.2	4.8 7.2
68 6.2	5.2 7.8

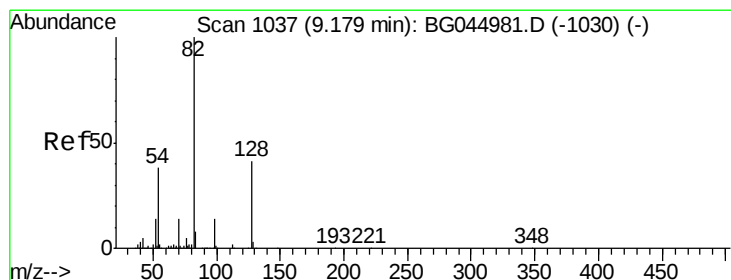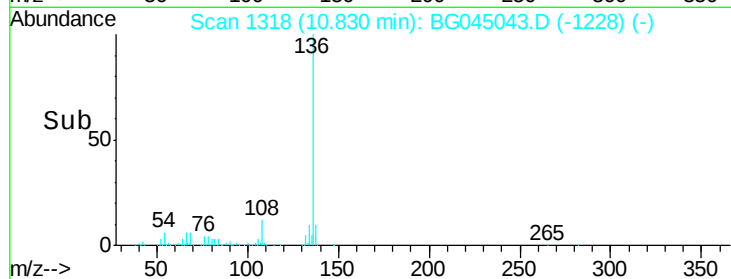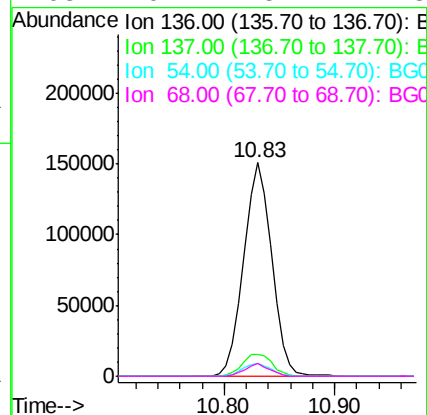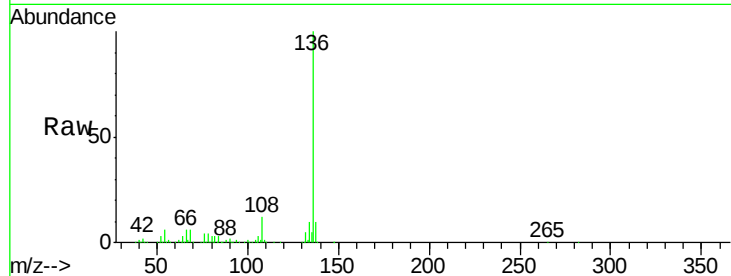

#23
Nitrobenzene-d5
Concen: 95.746 ng
RT: 9.18 min Scan# 1037
Delta R.T. -0.00 min
Lab File: BG045043.D
Acq: 17 Apr 2020 23:07

Tgt	Ion: 82	Resp:	566933
Ion	Ratio	Lower	Upper
82	100		
128	42.1	33.0	49.4
54	38.9	30.4	45.6

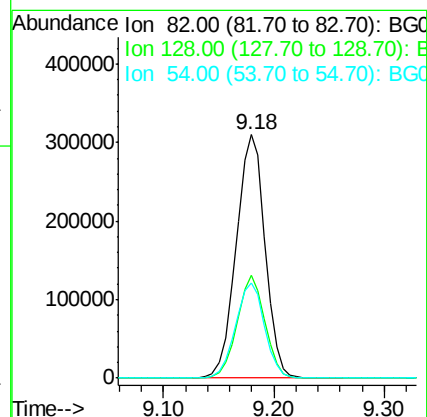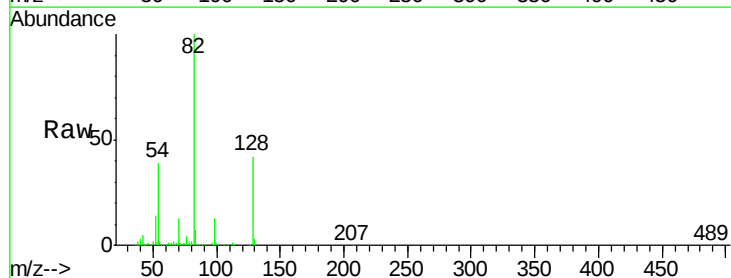

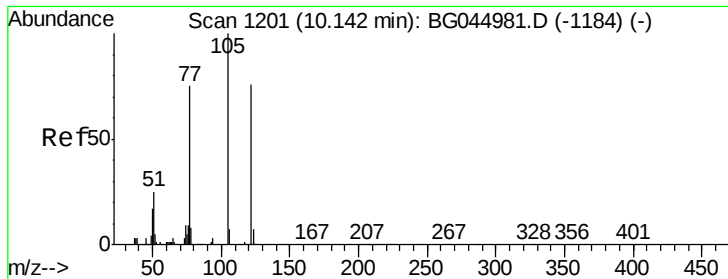

#32

Benzoic acid

Concen: 6.394 ng

RT: 10.01 min Scan# 1179

Delta R.T. -0.14 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07

Instrument :

BNA_G

ClientSampleId :

PB128298BL





Tot Ion:122 Resp: 77

Ion Ratio Lower Upper

122 100

105 0.0 108.4 148.4#

77 0.0 78.8 118.8#

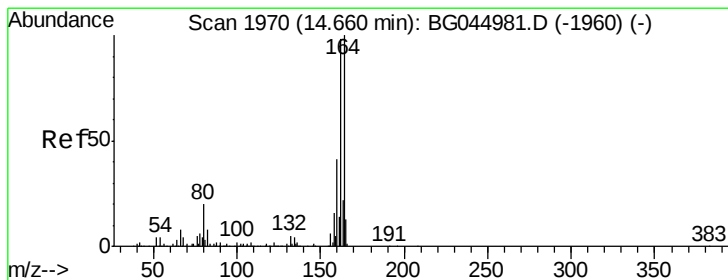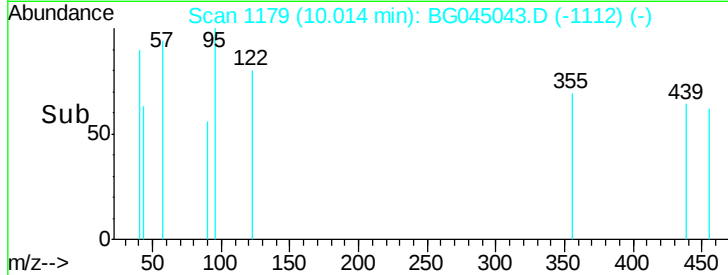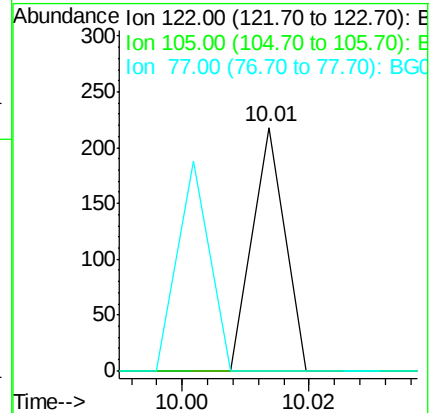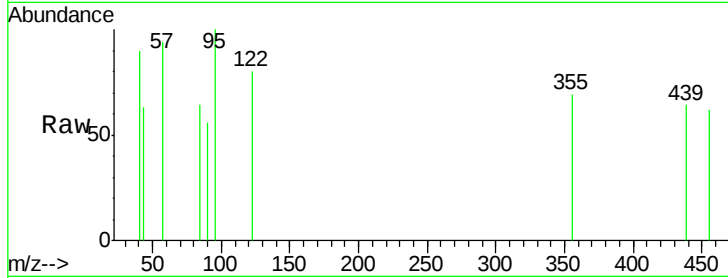

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.65 min Scan# 1969

Delta R.T. -0.00 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07




Tgt Ion:164 Resp: 217614


Ion Ratio Lower Upper

164 100

162 97.4 78.7 118.1

160 43.7 32.8 49.2


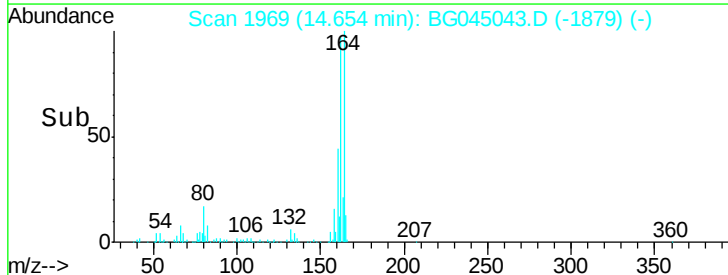
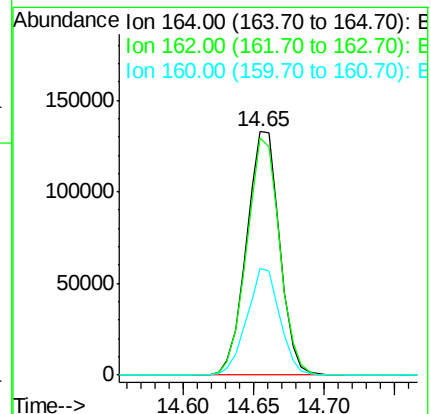
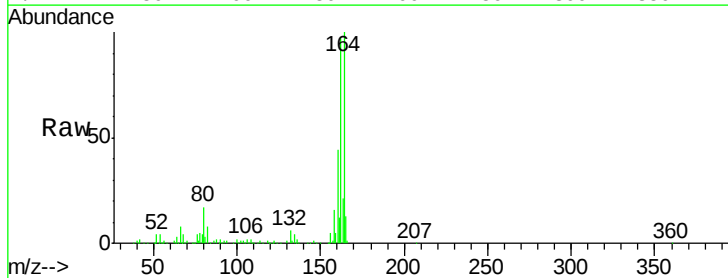


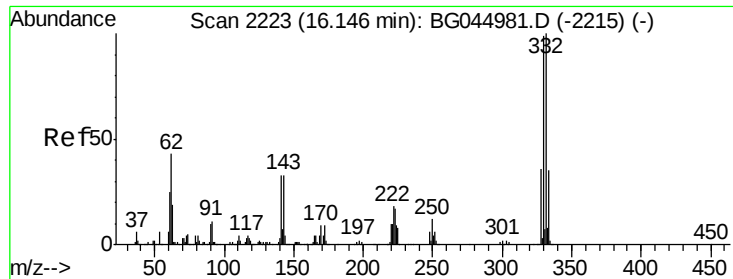

#42
 2,4,6-Tribromophenol
 Concen: 145.878 ng
 RT: 16.15 min Scan# 2223
 Delta R.T. 0.00 min
 Lab File: BG045043.D
 Acq: 17 Apr 2020 23:07




Instrument :
 BNA_G
 ClientSampleId :
 PB128298BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	79.1	118.7
141	34.3	27.1	40.7

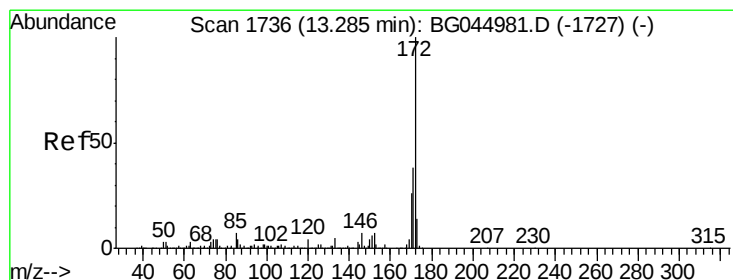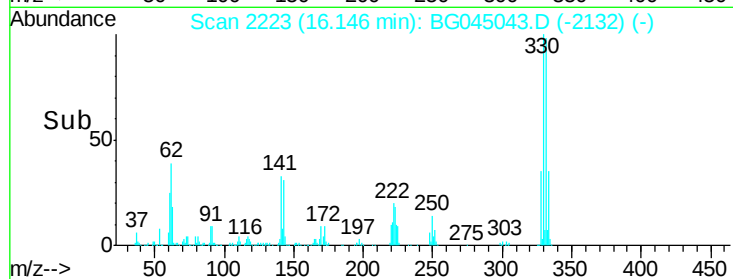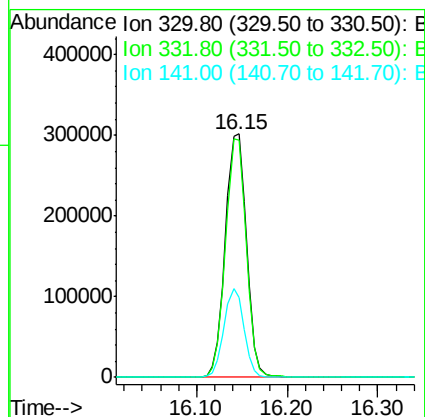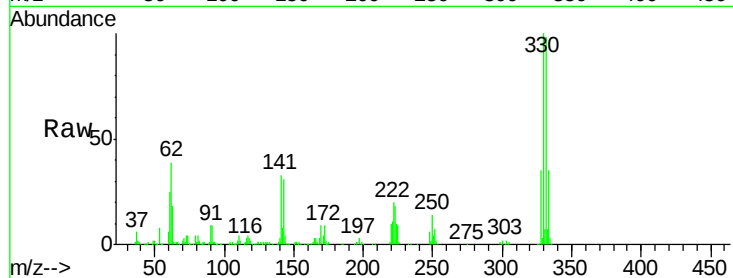

#45
 2-Fluorobiphenyl
 Concen: 95.035 ng
 RT: 13.28 min Scan# 1735
 Delta R.T. -0.00 min
 Lab File: BG045043.D
 Acq: 17 Apr 2020 23:07

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	30.6	46.0
170	24.6	20.5	30.7

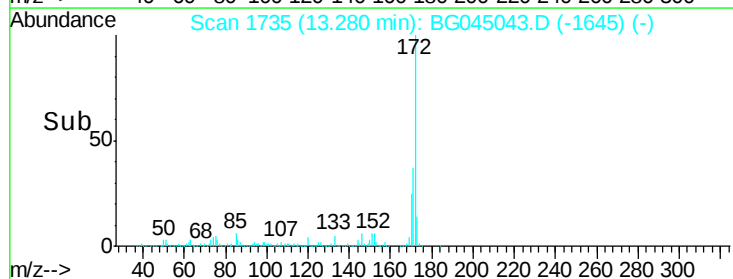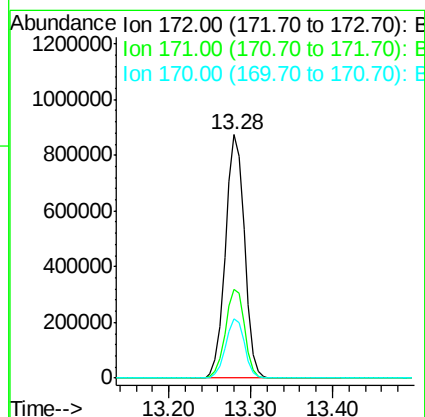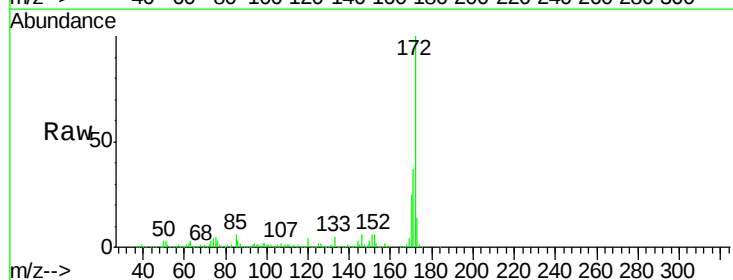


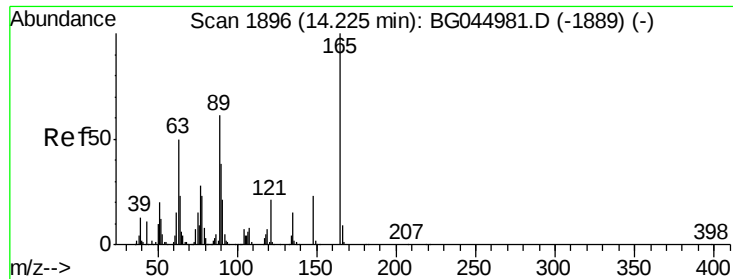




#51
 2,6-Dinitrotoluene
 Concen: 6.926 ng
 RT: 14.65 min Scan# 1969
 Delta R.T. 0.43 min
 Lab File: BG045043.D
 Acq: 17 Apr 2020 23:07

Instrument :
 BNA_G
 ClientSampleId :
 PB128298BL

Tot Ion	Ratio	Lower	Upper
165	100		
63	2.8	40.4	60.6#
89	2.5	49.1	73.7#

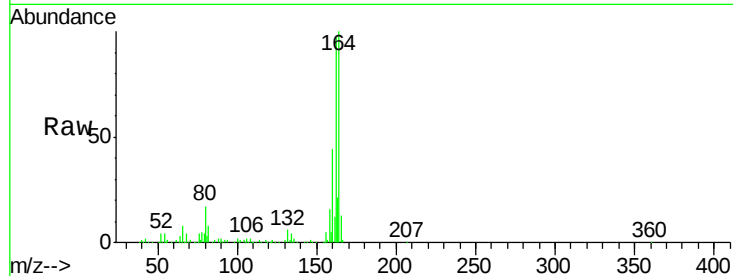


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC

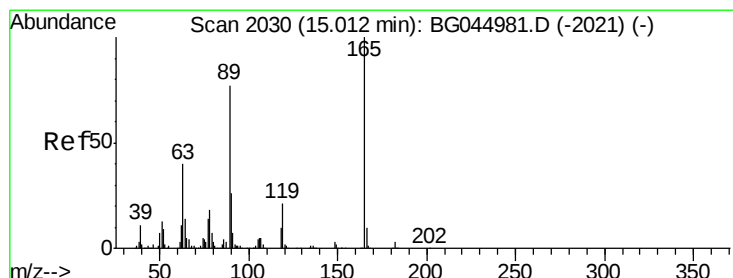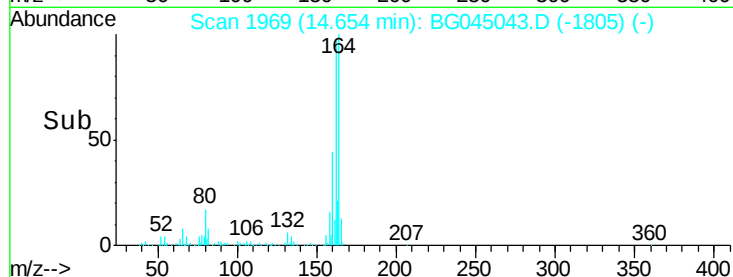
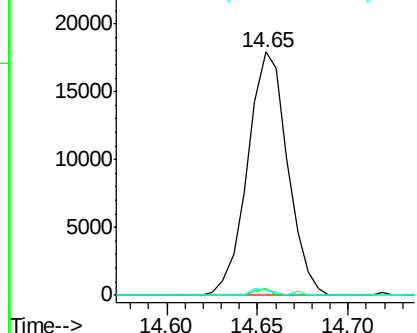



#57
 2,4-Dinitrotoluene
 Concen: 4.739 ng
 RT: 14.65 min Scan# 1969
 Delta R.T. -0.36 min
 Lab File: BG045043.D
 Acq: 17 Apr 2020 23:07

Tgt Ion	Ratio	Lower	Upper
165	100		
63	2.8	32.2	48.2#
89	2.5	61.7	92.5#
182	0.0	2.0	3.0#

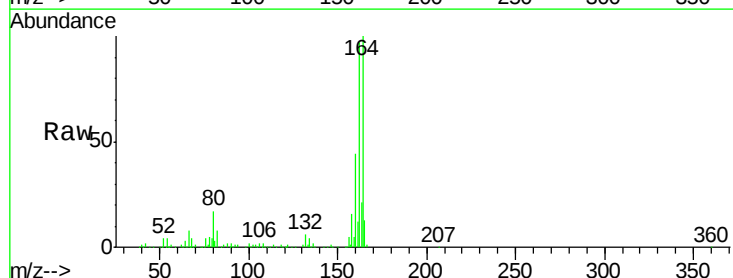

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

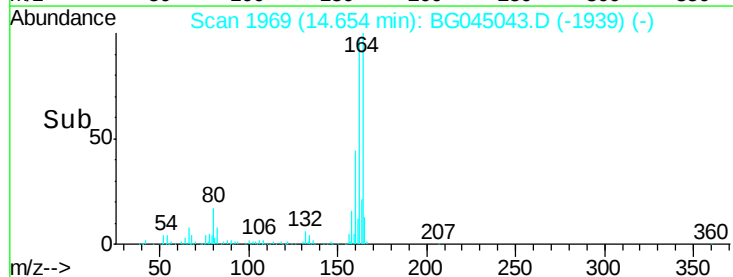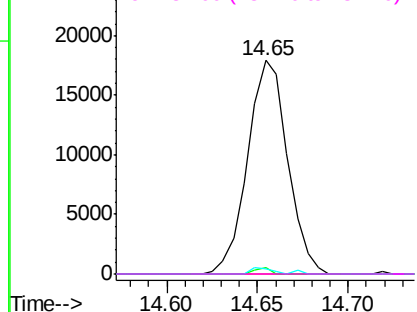

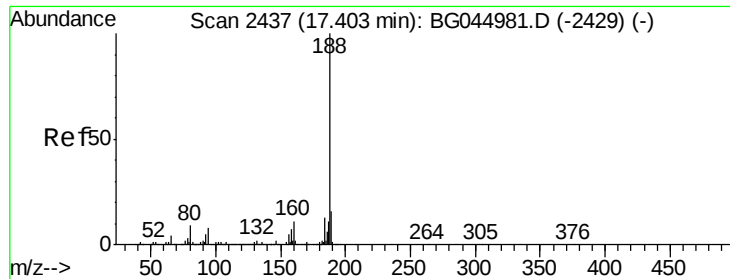

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2436

Delta R.T. -0.00 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07

Instrument :

BNA_G

ClientSampleId :

PB128298BL


Tot Ion:188 Resp: 523822

Ion Ratio Lower Upper

188 100

94 7.9 6.2 9.4




80 8.1 7.0 10.6

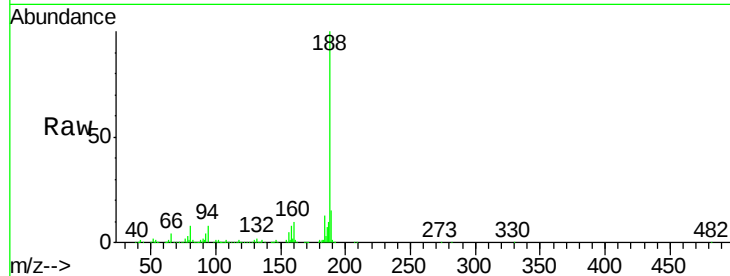

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

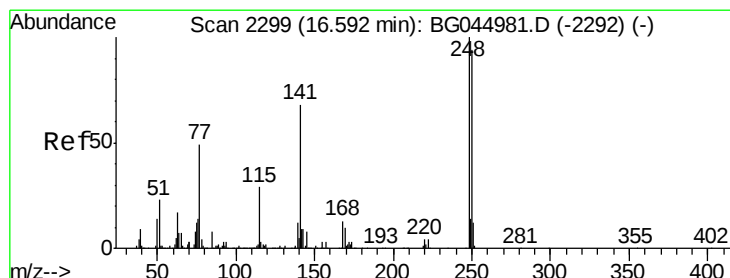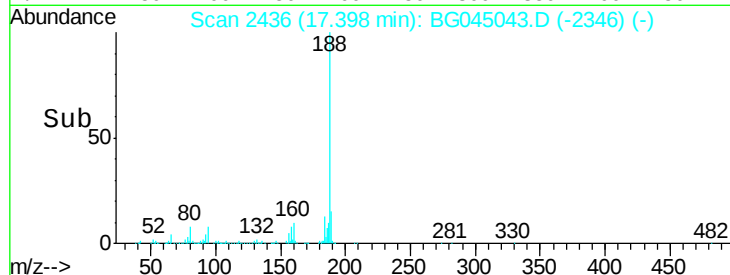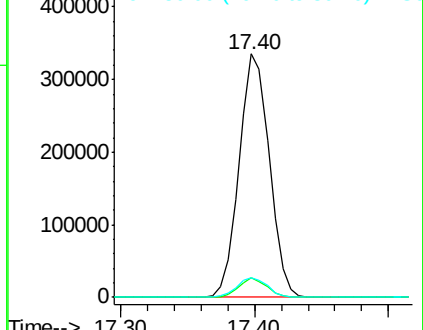

#67

4-Bromophenyl-phenylether

Concen: 4.810 ng

RT: 16.14 min Scan# 2222

Delta R.T. -0.45 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07


Tgt Ion:248 Resp: 32503

Ion Ratio Lower Upper

248 100

250 188.2 75.4 113.2#



141 494.1 54.4 81.6#

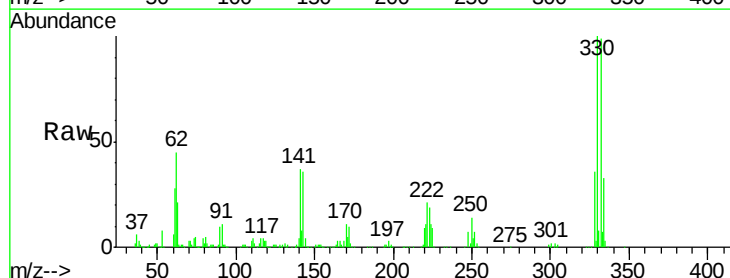


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

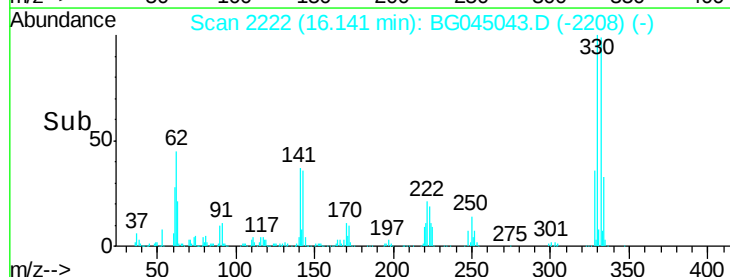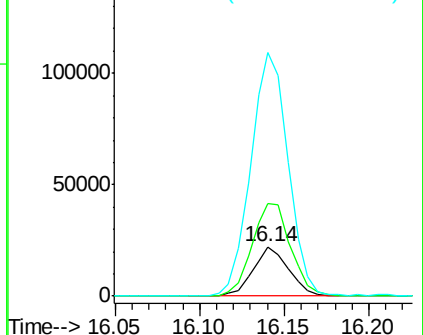



#69

Atrazine

Concen: Below Cal

RT: 16.41 min Scan# 2268

Delta R.T. -0.45 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07

Instrument :

BNA_G

ClientSampleId :

PB128298BL


Tot Ion:200 Resp: 66

Ion Ratio Lower Upper

200 100

173 0.0 4.5 44.5#




215 0.0 30.0 70.0#

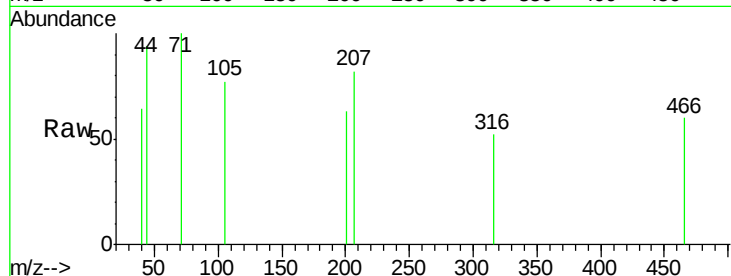

Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

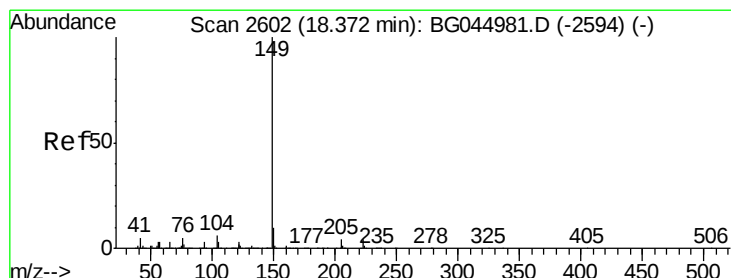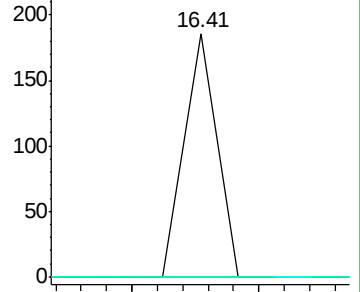

#74

Di-n-butylphthalate

Concen: Below Cal

RT: 18.44 min Scan# 2613

Delta R.T. 0.07 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07


Tgt Ion:149 Resp: 68

Ion Ratio Lower Upper

149 100

150 0.0 8.2 12.2#



104 0.0 4.8 7.2#

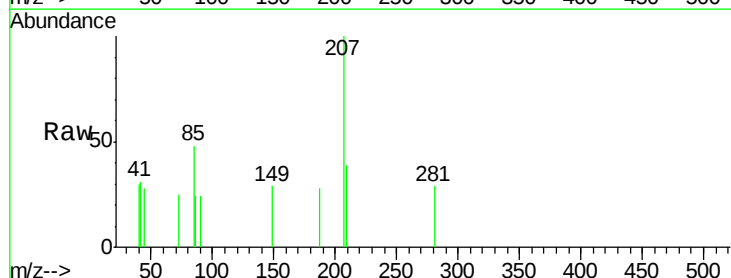


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

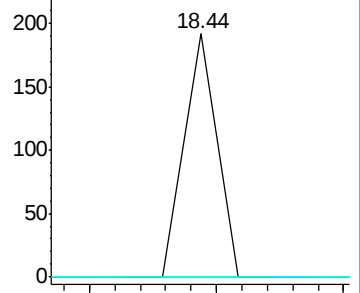



#75

Fluoranthene

Concen: Below Cal

RT: 19.45 min Scan# 2786

Delta R.T. 0.00 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07


Instrument :

BNA_G

ClientSampleId :

PB128298BL




Tot Ion:	202	Resp:	61
Ion	Ratio	Lower	Upper
202	100		
101	0.0	0.0	29.6
203	0.0	0.0	39.7

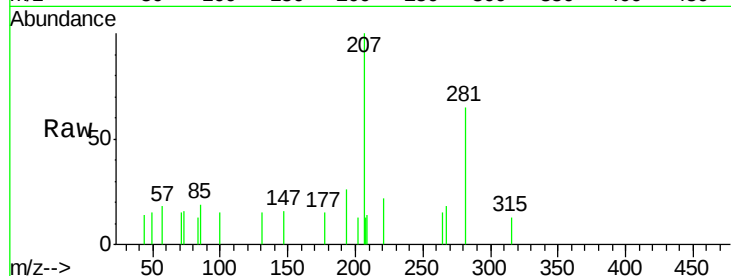

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

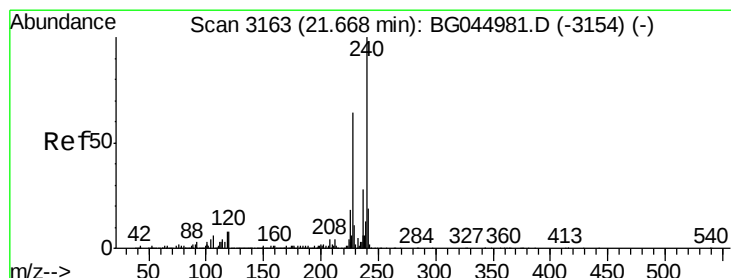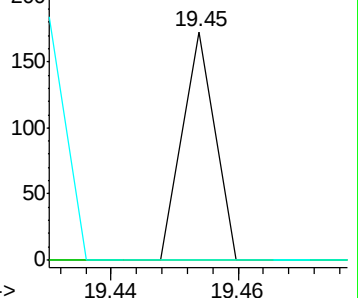

#76

Chrysene-d12

Concen: 20.000 ng


RT: 21.66 min Scan# 3162

Delta R.T. -0.00 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07



Tgt Ion:	240	Resp:	513252
Ion	Ratio	Lower	Upper
240	100		
120	6.8	6.6	10.0
236	26.3	22.2	33.2

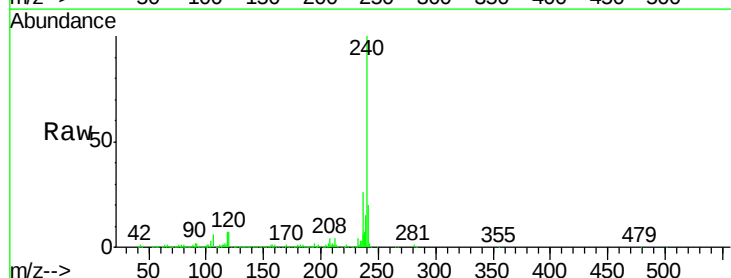

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

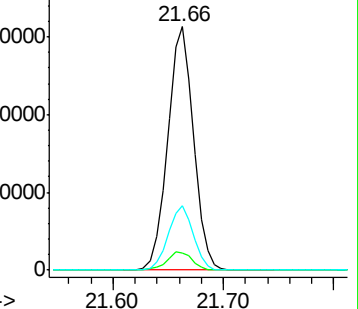



#77

Benzidine

Concen: Below Cal

RT: 20.01 min Scan# 2881

Delta R.T. 0.39 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07

Instrument :

BNA_G

ClientSampleId :

PB128298BL


Tot Ion:184 Resp: 47673

Ion Ratio Lower Upper

184 100

185 16.0 12.6 19.0




183 7.2 11.3 16.9#

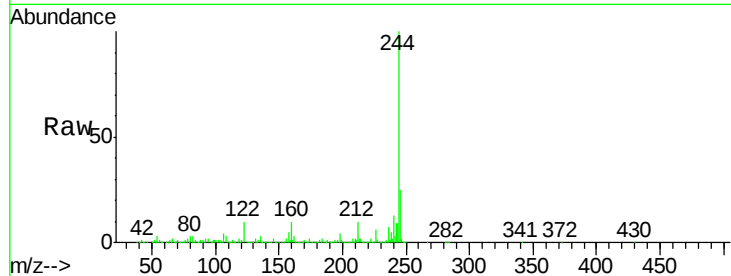

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

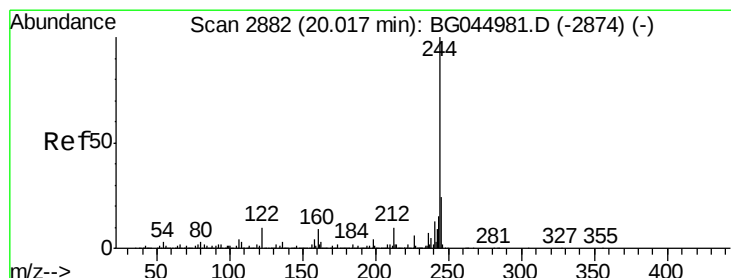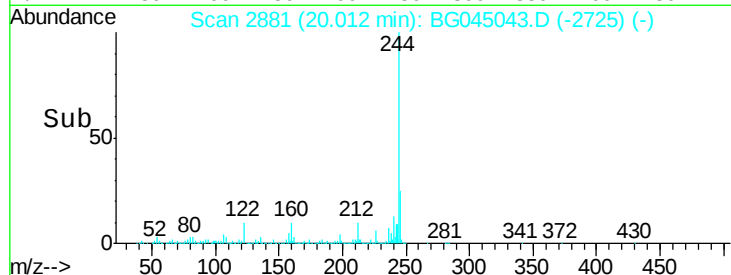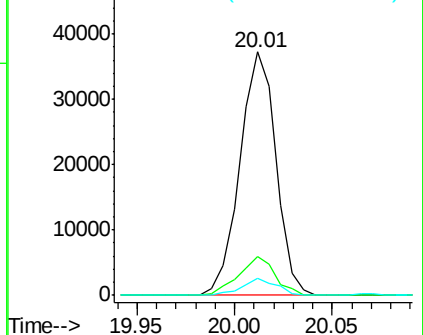

#79

Terphenyl-d14

Concen: 101.452 ng

RT: 20.01 min Scan# 2881

Delta R.T. -0.00 min

Lab File: BG045043.D

Acq: 17 Apr 2020 23:07


Tgt Ion:244 Resp: 2389022

Ion Ratio Lower Upper

244 100

212 10.5 7.9 11.9



122 9.9 7.7 11.5

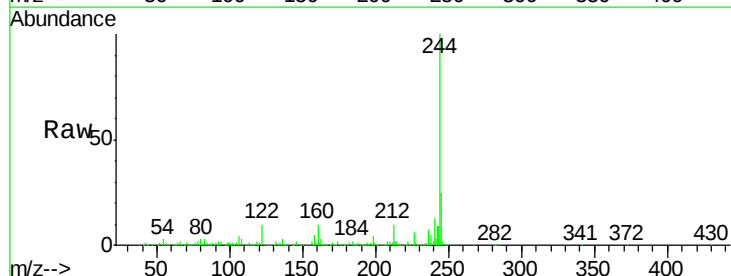


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

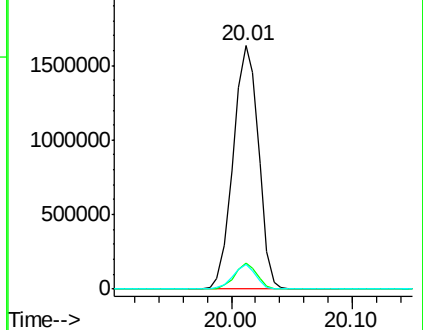




#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.85 min Scan# 3705
Delta R.T. -0.00 min
Lab File: BG045043.D
Acq: 17 Apr 2020 23:07

Instrument :
BNA_G
ClientSampleId :
PB128298BL

Tot Ion	Ratio	Lower	Upper
264	100		
260	21.8	19.2	28.8
265	22.8	19.0	28.4


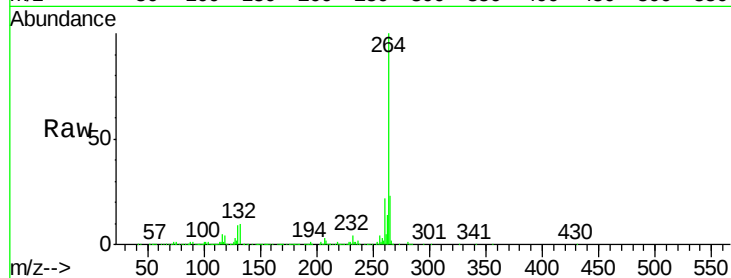


Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

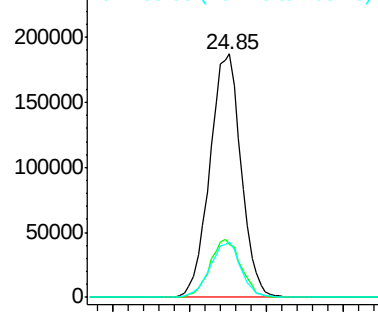

Time-->