
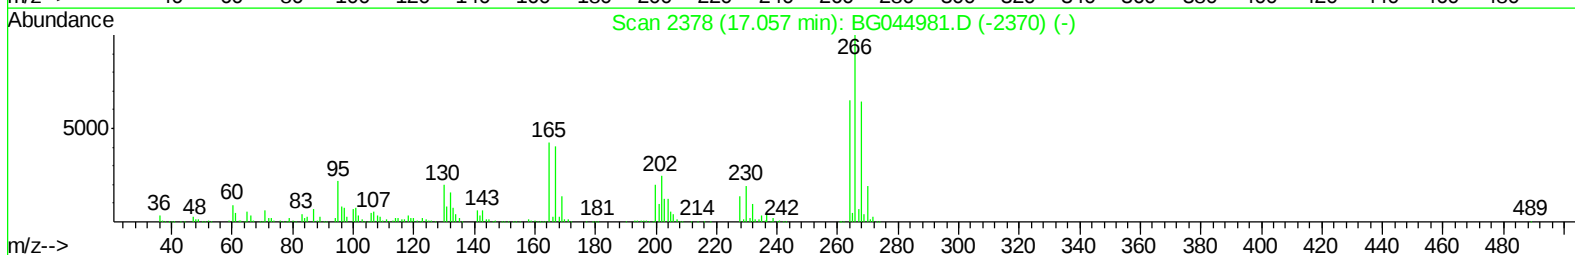
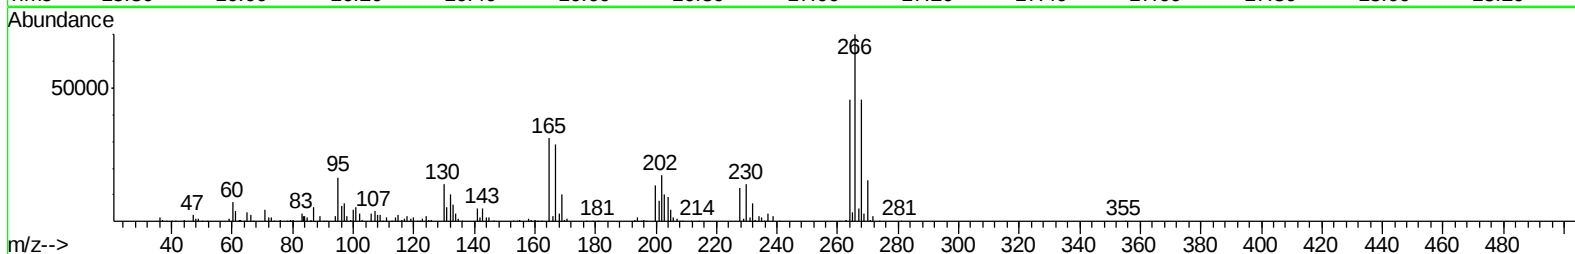


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG041720\
 Data File : BG045041.D
 Acq On : 17 Apr 2020 21:07
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 04:15:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 17 11:08:29 2020
 Response via : Initial Calibration

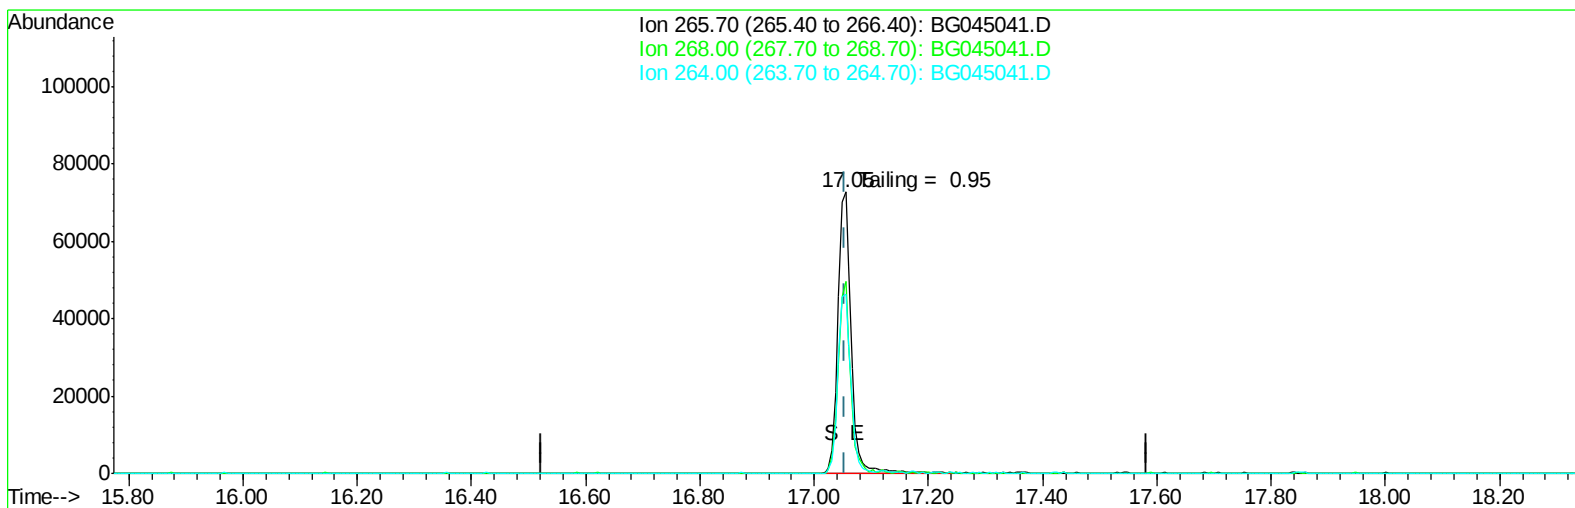

TIC: BG045041.D

(70) Pentachlorophenol (C)




17.054min (+0.001) 249226.28ng

response 116601

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	68.36
264.00	65.30	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG041720\
Data File : BG045041.D
Acq On : 17 Apr 2020 21:07
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 04:15:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 11:08:29 2020
Response via : Initial Calibration

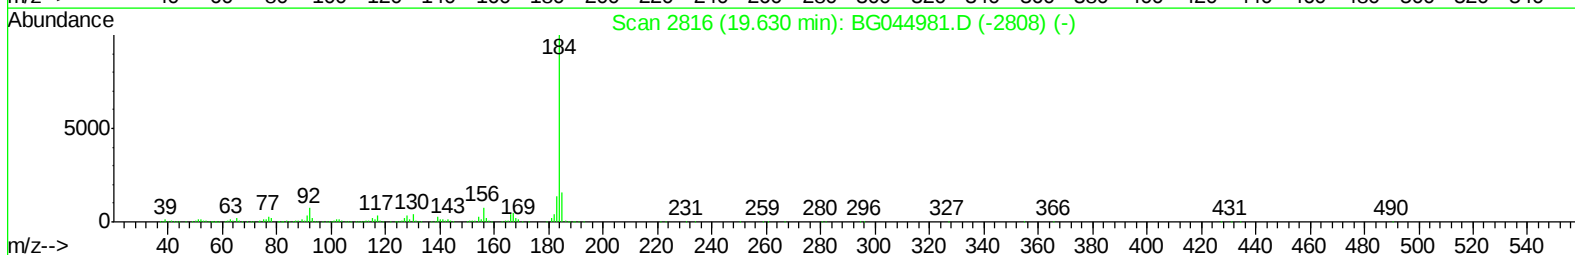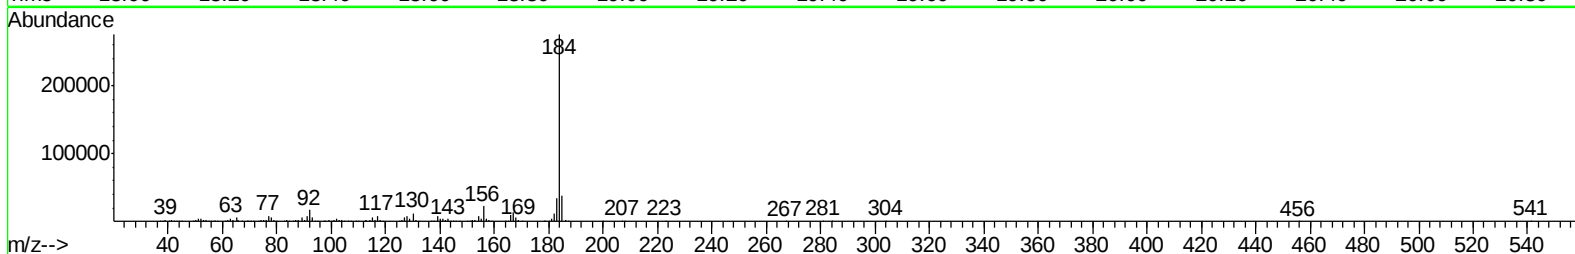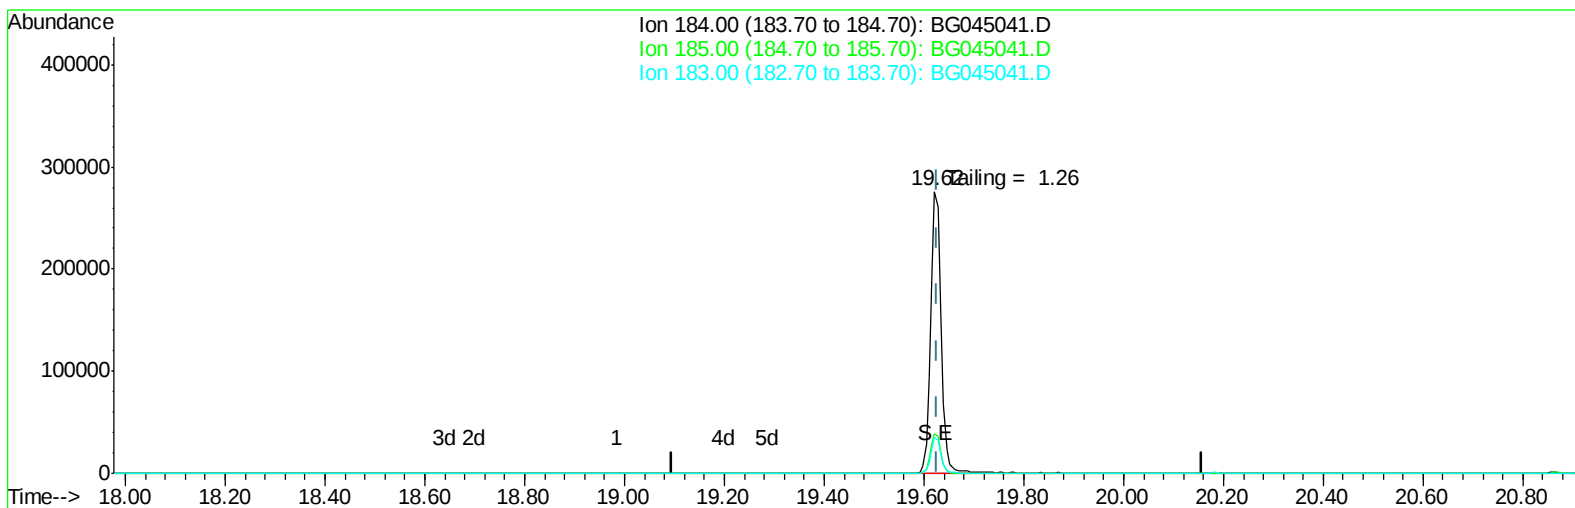

TIC: BG045041.D

(77) Benzidine

18.987min (-0.640) -6.20ng

response 81

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	0.00#
183.00	14.10	0.00#
0.00	0.00	0.00