
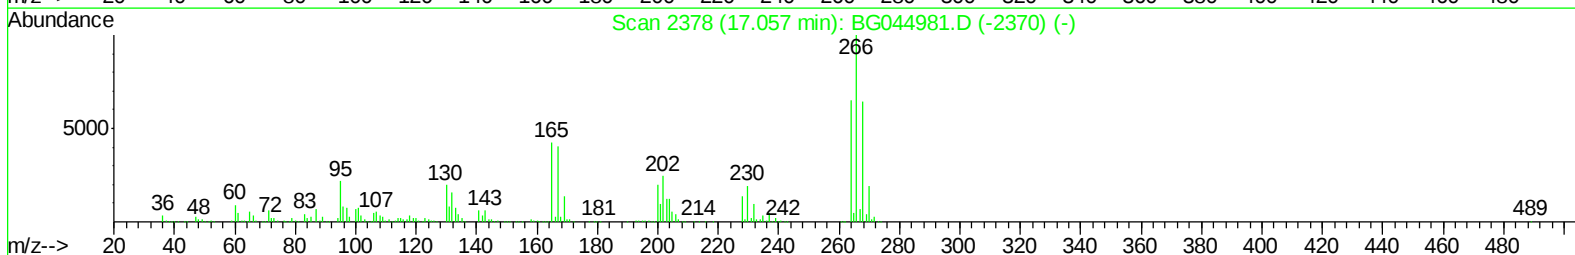
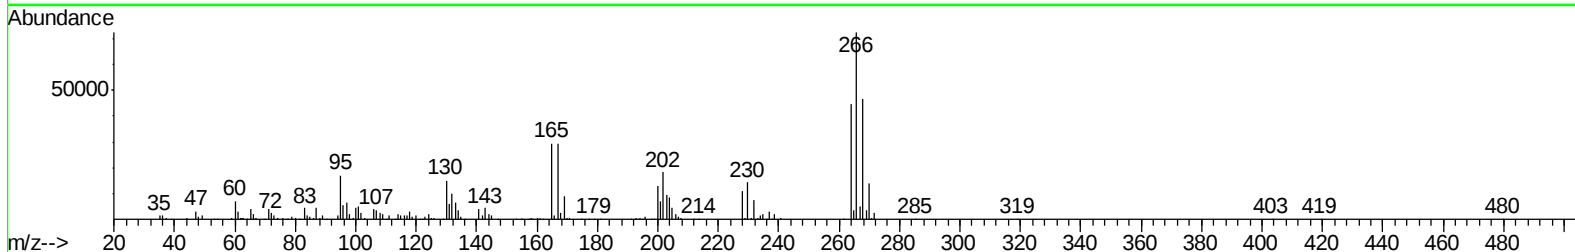


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041720\
Data File : BG045059.D
Acq On : 18 Apr 2020 9:45
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 10:25:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 11:08:29 2020
Response via : Initial Calibration

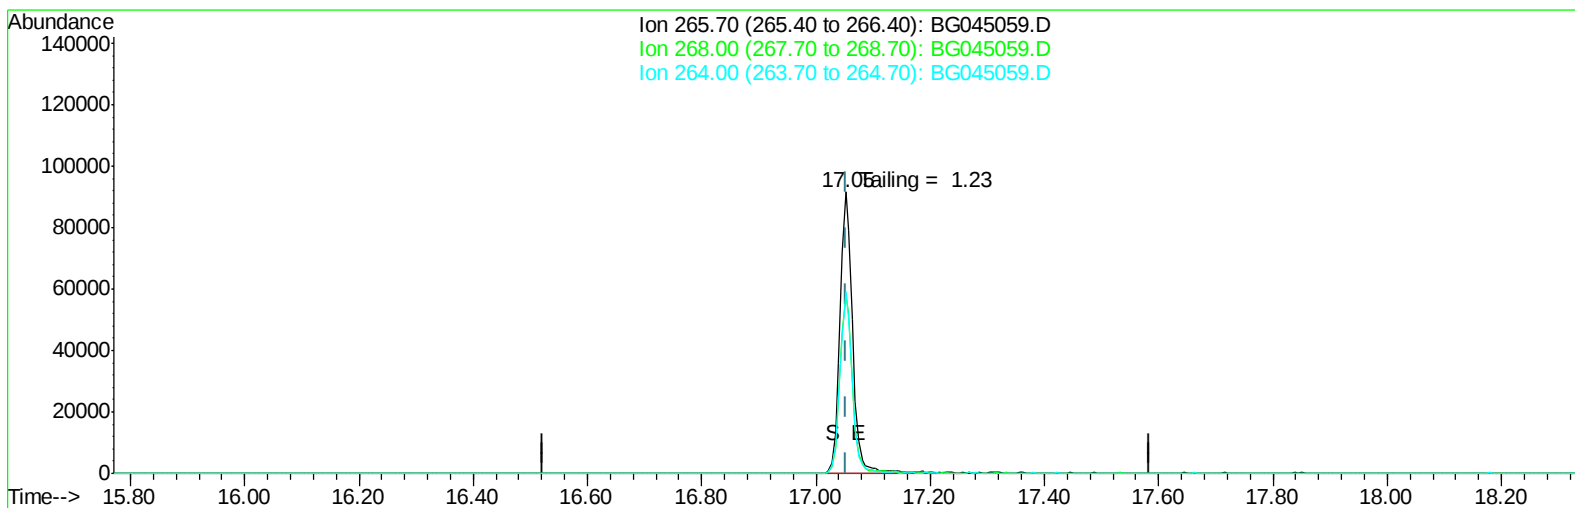

TIC: BG045059.D

(70) Pentachlorophenol (C)




17.051min (-0.002) 37602.84ng

response 138580

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.21
264.00	65.30	64.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041720\
Data File : BG045059.D
Acq On : 18 Apr 2020 9:45
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 10:25:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 11:08:29 2020
Response via : Initial Calibration

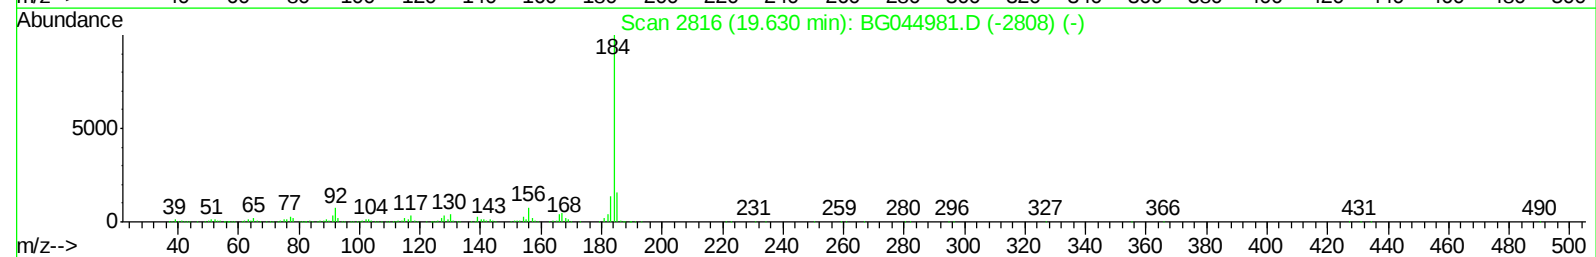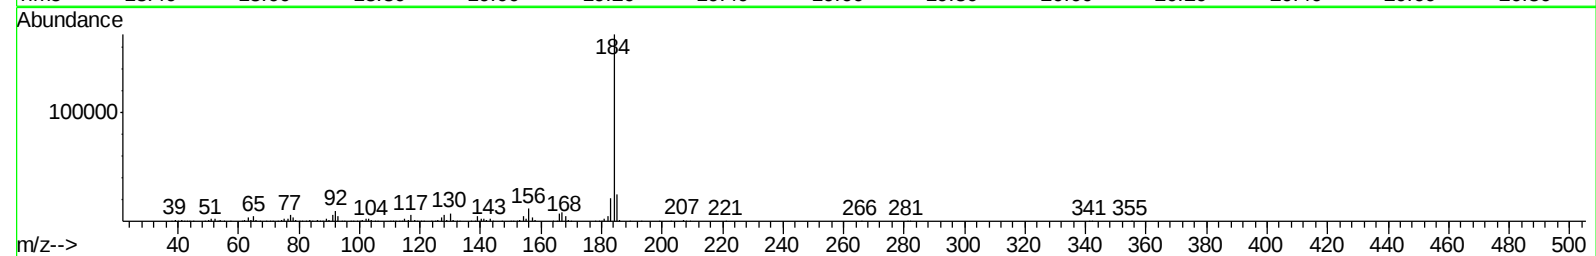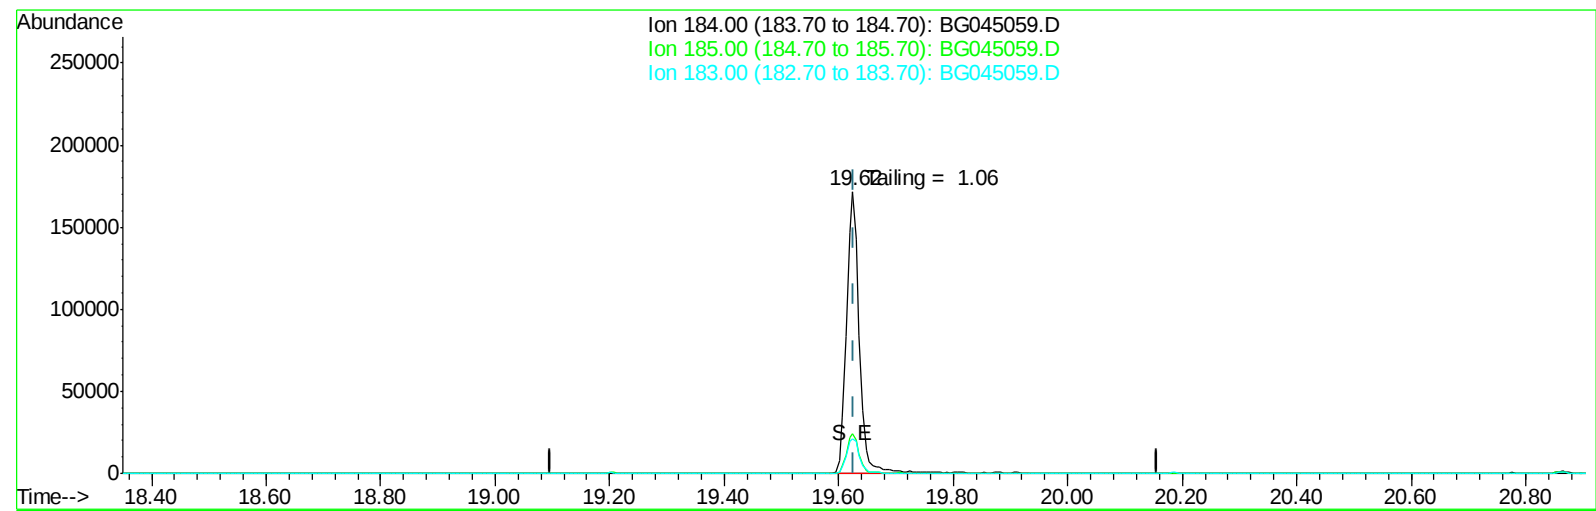

TIC: BG045059.D

(77) Benzidine

19.624min (-0.002) 154144.87ng

response 216942

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.19
183.00	14.10	12.22
0.00	0.00	0.00