
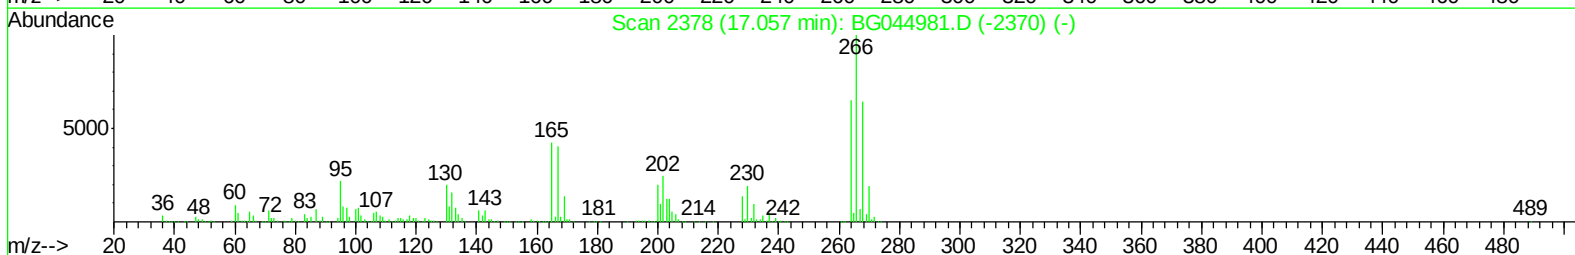
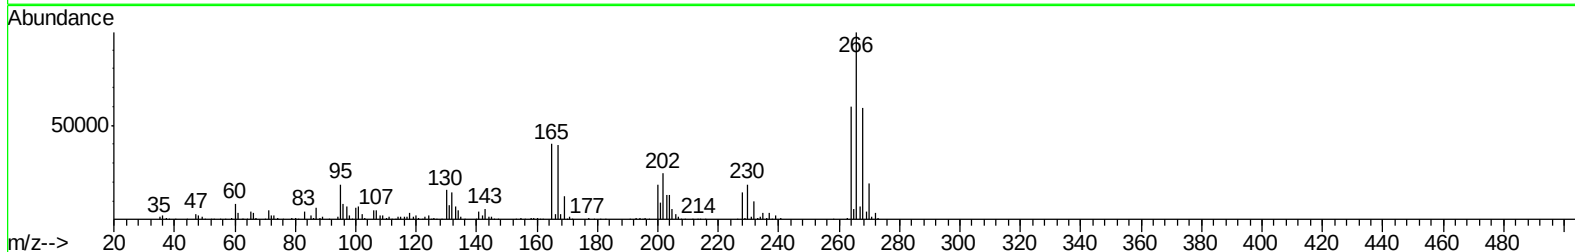


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG041720\
 Data File : BG045072.D
 Acq On : 18 Apr 2020 18:22
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 05:49:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 17 11:08:29 2020
 Response via : Initial Calibration

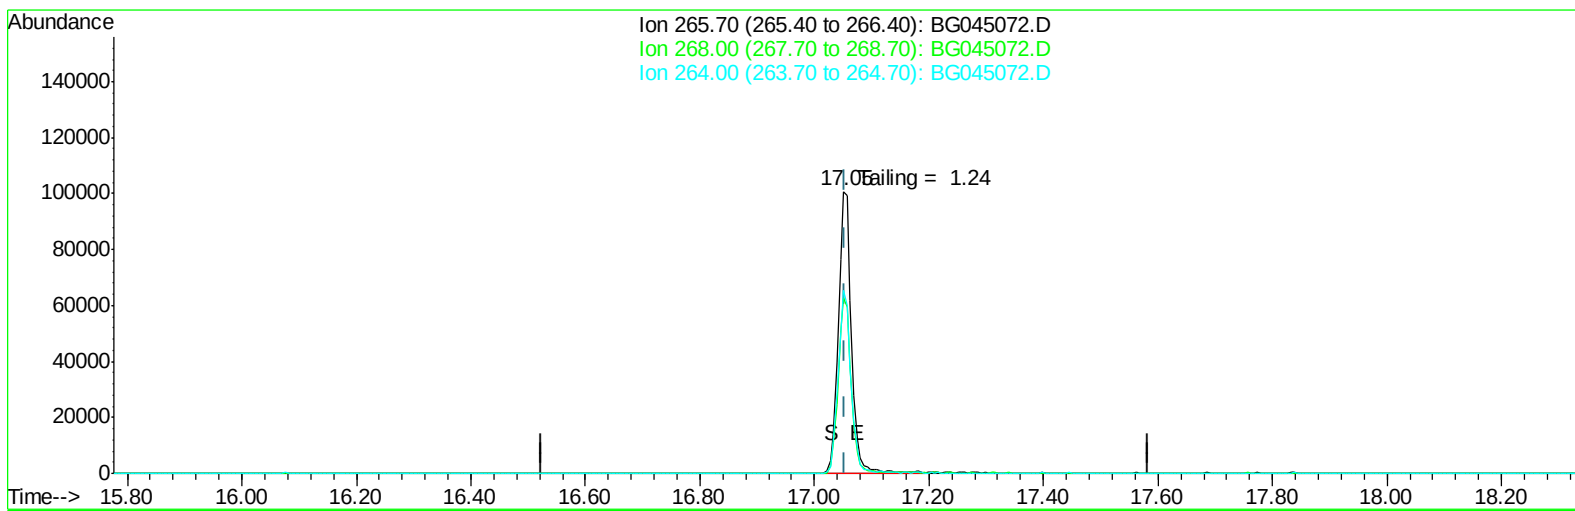

TIC: BG045072.D

(70) Pentachlorophenol (C)




17.051min (-0.003) 274219.57ng

response 159805

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.09
264.00	65.30	64.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG041720\
 Data File : BG045072.D
 Acq On : 18 Apr 2020 18:22
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 05:49:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 17 11:08:29 2020
 Response via : Initial Calibration

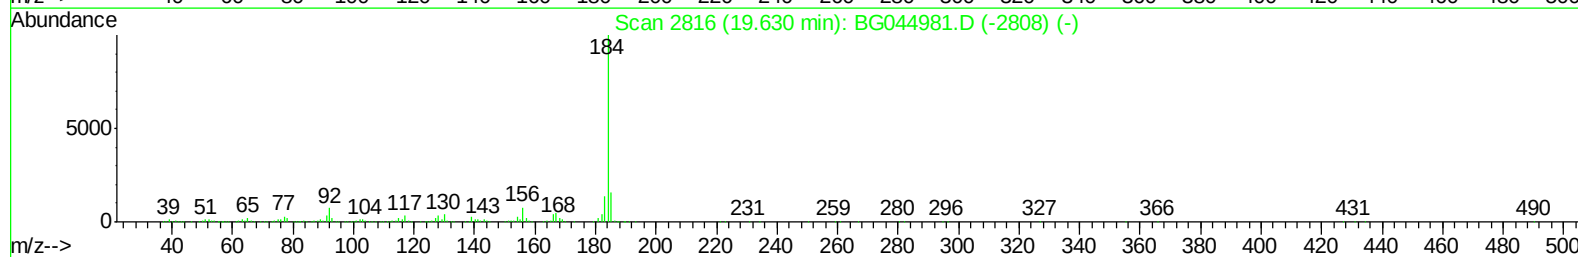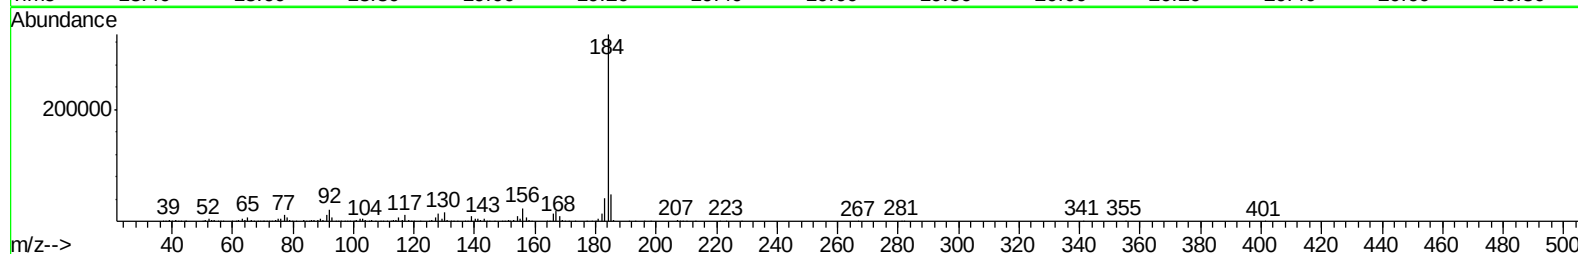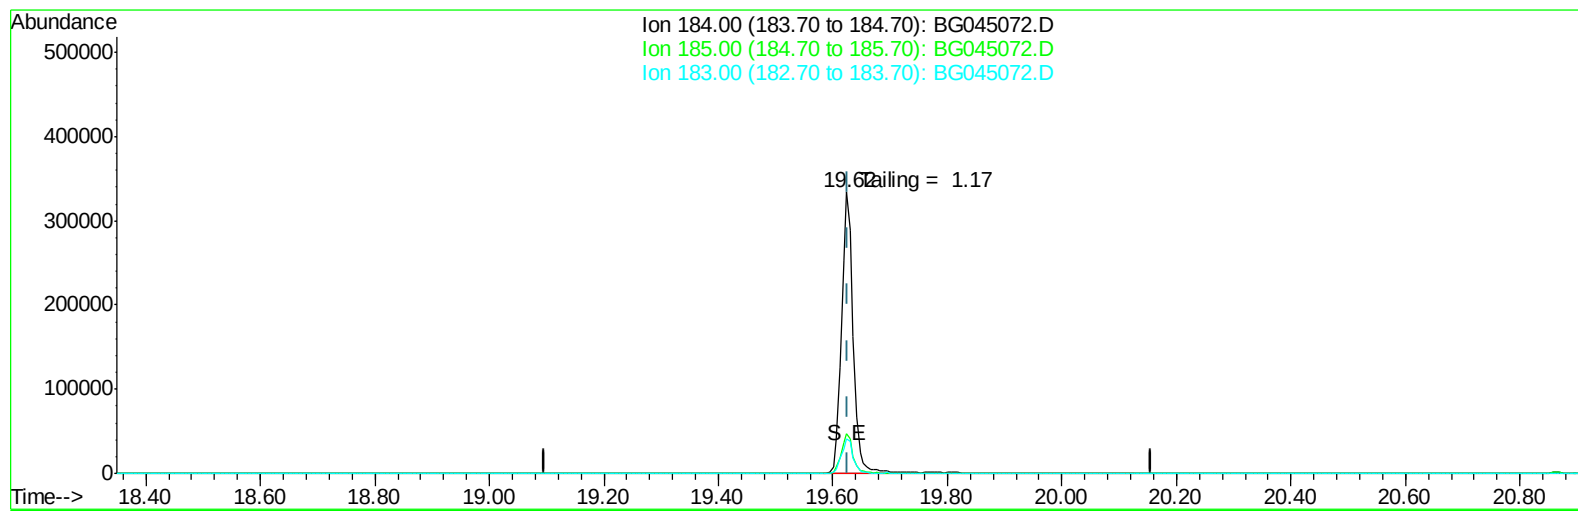

TIC: BG045072.D

(77) Benzidine

19.624min (-0.003) 144255.20ng

response 482182

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.15
183.00	14.10	12.28
0.00	0.00	0.00