


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041720\
 Data File : BG045024.D
 Acq On : 17 Apr 2020 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 11:08:29 2020

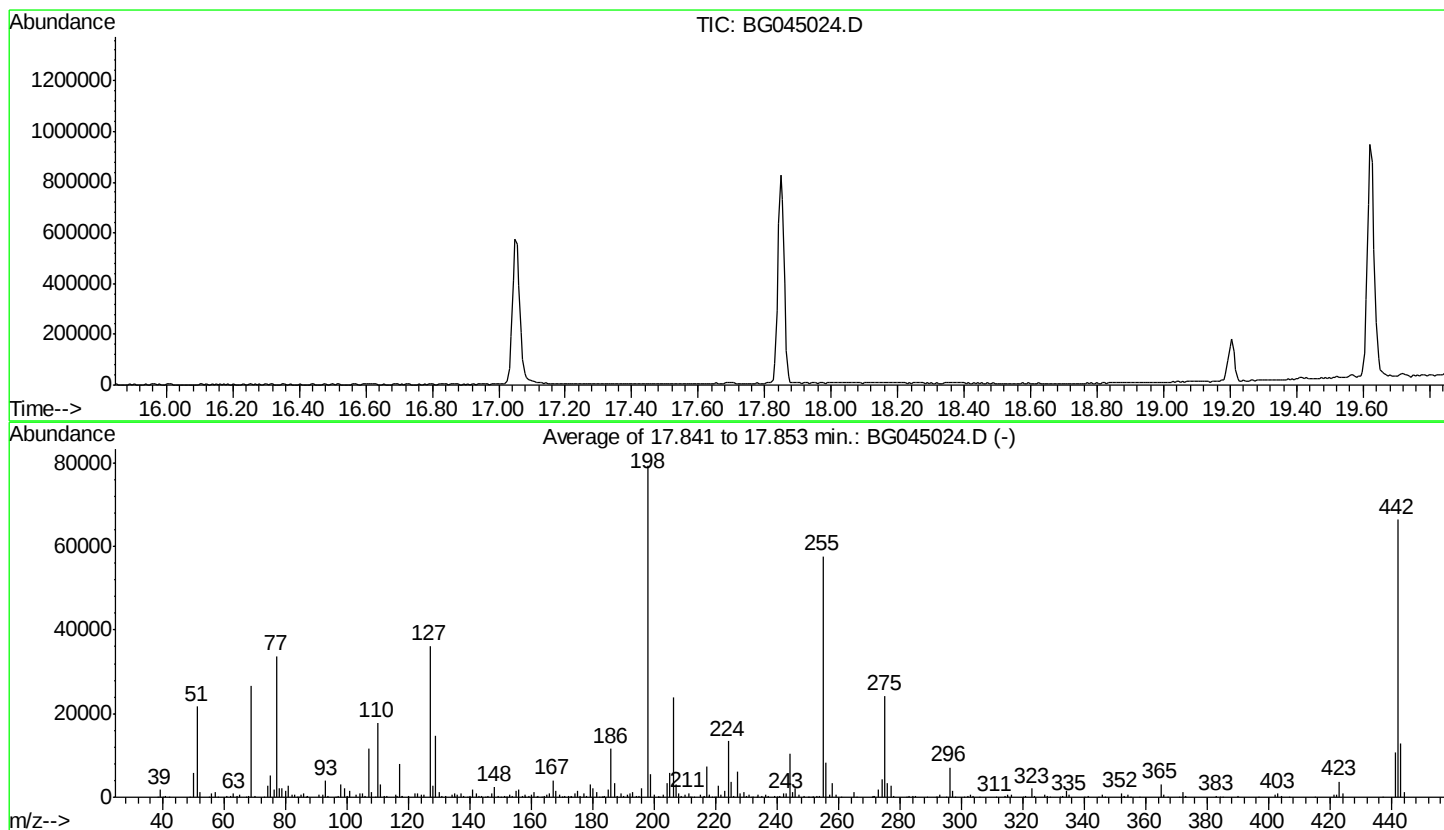

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	21680	PASS
68	69	0.00	2	1.1	305	PASS
69	198	0.00	100	33.6	26633	PASS
70	69	0.00	2	0.7	175	PASS
127	198	10	80	45.7	36240	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79314	PASS
199	198	5	9	6.9	5497	PASS
275	198	10	60	30.5	24224	PASS
365	198	1	100	3.9	3115	PASS
441	198	0.01	100	13.4	10640	PASS
442	198	50	100	83.7	66362	PASS
443	442	15	24	19.3	12817	PASS