


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041720\
 Data File : BG045041.D
 Acq On : 17 Apr 2020 21:07
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 11:08:29 2020

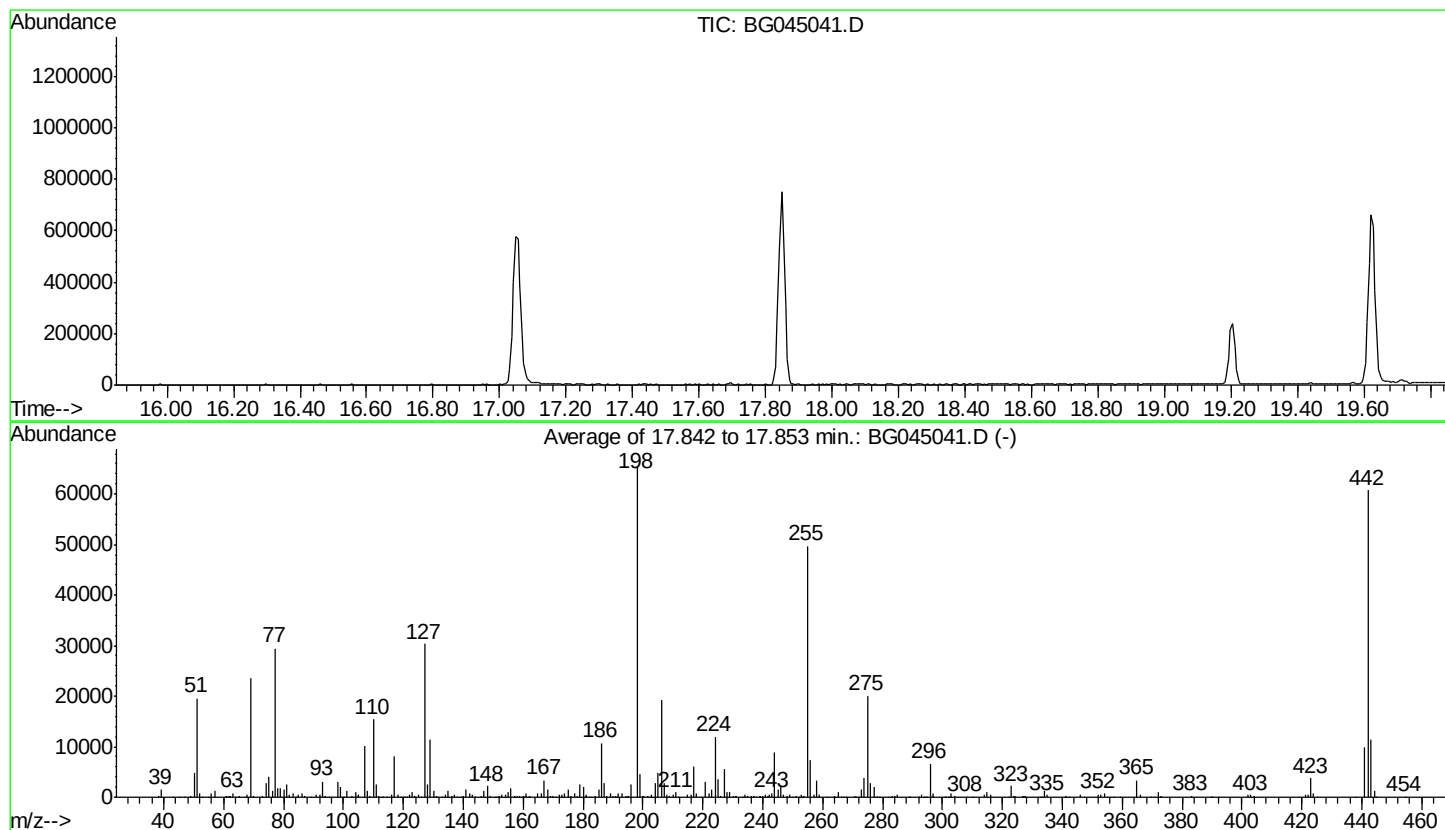

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	19520	PASS
68	69	0.00	2	1.8	418	PASS
69	198	0.00	100	36.0	23589	PASS
70	69	0.00	2	1.2	277	PASS
127	198	10	80	46.3	30376	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65608	PASS
199	198	5	9	6.9	4559	PASS
275	198	10	60	30.7	20109	PASS
365	198	1	100	5.1	3356	PASS
441	198	0.01	100	14.9	9801	PASS
442	198	50	100	92.5	60696	PASS
443	442	15	24	19.0	11509	PASS