


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041720\
 Data File : BG045072.D
 Acq On : 18 Apr 2020 18:22
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 11:08:29 2020

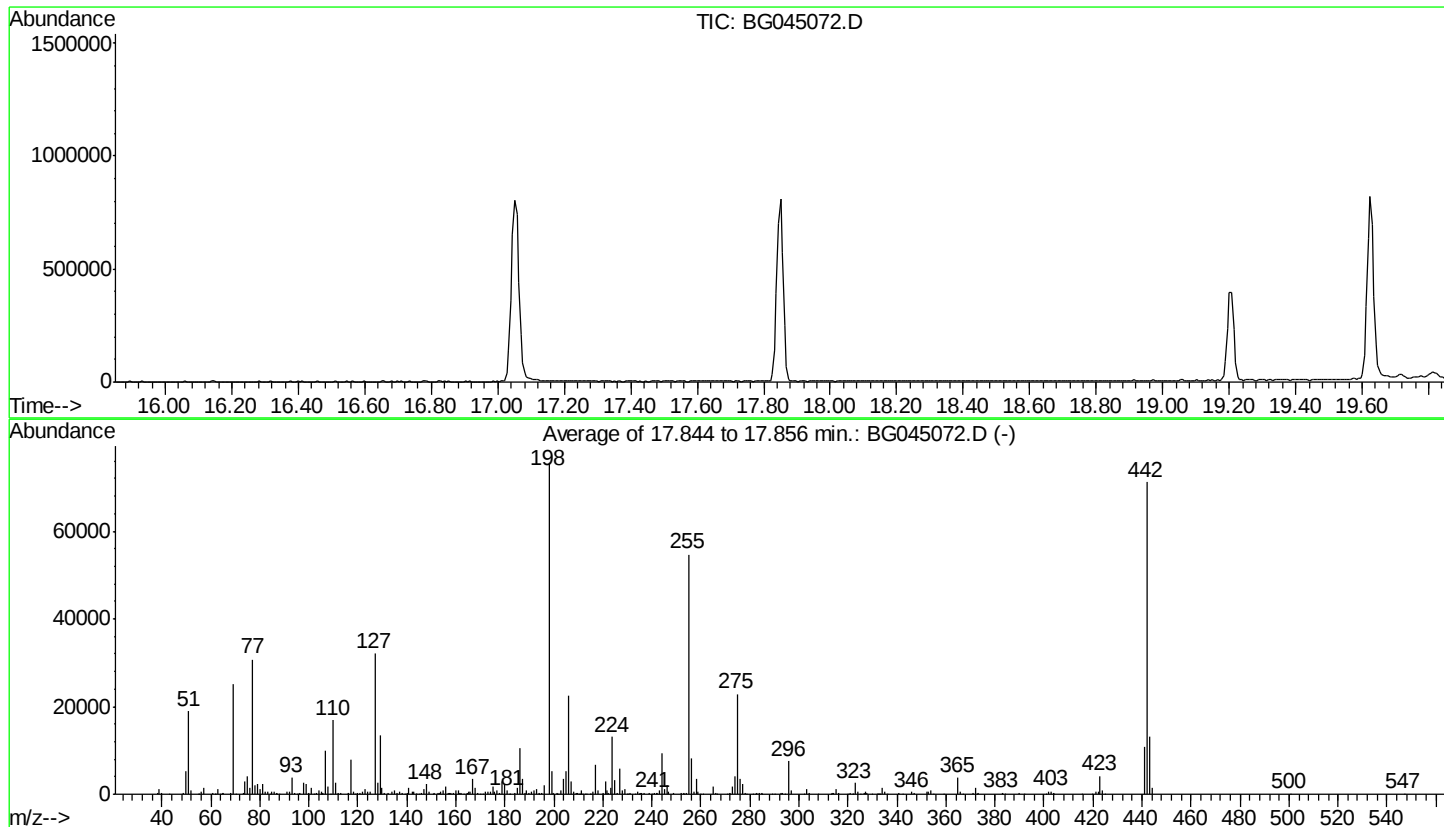

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	18934	PASS
68	69	0.00	2	1.0	245	PASS
69	198	0.00	100	33.2	25117	PASS
70	69	0.00	2	0.5	124	PASS
127	198	10	80	42.3	31992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75634	PASS
199	198	5	9	7.1	5374	PASS
275	198	10	60	30.2	22808	PASS
365	198	1	100	5.0	3751	PASS
441	198	0.01	100	14.2	10777	PASS
442	198	50	100	94.2	71229	PASS
443	442	15	24	18.5	13191	PASS