

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041919\
 Data File : BG040559.D
 Acq On : 19 Apr 2019 13:18
 Operator : JU/SJ
 Sample : PB119042BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB119042BL

Quant Time: Apr 20 01:54:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 13 00:33:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	40756	20.00	ng	-0.01
21) Naphthalene-d8	10.85	136	160454	20.00	ng	-0.01
39) Acenaphthene-d10	14.66	164	102159	20.00	ng	-0.01
64) Phenanthrene-d10	17.41	188	318507	20.00	ng	-0.01
76) Chrysene-d12	21.68	240	329488	20.00	ng	-0.02
87) Perylene-d12	24.95	264	353411	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	286281	116.77	ng	-0.01
7) Phenol-d6	7.19	99	390277	115.19	ng	-0.01
23) Nitrobenzene-d5	9.21	82	222663	73.76	ng	-0.01
42) 2,4,6-Tribromophenol	16.16	330	153290	138.84	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	690739	100.19	ng	-0.01
79) Terphenyl-d14	20.01	244	1518556	103.68	ng	-0.01


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041919\
Data File : BG040559.D
Acq On : 19 Apr 2019 13:18
Operator : JU/SJ
Sample : PB119042BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB119042BL

Quant Time: Apr 20 01:54:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration




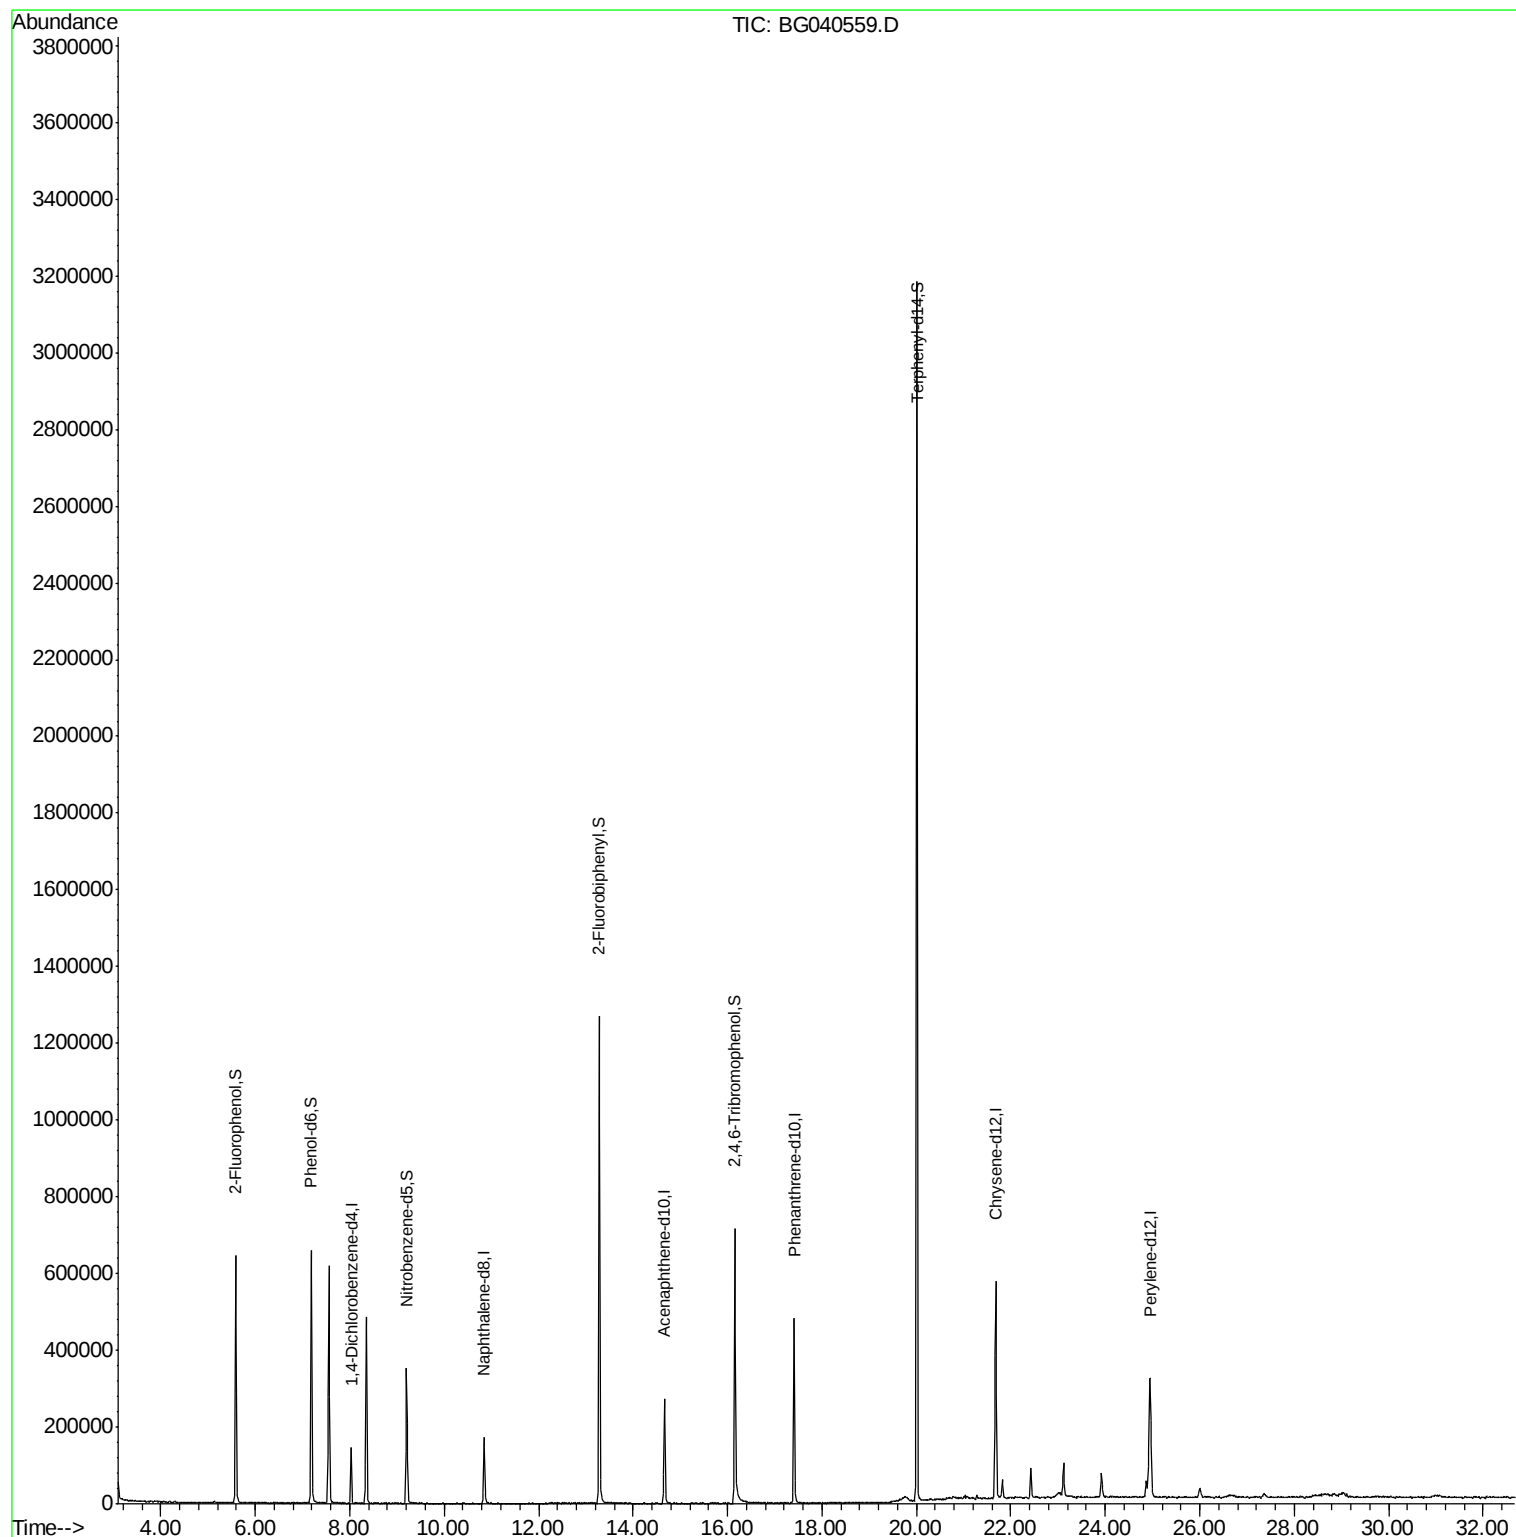




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.03 min Scan# 841
 Delta R.T. -0.01 min
 Lab File: BG040559.D
 Acq: 19 Apr 2019 13:18




Instrument :
 BNA_G
 ClientSampleID :
 PB119042BL


Tgt Ion:152 Resp: 40756
 Ion Ratio Lower Upper
 152 100
 150 160.1 123.7 185.5
 115 58.8 46.9 70.3

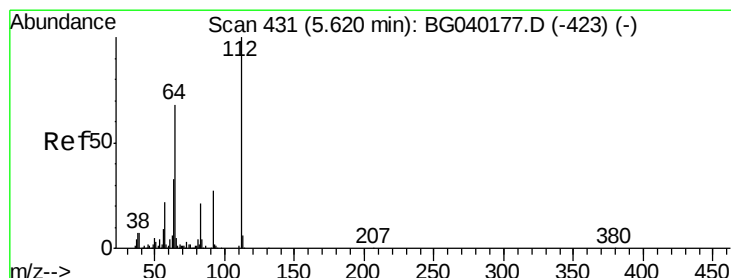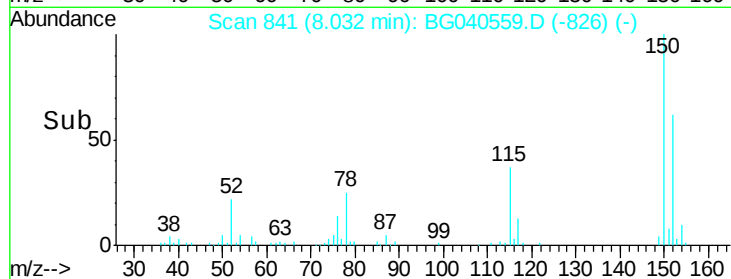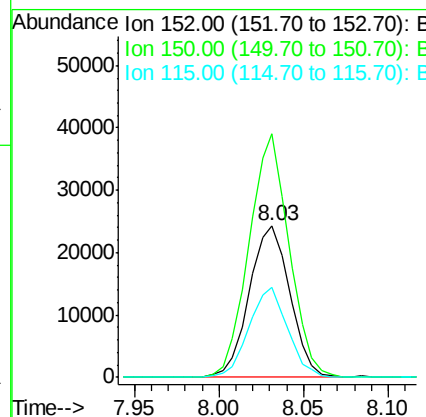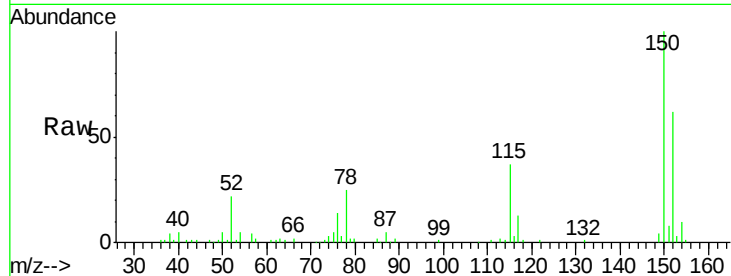

#5
 2-Fluorophenol
 Concen: 116.772 ng
 RT: 5.59 min Scan# 425
 Delta R.T. -0.01 min
 Lab File: BG040559.D
 Acq: 19 Apr 2019 13:18

Tgt Ion:112 Resp: 286281
 Ion Ratio Lower Upper
 112 100
 64 68.3 54.2 81.2
 63 34.0 26.4 39.6

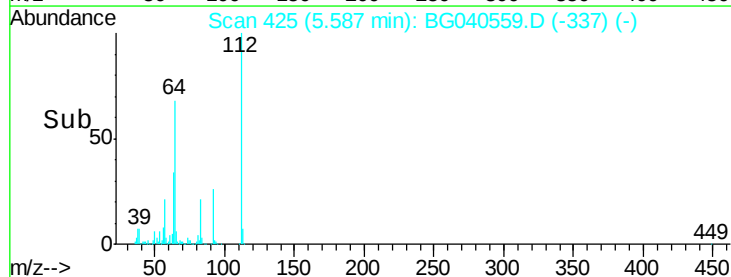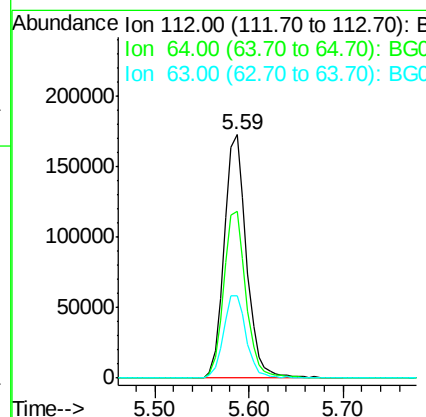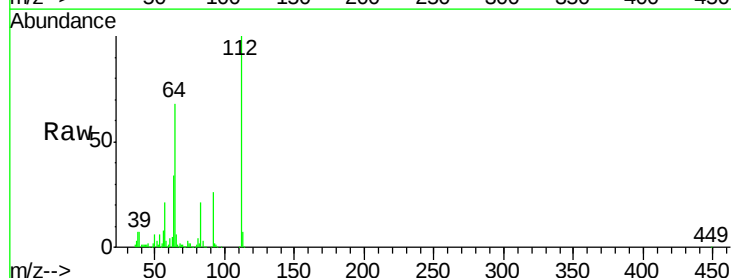

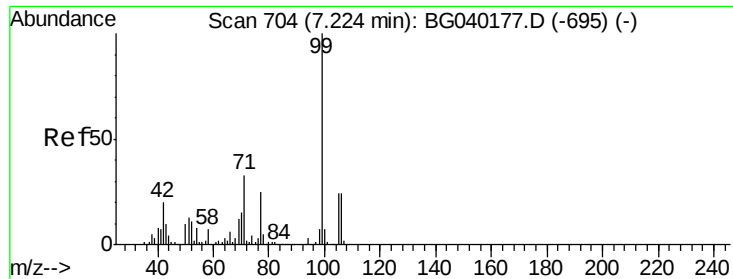

#7

Phenol-d6

Concen: 115.188 ng

RT: 7.19 min Scan# 697

Delta R.T. -0.01 min

Lab File: BG040559.D

Acq: 19 Apr 2019 13:18

Instrument :

BNA_G

ClientSampleId :

PB119042BL


Tgt Ion: 99 Resp: 390277

Ion Ratio Lower Upper




99 100

42 20.1 16.2 24.2

71 34.3 26.8 40.2

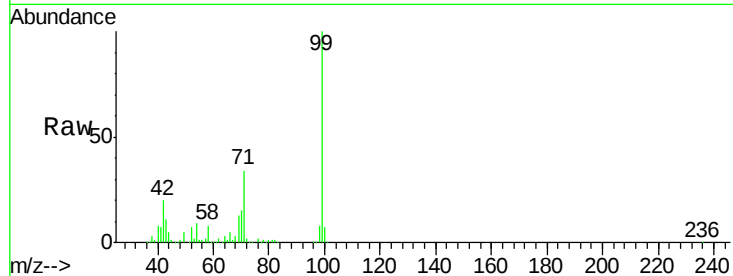

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

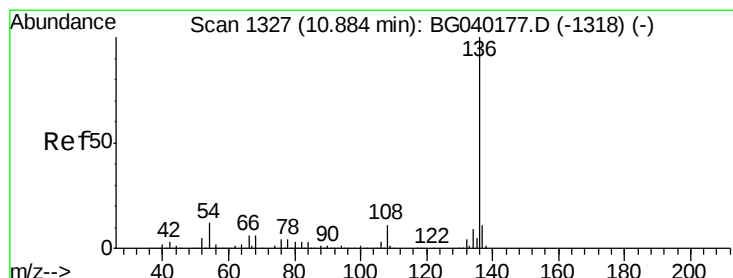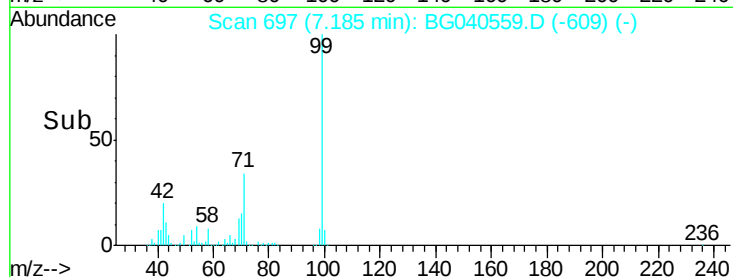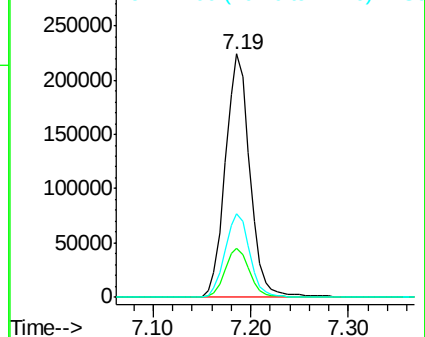

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BG040559.D

Acq: 19 Apr 2019 13:18

Tgt Ion: 136 Resp: 160454


Ion Ratio Lower Upper

136 100



137 10.6 8.9 13.3

54 9.3 9.6 14.4#

68 6.4 5.1 7.7

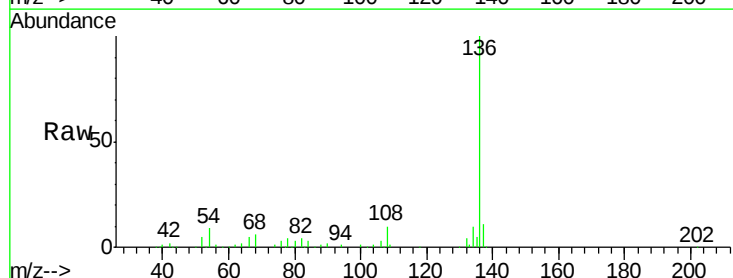

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

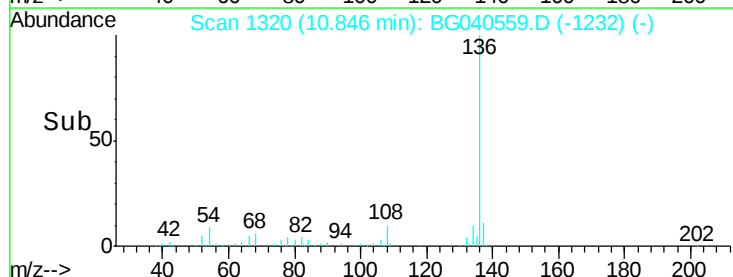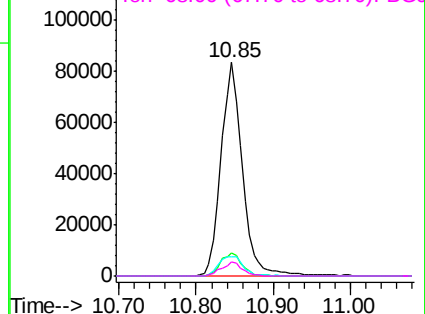







#23
 Nitrobenzene-d5
 Concen: 73.761 ng
 RT: 9.21 min Scan# 1041
 Delta R.T. -0.01 min
 Lab File: BG040559.D
 Acq: 19 Apr 2019 13:18

Instrument :
 BNA_G
 ClientSampleId :
 PB119042BL

Tgt Ion: 82 Resp: 222663
 Ion Ratio Lower Upper
 82 100
 128 43.5 35.8 53.8
 54 57.1 46.2 69.2

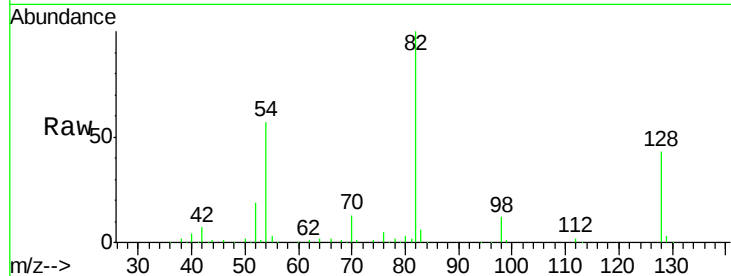


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

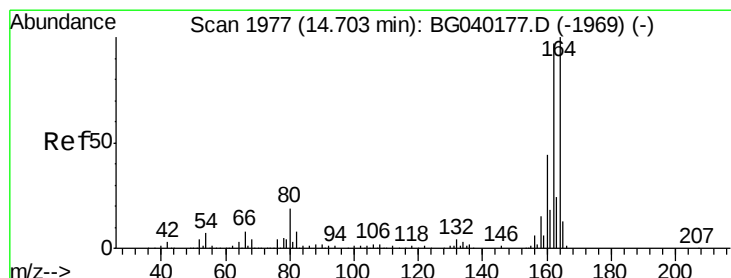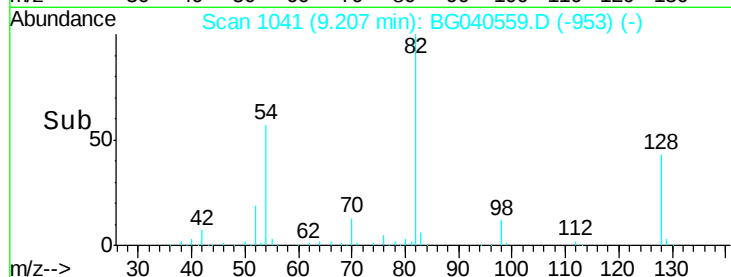
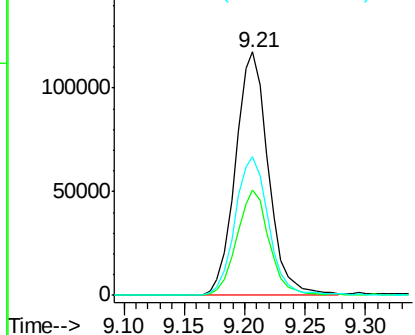


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1970
 Delta R.T. -0.01 min
 Lab File: BG040559.D
 Acq: 19 Apr 2019 13:18

Tgt Ion: 164 Resp: 102159
 Ion Ratio Lower Upper
 164 100
 162 102.5 77.4 116.2
 160 44.7 35.3 52.9

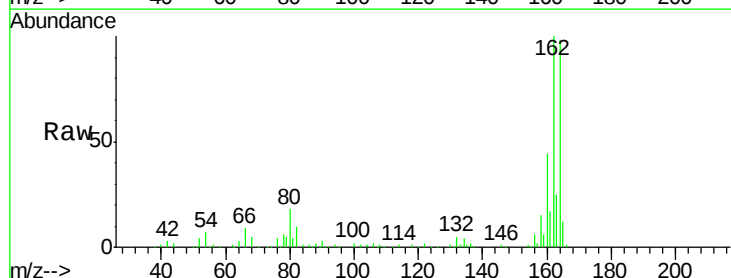

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



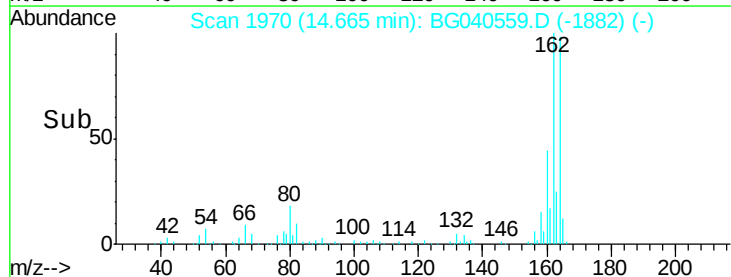
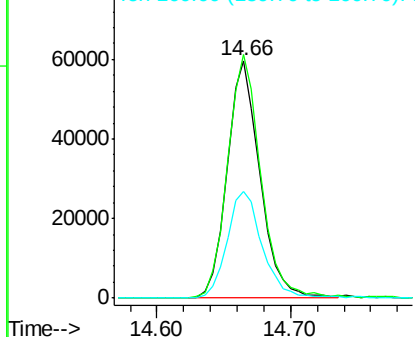




#42
 2,4,6-Tribromophenol
 Concen: 138.841 ng
 RT: 16.16 min Scan# 2224
 Delta R.T. -0.01 min
 Lab File: BG040559.D
 Acq: 19 Apr 2019 13:18




Instrument :
 BNA_G
 ClientSampleId :
 PB119042BL


Tgt Ion:330 Resp: 153290
 Ion Ratio Lower Upper
 330 100
 332 92.6 76.6 115.0
 141 39.6 32.6 48.8

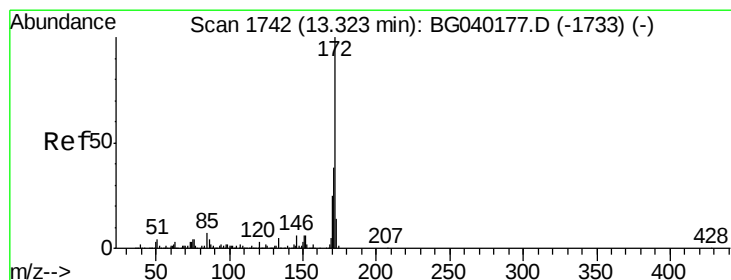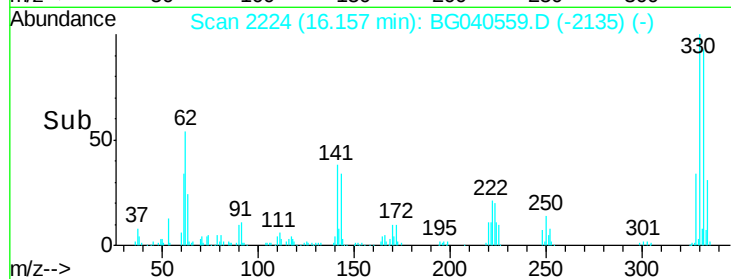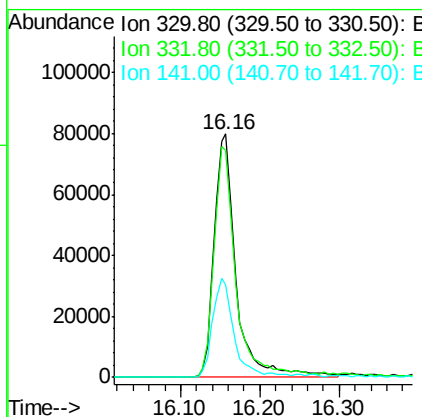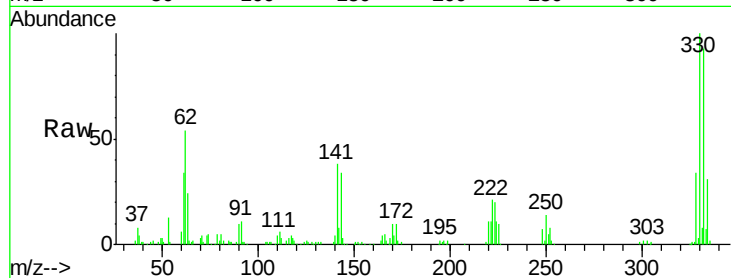

#45
 2-Fluorobiphenyl
 Concen: 100.188 ng
 RT: 13.28 min Scan# 1735
 Delta R.T. -0.01 min
 Lab File: BG040559.D
 Acq: 19 Apr 2019 13:18

Tgt Ion:172 Resp: 690739
 Ion Ratio Lower Upper
 172 100
 171 36.2 30.5 45.7
 170 23.9 20.1 30.1


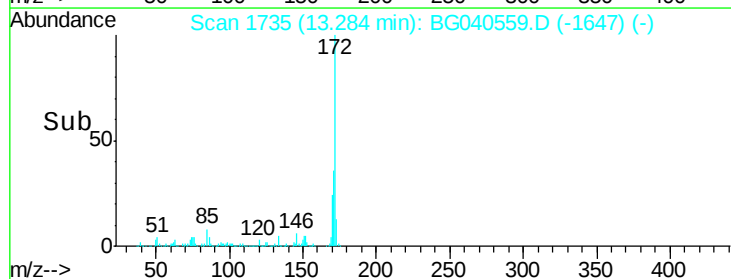
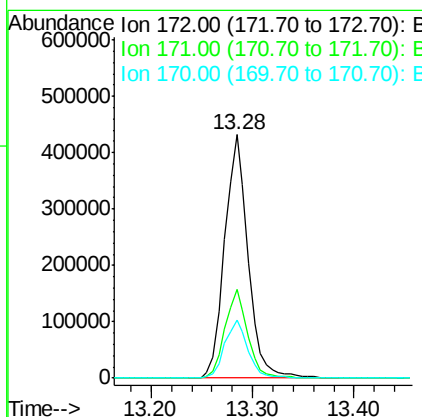
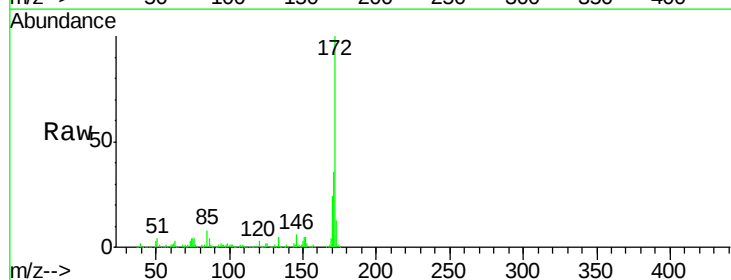


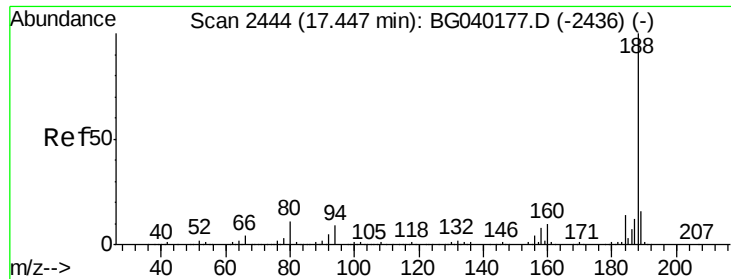

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2437
Delta R.T. -0.01 min
Lab File: BG040559.D
Acq: 19 Apr 2019 13:18




Instrument :
BNA_G
ClientSampleId :
PB119042BL

Tgt Ion:188 Resp: 318507
Ion Ratio Lower Upper
188 100
94 9.1 7.0 10.4
80 10.9 8.6 13.0

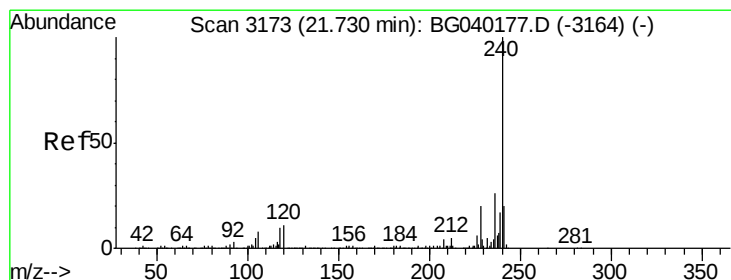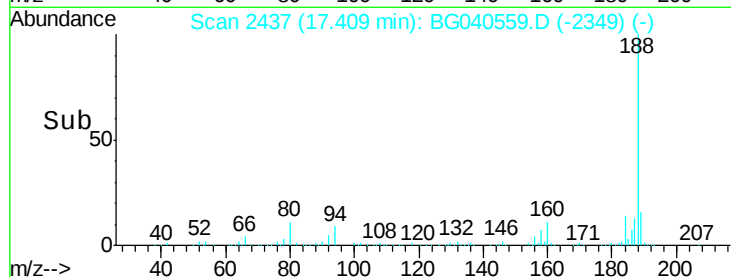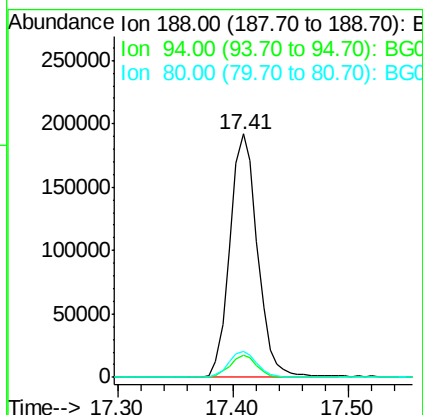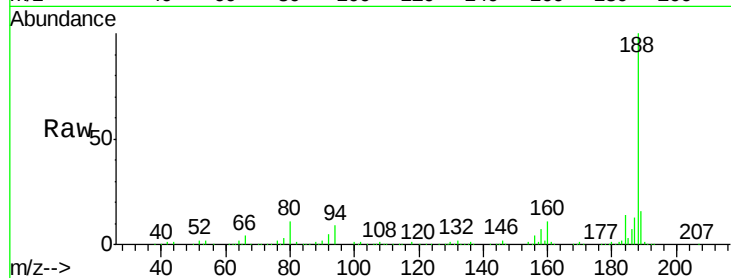

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.68 min Scan# 3164
Delta R.T. -0.02 min
Lab File: BG040559.D
Acq: 19 Apr 2019 13:18

Tgt Ion:240 Resp: 329488
Ion Ratio Lower Upper
240 100
120 10.1 8.4 12.6
236 25.4 20.8 31.2

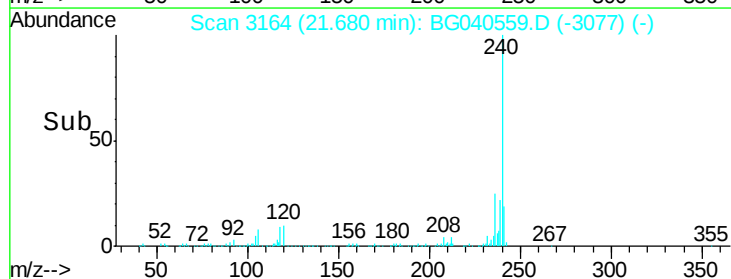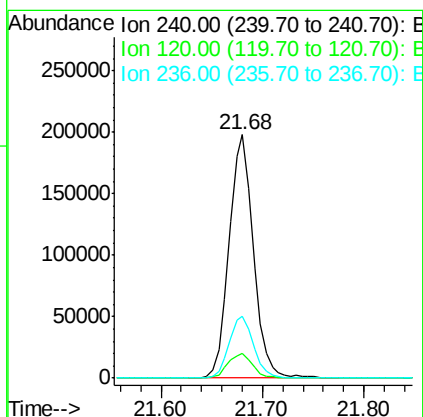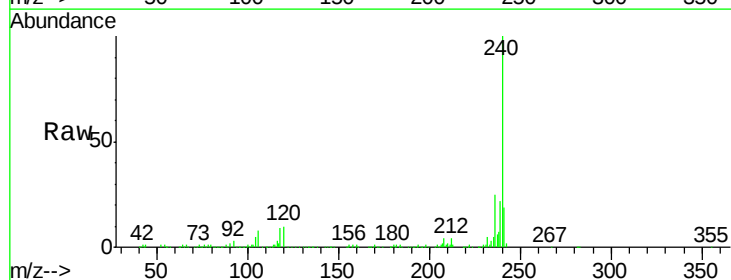



#79

Terphenyl-d14

Concen: 103.683 ng

RT: 20.01 min Scan# 2880

Delta R.T. -0.01 min

Lab File: BG040559.D

Acq: 19 Apr 2019 13:18

Instrument :

BNA_G

ClientSampleId :

PB119042BL


Tgt Ion:244 Resp: 1518556

Ion Ratio Lower Upper

244 100

212 8.6 7.0 10.6




122 11.9 8.5 12.7

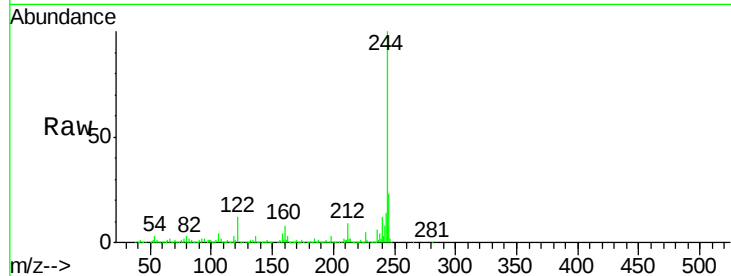

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

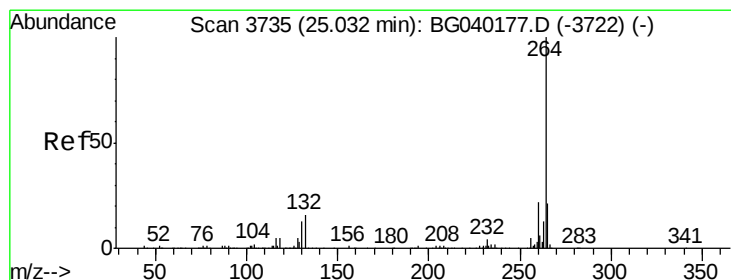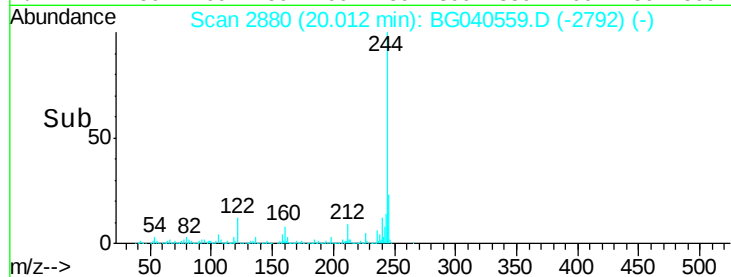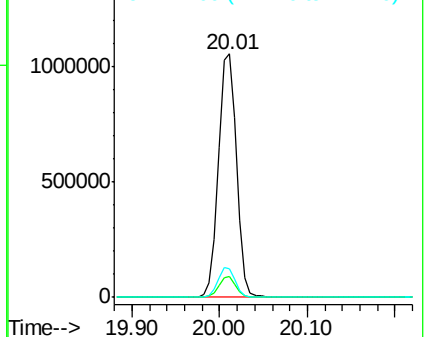

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.95 min Scan# 3720

Delta R.T. -0.02 min

Lab File: BG040559.D

Acq: 19 Apr 2019 13:18


Tgt Ion:264 Resp: 353411

Ion Ratio Lower Upper

264 100

260 22.9 17.9 26.9

265 22.5 16.8 25.2

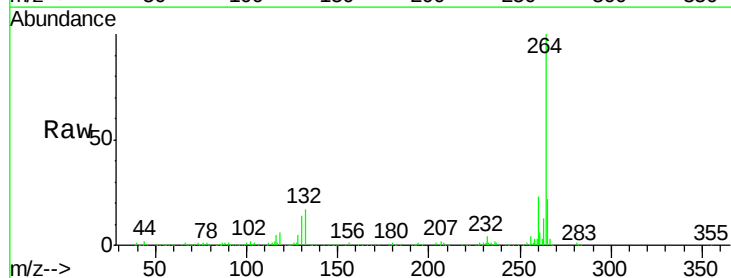

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

