


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041919\
 Data File : BG040556.D
 Acq On : 19 Apr 2019 11:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Apr 13 00:33:11 2019

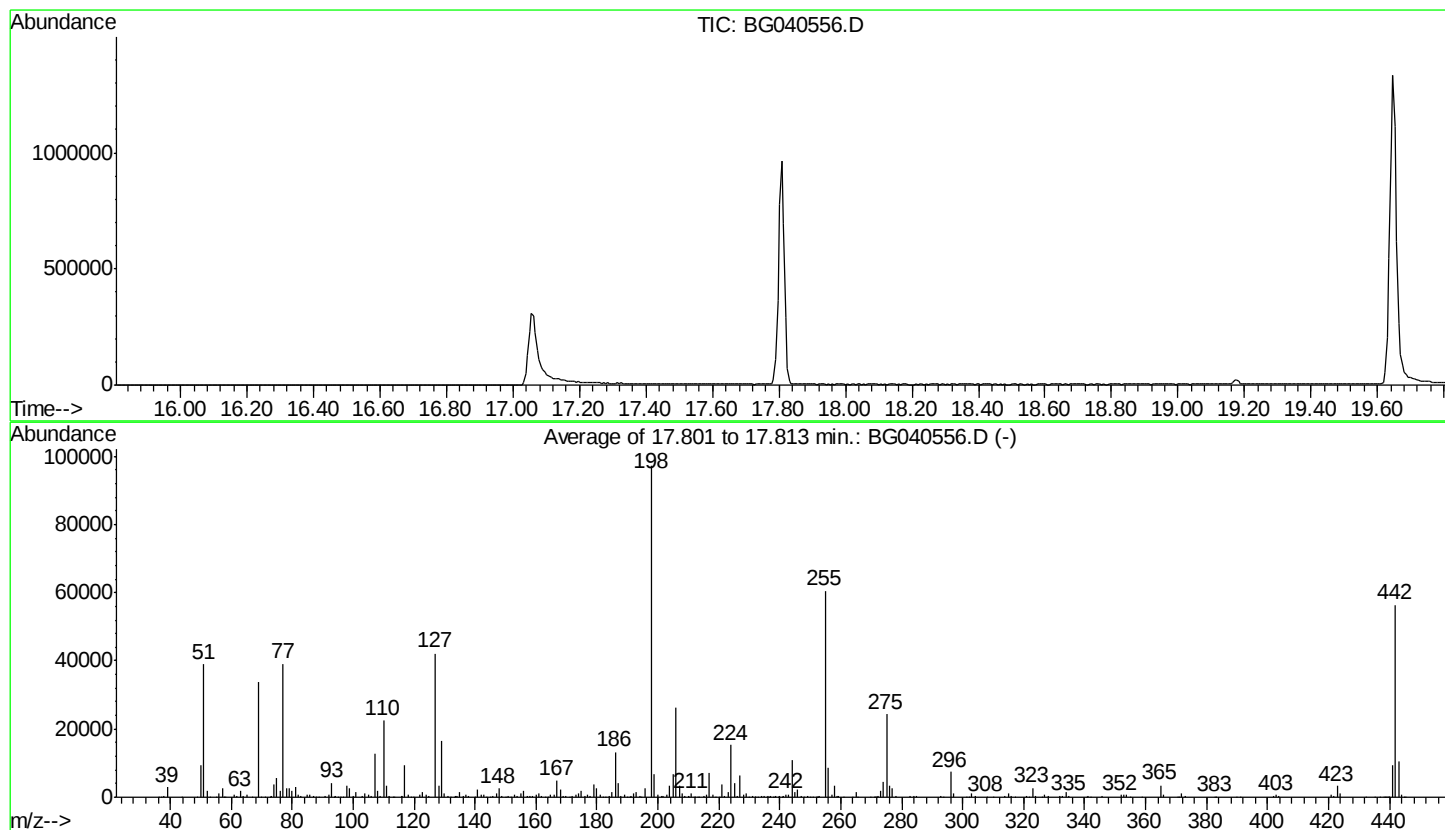

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	38968	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.6	33634	PASS
70	69	0.00	2	0.4	133	PASS
127	198	10	80	43.4	42218	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97240	PASS
199	198	5	9	6.8	6614	PASS
275	198	10	60	25.0	24320	PASS
365	198	1	100	3.7	3563	PASS
441	198	0.01	100	9.6	9324	PASS
442	198	50	100	58.0	56360	PASS
443	442	15	24	18.9	10628	PASS