
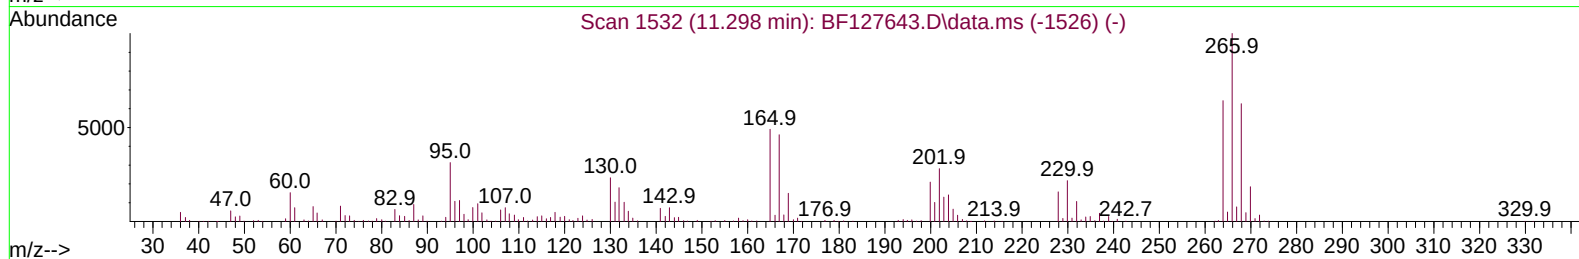
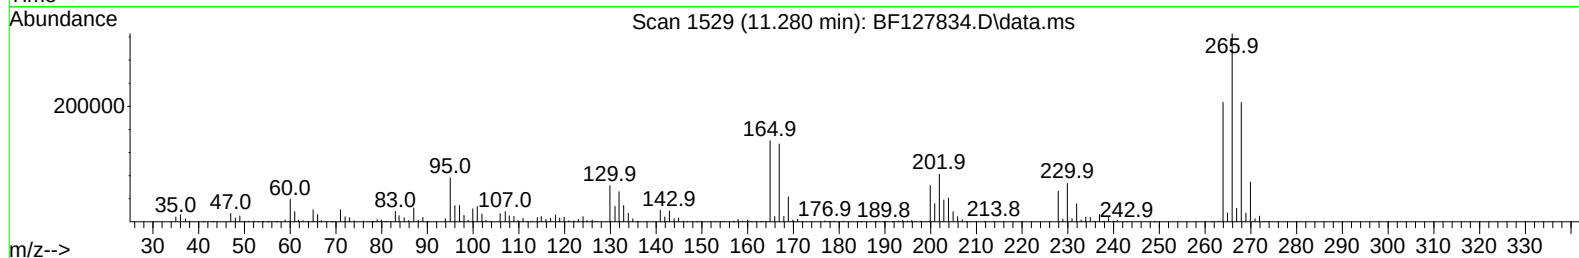


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041922\  
 Data File : BF127834.D  
 Acq On : 19 Apr 2022 10:37  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 13:33:16 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF041922.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Apr 19 13:24:29 2022  
 Response via : Initial Calibration

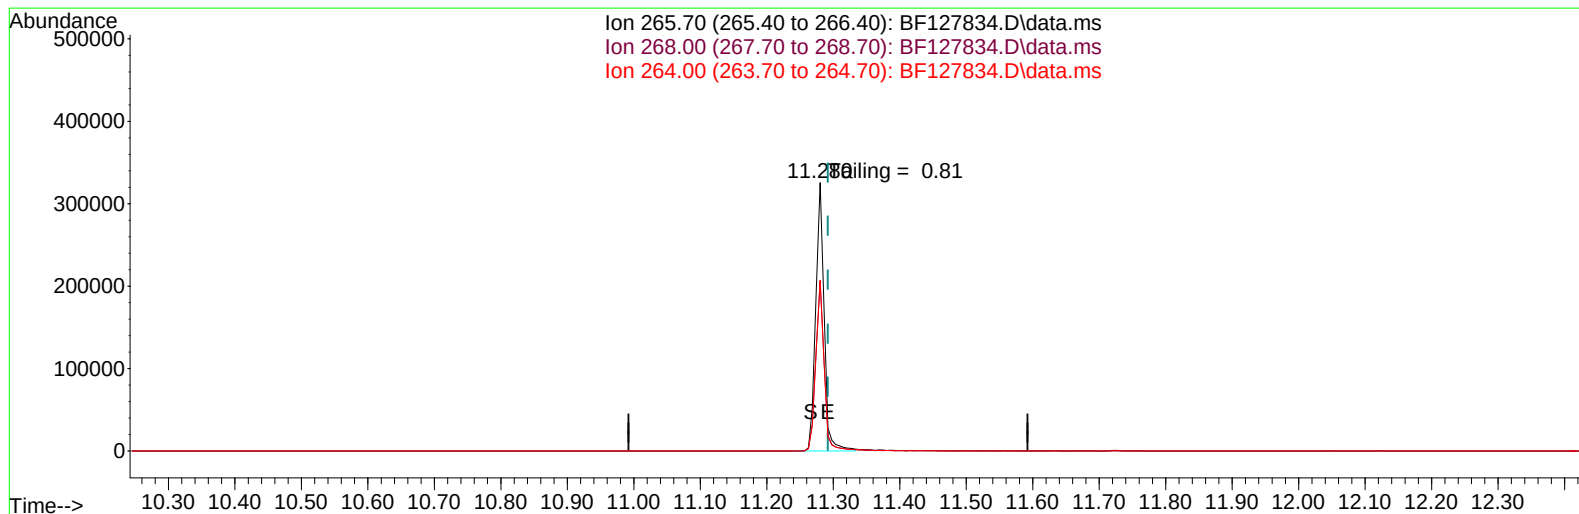

TIC: BF127834.D\data.ms

**(70) Pentachlorophenol (C)**

11.280min (-0.012) 228315.74 ng

response 293075

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 63.38  |
| 264.00 | 60.60  | 63.54  |
| 0.00   | 0.00   | 0.00   |