

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
 Data File : BG053204.D
 Acq On : 19 Apr 2022 20:33
 Operator : CG/JU
 Sample : N2452-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-15-1-3

Quant Time: Apr 20 05:43:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	32676	20.000	ng	0.00
21) Naphthalene-d8	10.936	136	133010	20.000	ng	# 0.00
39) Acenaphthene-d10	14.742	164	93319	20.000	ng	0.00
64) Phenanthrene-d10	17.486	188	176457	20.000	ng	0.00
76) Chrysene-d12	21.780	240	170864	20.000	ng	0.00
86) Perylene-d12	25.093	264	177632	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.684	112	166557	87.376	ng	0.00
7) Phenol-d6	7.276	99	250292	85.145	ng	0.00
23) Nitrobenzene-d5	9.279	82	185198	56.535	ng	0.00
42) 2,4,6-Tribromophenol	16.229	330	110672	74.543	ng	0.00
45) 2-Fluorobiphenyl	13.368	172	406929	60.129	ng	0.00
79) Terphenyl-d14	20.094	244	563713	55.720	ng	0.00
Target Compounds						
						Qvalue
18) Hexachloroethane	9.238	117	1906	2.085	ng	# 1
32) Benzoic acid	10.149	122	274	3.833	ng	# 78
37) 2-Methylnaphthalene	12.581	142	20708	3.944	ng	# 85
38) 1-Methylnaphthalene	12.798	142	27531	5.371	ng	# 86
56) 4-Nitrophenol	14.948	139	3980	3.169	ng	# 37
66) n-Nitrosodiphenylamine	15.994	169	15014	2.959	ng	# 46
71) Phenanthrene	17.527	178	37447	3.885	ng	# 87
83) Chrysene	21.821	228	37649	3.472	ng	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
Data File : BG053204.D
Acq On : 19 Apr 2022 20:33
Operator : CG/JU
Sample : N2452-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-15-1-3


Quant Time: Apr 20 05:43:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

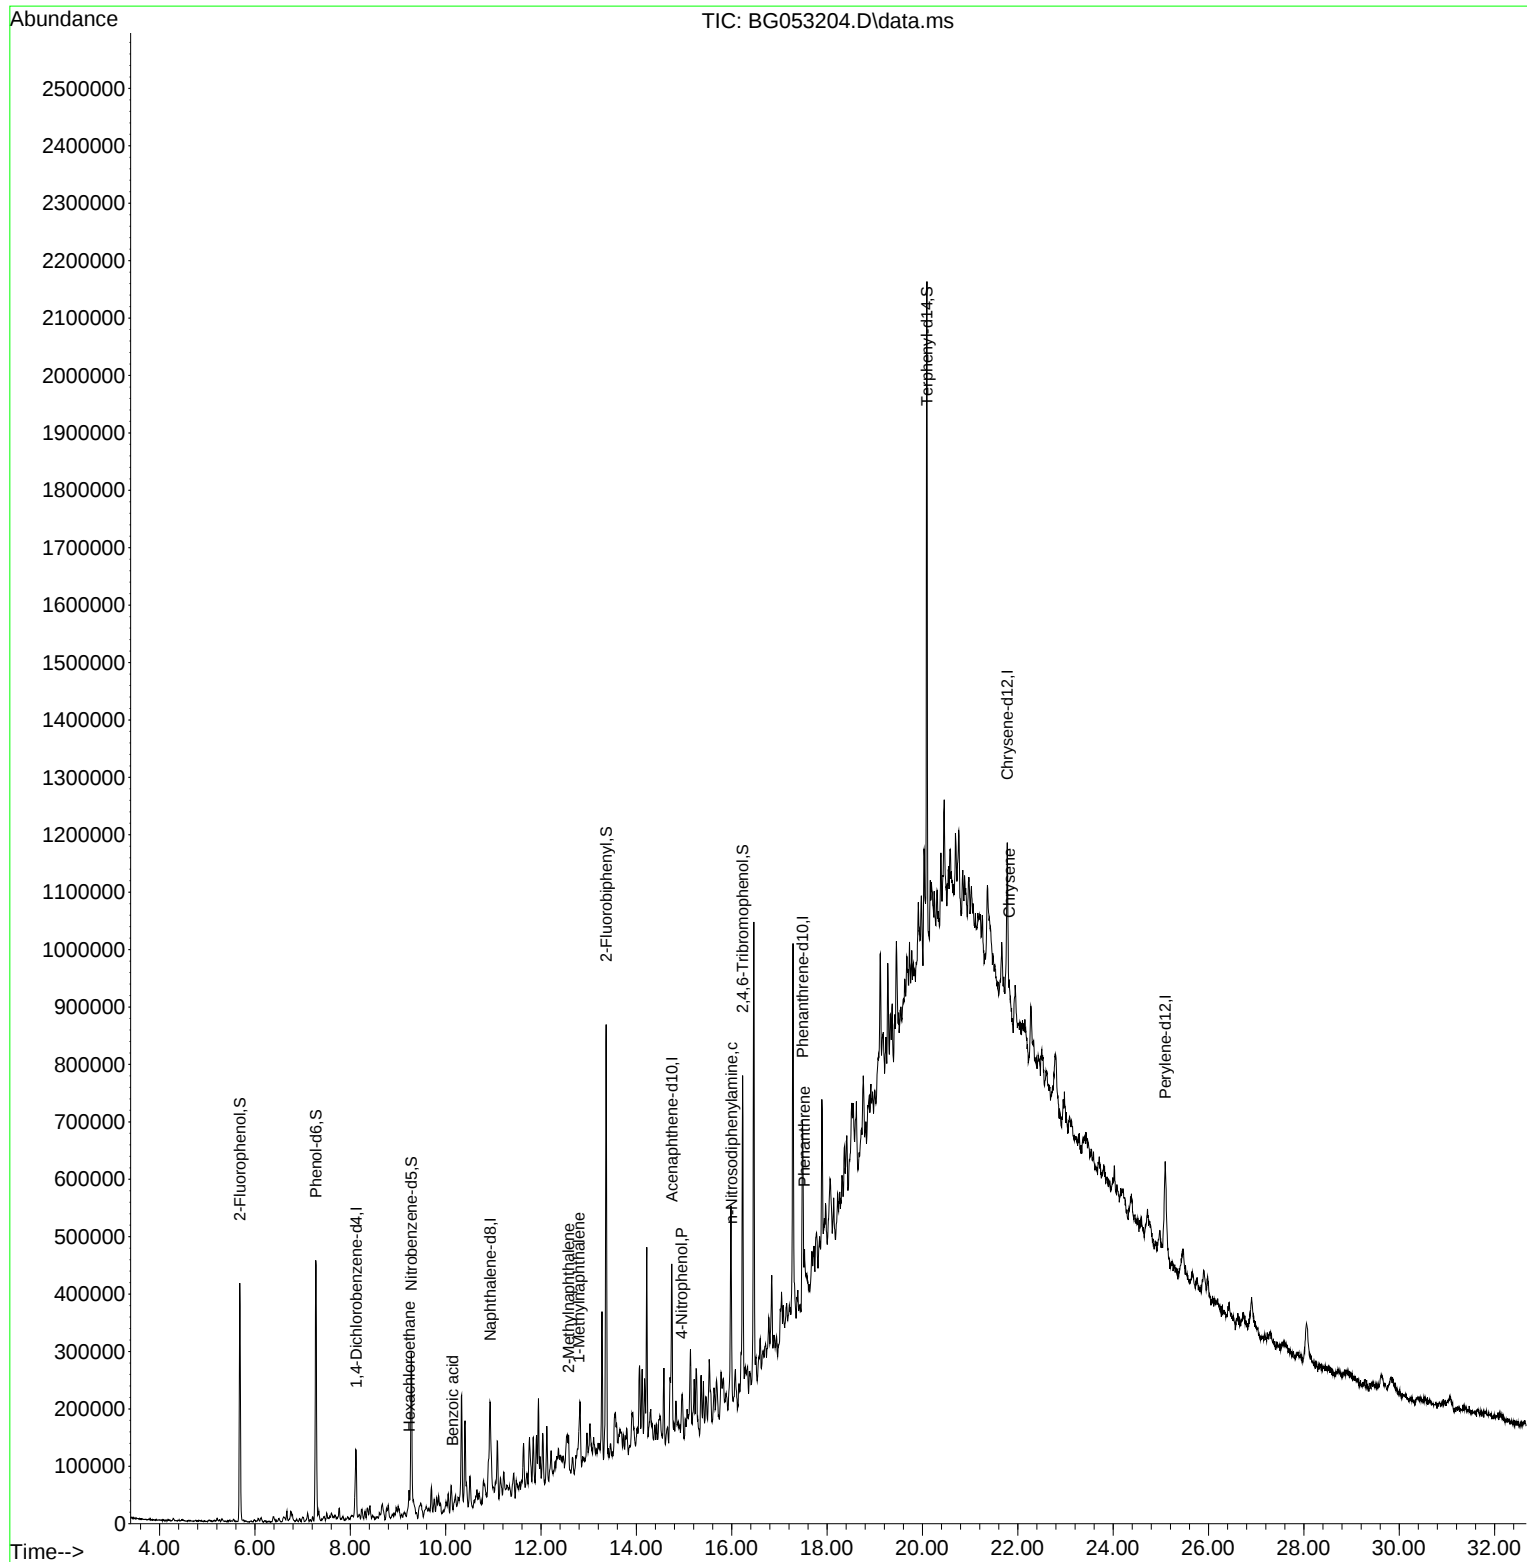






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.122 min Scan# 806
Delta R.T. -0.000 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Instrument :
BNA_G
ClientSampleId :
WC-15-1-3







Tgt Ion:152 Resp: 32676
Ion Ratio Lower Upper
152 100
150 154.1 114.6 172.0
115 58.2 45.9 68.9

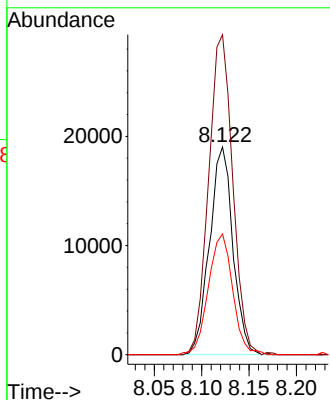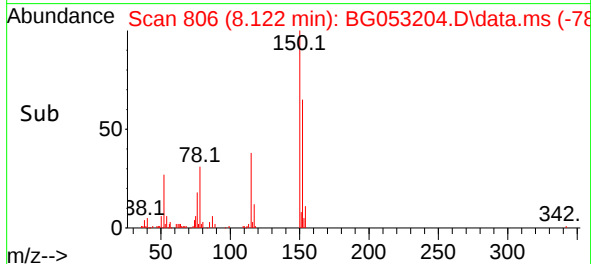

#5
2-Fluorophenol
Concen: 87.376 ng
RT: 5.684 min Scan# 391
Delta R.T. 0.000 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Tgt Ion:112 Resp: 166557
Ion Ratio Lower Upper
112 100
64 69.3 48.0 72.0
63 42.0 26.5 39.7#


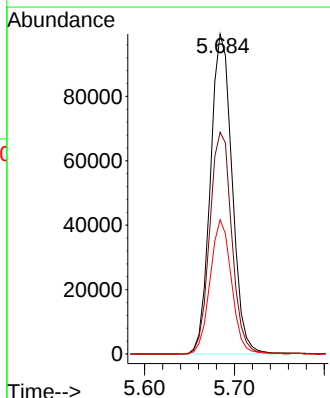
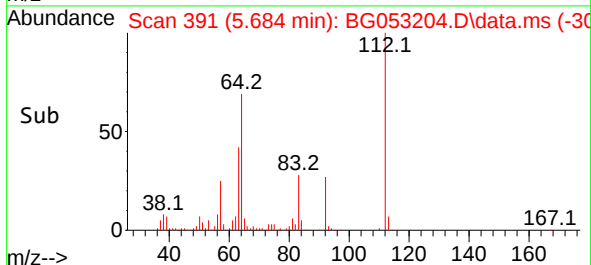
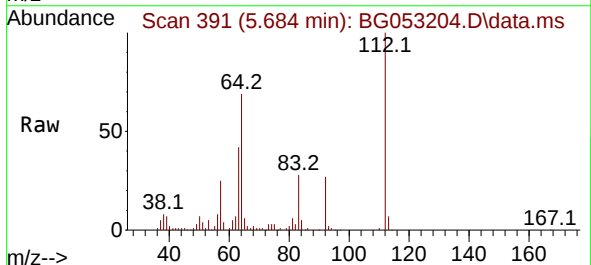




#7
Phenol-d6
Concen: 85.145 ng
RT: 7.276 min Scan# 60
Delta R.T. -0.006 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33




Instrument :
BNA_G
ClientSampleId :
WC-15-1-3


Tgt Ion: 99 Resp: 250292
Ion Ratio Lower Upper
99 100
42 20.9 14.7 22.1
71 43.9 29.2 43.8#

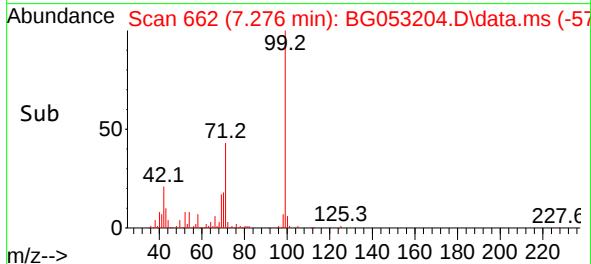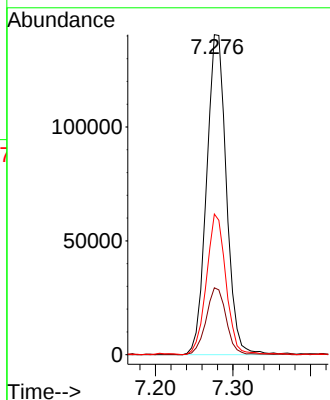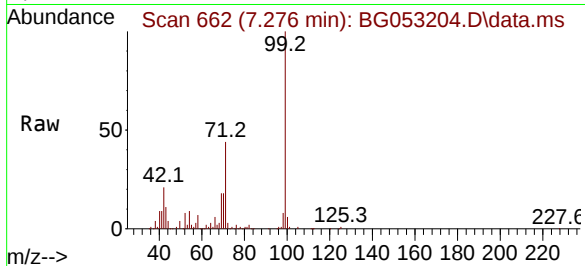

#18
Hexachloroethane
Concen: 2.085 ng
RT: 9.238 min Scan# 996
Delta R.T. 0.024 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Tgt Ion: 117 Resp: 1906
Ion Ratio Lower Upper
117 100
119 370.5 75.1 112.7#
201 0.0 96.6 145.0#


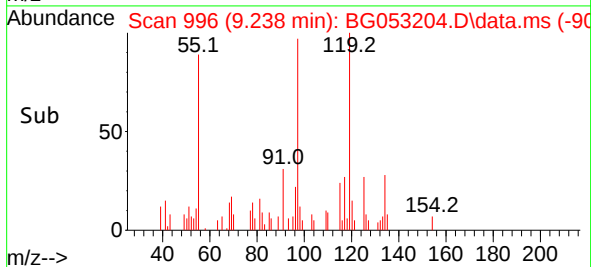
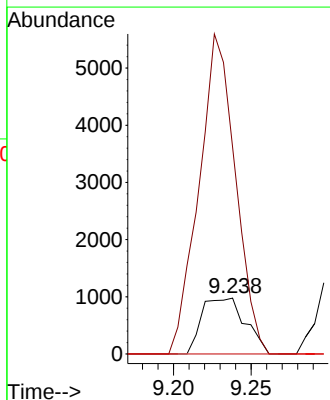
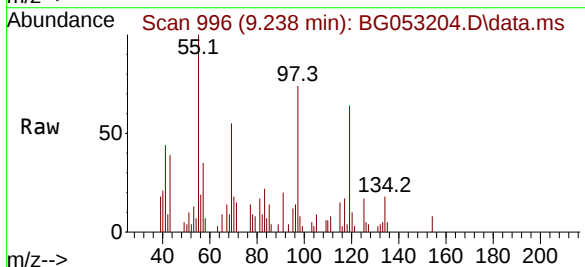


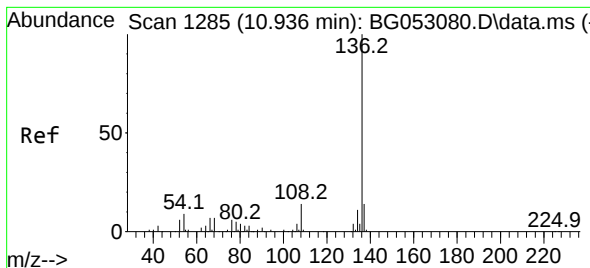

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.936 min Scan# 11
Delta R.T. -0.000 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33




Instrument :
BNA_G
ClientSampleId :
WC-15-1-3


Tgt Ion:136 Resp: 133010
Ion Ratio Lower Upper
136 100
137 11.2 9.4 14.2
54 9.5 6.4 9.6
68 7.9 5.0 7.6#

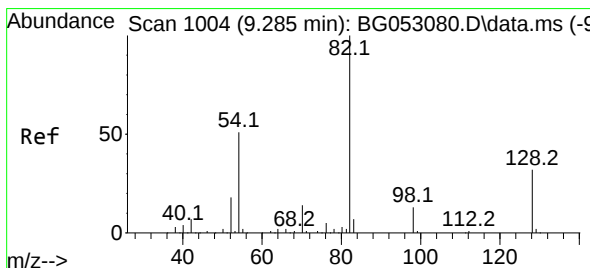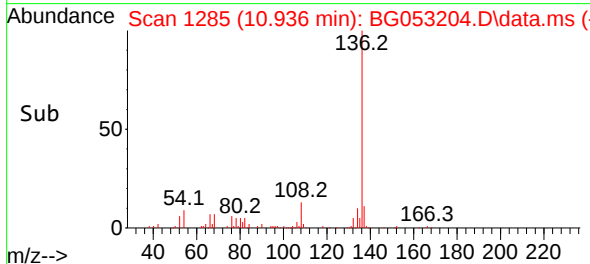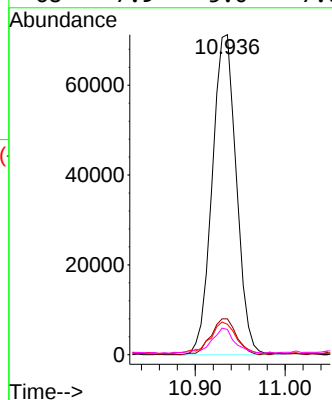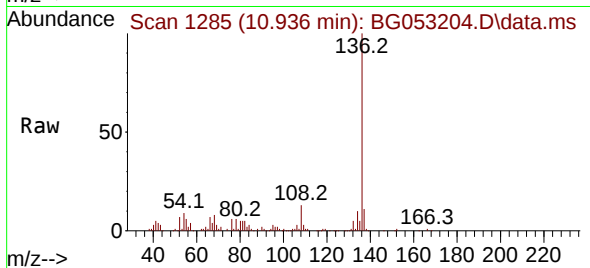

#23
Nitrobenzene-d5
Concen: 56.535 ng
RT: 9.279 min Scan# 1003
Delta R.T. -0.006 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Tgt Ion: 82 Resp: 185198
Ion Ratio Lower Upper
82 100
128 37.5 31.3 46.9
54 50.0 37.8 56.8

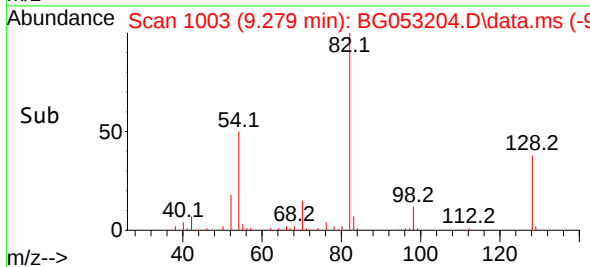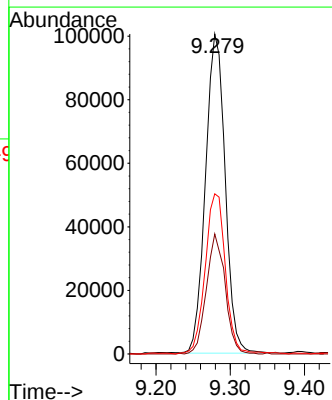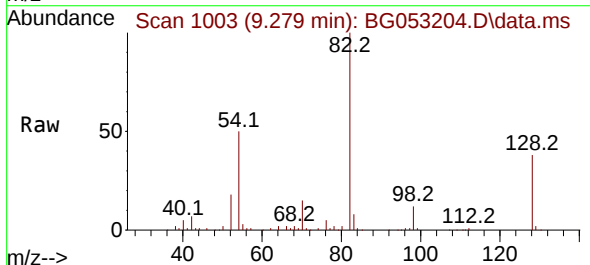



#32

Benzoic acid

Concen: 3.833 ng

RT: 10.149 min Scan# 1166

Delta R.T. -0.088 min

Lab File: BG053204.D

Acq: 19 Apr 2022 20:33





Instrument :

BNA_G

ClientSampleId :

WC-15-1-3

Tgt Ion:	122	Resp:	274
Ion	Ratio	Lower	Upper
122	100		
105	120.8	112.8	152.8
77	135.2	78.4	118.4#

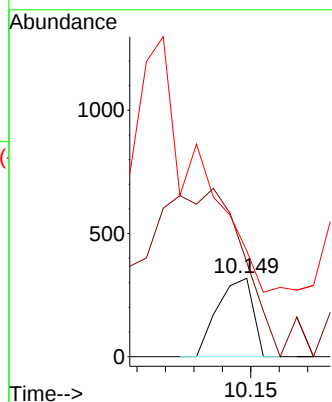

#37

2-Methylnaphthalene

Concen: 3.944 ng




RT: 12.581 min Scan# 1565


Delta R.T. 0.000 min

Lab File: BG053204.D

Acq: 19 Apr 2022 20:33

Tgt Ion:	142	Resp:	20708
Ion	Ratio	Lower	Upper
142	100		
141	99.6	71.3	106.9
115	50.7	29.5	44.3#


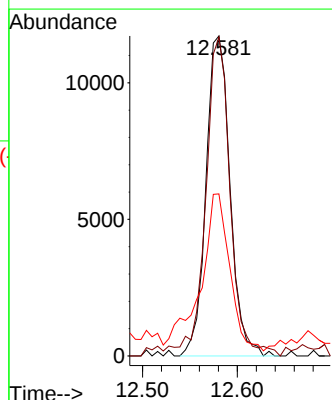
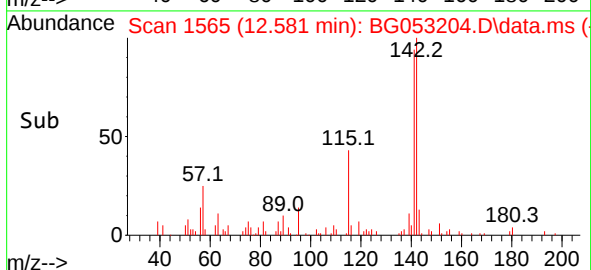





#38
1-Methylnaphthalene
Concen: 5.371 ng
RT: 12.798 min Scan# 1
Delta R.T. 0.000 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33




Instrument :
BNA_G
ClientSampleId :
WC-15-1-3


Tgt Ion:142 Resp: 27531
Ion Ratio Lower Upper
142 100
141 100.9 70.5 105.7
116 7.0 3.1 4.7#

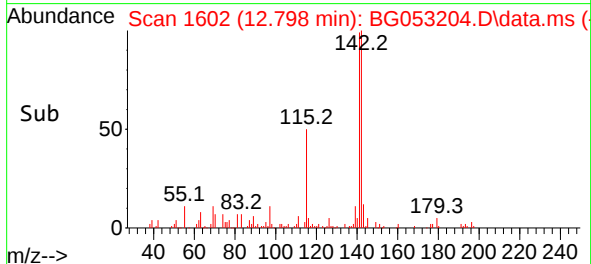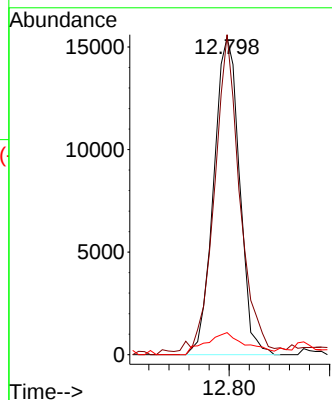

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.742 min Scan# 1933
Delta R.T. -0.006 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Tgt Ion:164 Resp: 93319
Ion Ratio Lower Upper
164 100
162 105.4 80.0 120.0
160 43.0 38.8 58.2


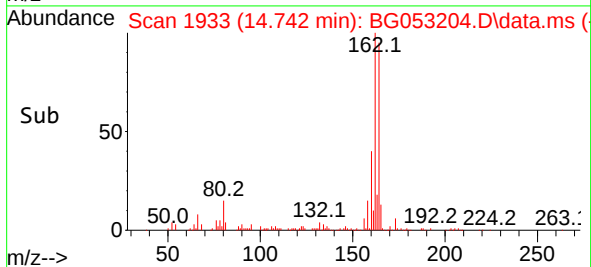
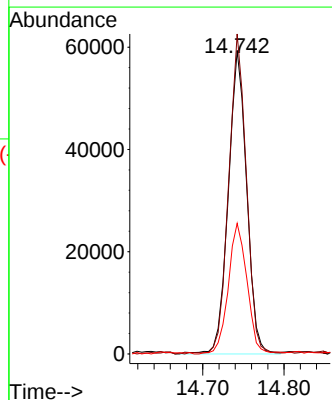
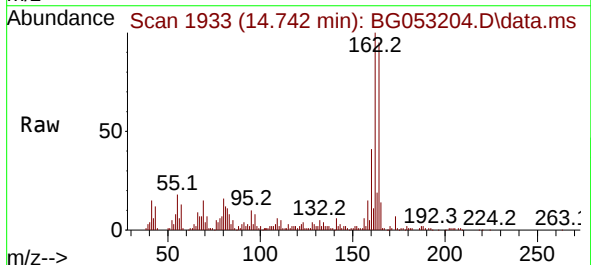




#42
2,4,6-Tribromophenol
Concen: 74.543 ng
RT: 16.229 min Scan# 2187
Delta R.T. -0.006 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33




Instrument :
BNA_G
ClientSampleId :
WC-15-1-3


Tgt Ion:330 Resp: 110672
Ion Ratio Lower Upper
330 100
332 96.5 75.8 113.6
141 32.9 24.6 36.8

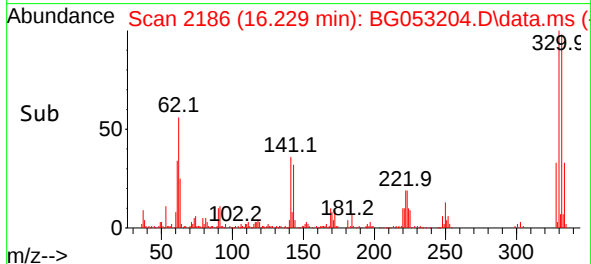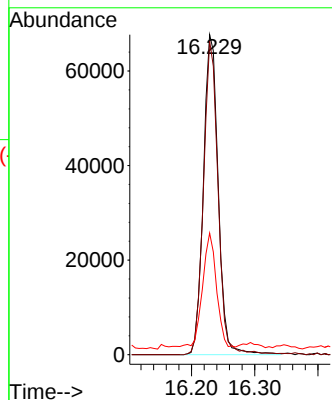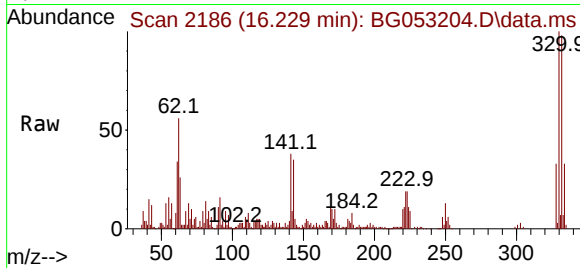

#45
2-Fluorobiphenyl
Concen: 60.129 ng
RT: 13.368 min Scan# 1699
Delta R.T. 0.000 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Tgt Ion:172 Resp: 406929
Ion Ratio Lower Upper
172 100
171 36.1 28.3 42.5
170 23.6 18.0 27.0


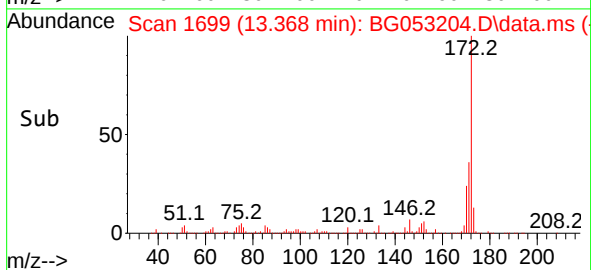
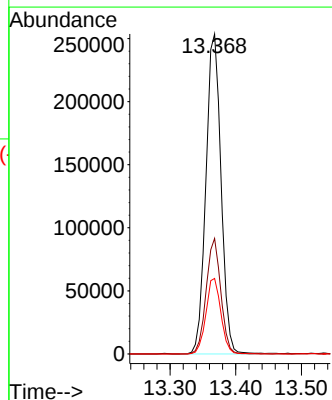
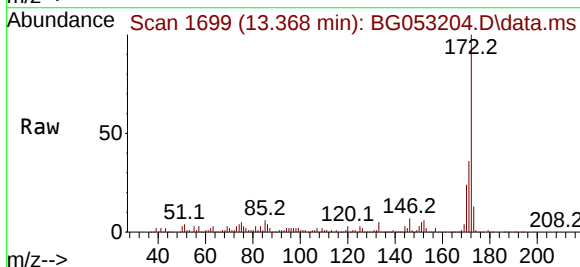




#56
4-Nitrophenol
Concen: 3.169 ng
RT: 14.948 min Scan# 1968
Delta R.T. 0.000 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33




Instrument :
BNA_G
ClientSampleId :
WC-15-1-3


Tgt Ion:139 Resp: 3980
Ion Ratio Lower Upper
139 100
109 170.2 67.1 107.1#
65 65.3 88.2 128.2#

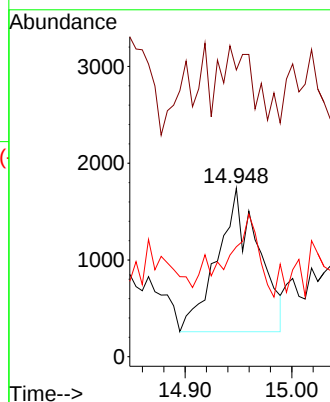

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.486 min Scan# 2400
Delta R.T. -0.006 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Tgt Ion:188 Resp: 176457
Ion Ratio Lower Upper
188 100
94 8.2 5.7 8.5
80 8.9 7.2 10.8


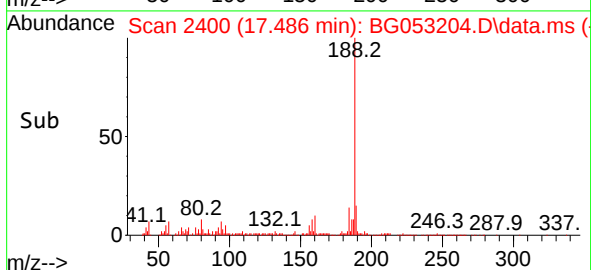
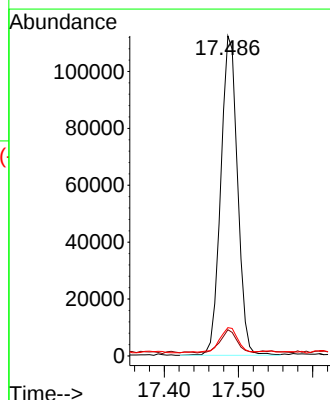





#66
 n-Nitrosodiphenylamine
 Concen: 2.959 ng
 RT: 15.994 min Scan# 2146
 Delta R.T. 0.000 min
 Lab File: BG053204.D
 Acq: 19 Apr 2022 20:33




Instrument :
 BNA_G
 ClientSampleId :
 WC-15-1-3


Tgt Ion:169 Resp: 15014
 Ion Ratio Lower Upper
 169 100
 168 16.4 54.5 81.7#
 167 15.0 29.6 44.4#

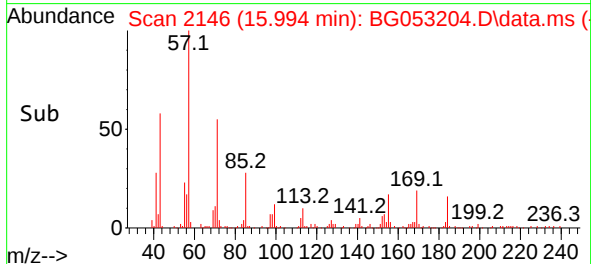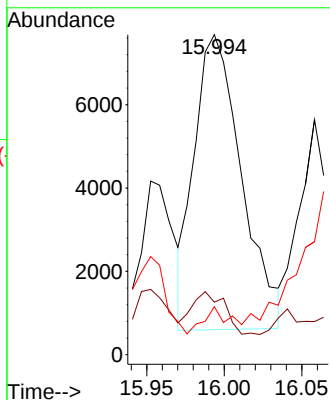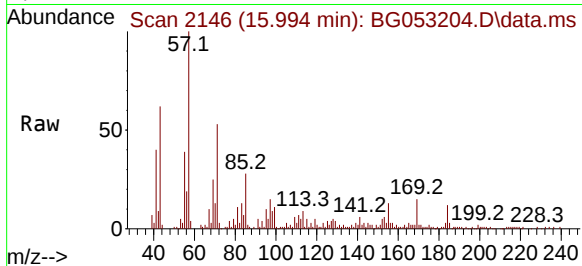

#71
 Phenanthrene
 Concen: 3.885 ng
 RT: 17.527 min Scan# 2407
 Delta R.T. -0.006 min
 Lab File: BG053204.D
 Acq: 19 Apr 2022 20:33

Tgt Ion:178 Resp: 37447
 Ion Ratio Lower Upper
 178 100
 176 17.8 15.9 23.9
 179 26.3 13.4 20.2#


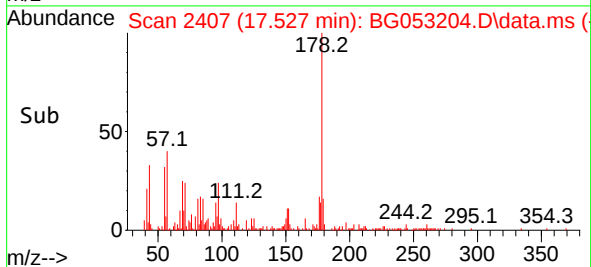
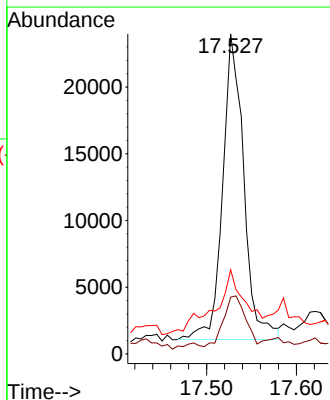
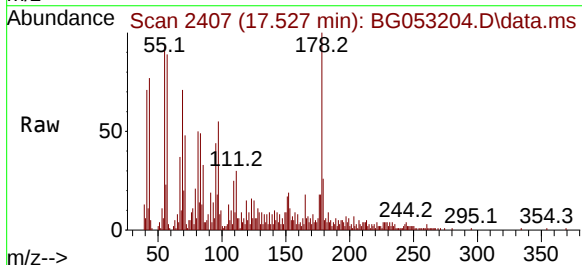




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.780 min Scan# 3130
Delta R.T. 0.006 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33




Instrument :
BNA_G
ClientSampleId :
WC-15-1-3


Tgt Ion:240 Resp: 170864
Ion Ratio Lower Upper
240 100
120 7.4 5.4 8.0
236 26.5 19.8 29.6

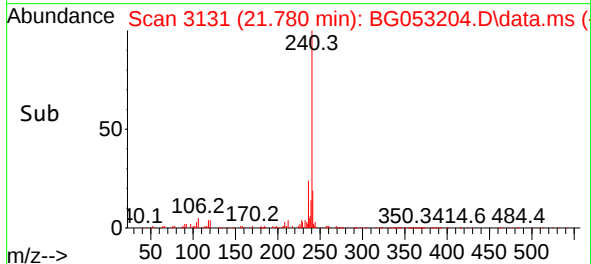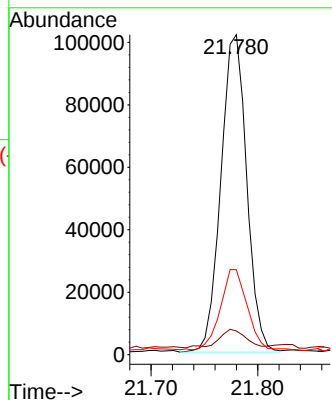

#79
Terphenyl-d14
Concen: 55.720 ng
RT: 20.094 min Scan# 2844
Delta R.T. 0.000 min
Lab File: BG053204.D
Acq: 19 Apr 2022 20:33

Tgt Ion:244 Resp: 563713
Ion Ratio Lower Upper
244 100
212 7.8 5.4 8.2
122 5.6 5.8 8.6#

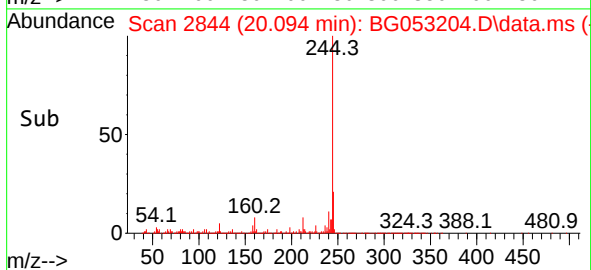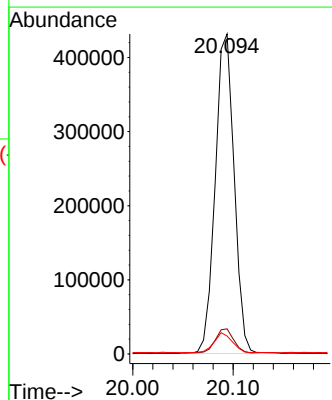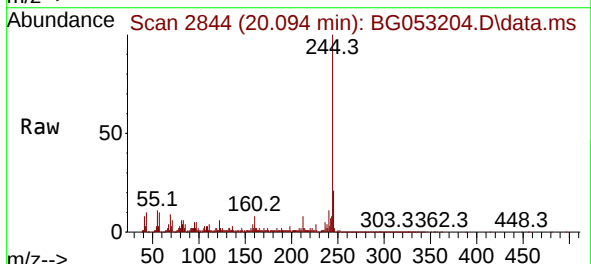



#83

Chrysene

Concen: 3.472 ng

RT: 21.821 min Scan# 3139

Delta R.T. -0.006 min

Lab File: BG053204.D

Acq: 19 Apr 2022 20:33

Instrument :

BNA_G

ClientSampleId :

WC-15-1-3





Tgt Ion:228 Resp: 37649

Ion Ratio Lower Upper

228 100

226 38.7 24.2 36.4#

229 53.9 16.3 24.5#

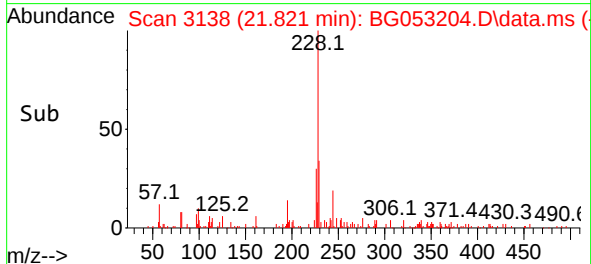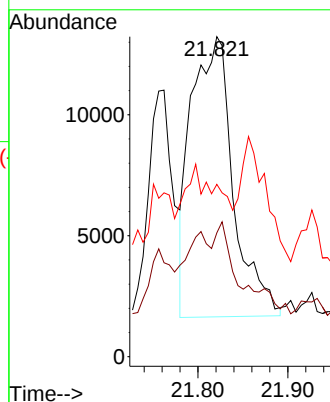

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.093 min Scan# 3695

Delta R.T. 0.018 min

Lab File: BG053204.D

Acq: 19 Apr 2022 20:33

Tgt Ion:264 Resp: 177632

Ion Ratio Lower Upper

264 100

260 21.9 18.2 27.2

265 21.1 15.1 22.7

