

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
 Data File : BG053197.D
 Acq On : 19 Apr 2022 16:01
 Operator : CG/JU
 Sample : N2462-03 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.682	384	390	396	rBV	43984	69363	11.06%	1.727%
2	7.274	655	661	670	rBV3	45592	87175	13.90%	2.170%
3	8.120	798	805	812	rVB	111052	196671	31.36%	4.896%
4	9.277	996	1002	1011	rBV2	28611	57824	9.22%	1.440%
5	10.928	1273	1283	1290	rBV	159405	297320	47.40%	7.402%
6	12.332	1517	1522	1525	rBV3	4076	7370	1.18%	0.183%
7	12.467	1541	1545	1552	rVB4	4079	6597	1.05%	0.164%
8	13.360	1689	1697	1708	rBV	88704	147531	23.52%	3.673%
9	13.560	1726	1731	1734	rBV4	4858	7419	1.18%	0.185%
10	14.629	1908	1913	1916	rVB4	5617	8457	1.35%	0.211%
11	14.740	1925	1932	1939	rBV	278470	456445	72.77%	11.364%
12	14.964	1963	1970	1975	rVB4	11278	17669	2.82%	0.440%
13	15.069	1984	1988	1994	rVB6	4710	8654	1.38%	0.215%
14	15.569	2070	2073	2079	rVB4	6576	10209	1.63%	0.254%
15	15.974	2138	2142	2147	rBV4	4823	8611	1.37%	0.214%
16	16.227	2178	2185	2195	rBV2	62298	115675	18.44%	2.880%
17	16.432	2216	2220	2221	rBV3	8744	8929	1.42%	0.222%
18	16.456	2221	2224	2231	rVB3	17408	23793	3.79%	0.592%
19	16.702	2262	2266	2270	rVB6	9727	14700	2.34%	0.366%
20	16.808	2280	2284	2287	rBV3	21140	28484	4.54%	0.709%
21	16.896	2294	2299	2302	rBV6	4005	7689	1.23%	0.191%
22	17.225	2351	2355	2359	rBV6	7566	11401	1.82%	0.284%
23	17.278	2361	2364	2367	rVB5	6513	9605	1.53%	0.239%
24	17.484	2392	2399	2412	rBV	400624	627221	100.00%	15.615%
25	17.965	2477	2481	2485	rVB5	9558	13790	2.20%	0.343%
26	18.077	2495	2500	2504	rBV5	11719	18550	2.96%	0.462%
27	18.142	2507	2511	2517	rVB9	5642	8048	1.28%	0.200%
28	18.294	2534	2537	2542	rVB6	6084	10543	1.68%	0.262%
29	18.371	2546	2550	2557	rVV	31384	47134	7.51%	1.173%
30	18.429	2557	2560	2564	rVB	12177	16650	2.65%	0.415%
31	18.653	2595	2598	2601	rBV5	7198	7449	1.19%	0.185%
32	18.776	2617	2619	2626	rVB7	6190	8874	1.41%	0.221%
33	19.275	2702	2704	2709	rVB6	8889	10735	1.71%	0.267%
34	19.440	2730	2732	2738	rVB6	11674	15687	2.50%	0.391%
35	19.628	2762	2764	2768	rVB5	8076	7636	1.22%	0.190%
36	19.675	2769	2772	2779	rBV2	32296	49440	7.88%	1.231%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
Data File : BG053197.D
Acq On : 19 Apr 2022 16:01
Operator : CG/JU
Sample : N2462-03 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-05

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	20.080	2837	2841	2847	rVB	193608	259130	41.31%	6.451%
38	20.579	2923	2926	2929	rBV3	14761	17828	2.84%	0.444%
39	20.779	2957	2960	2963	rVB3	35124	37089	5.91%	0.923%
40	21.766	3122	3128	3136	rVB	357206	611894	97.56%	15.234%
41	24.674	3621	3623	3630	rBV8	8866	18149	2.89%	0.452%
42	25.068	3680	3690	3700	rBV3	216303	623316	99.38%	15.518%




Sum of corrected areas: 4016754

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
Data File : BG053197.D
Acq On : 19 Apr 2022 16:01
Operator : CG/JU
Sample : N2462-03 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

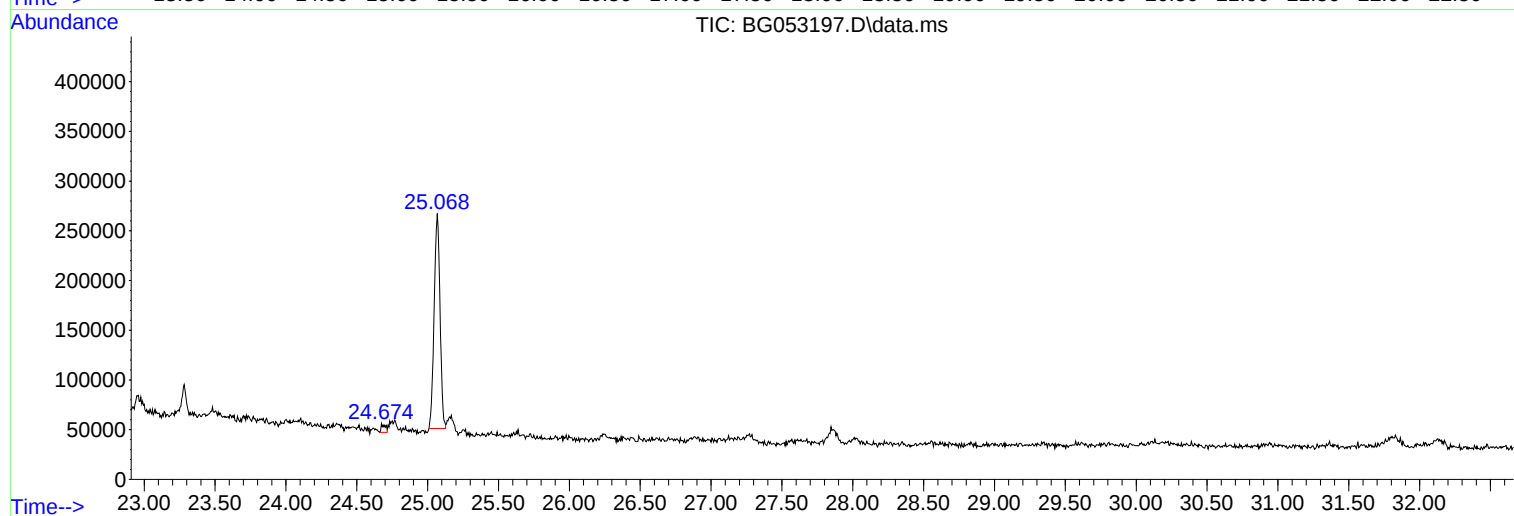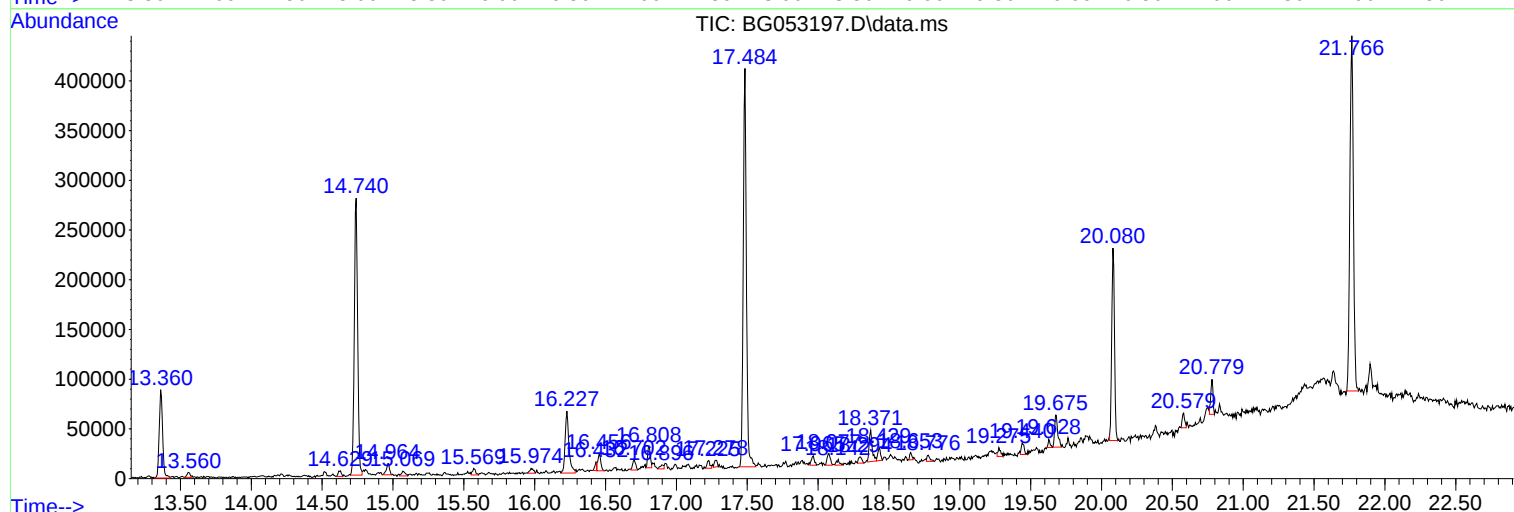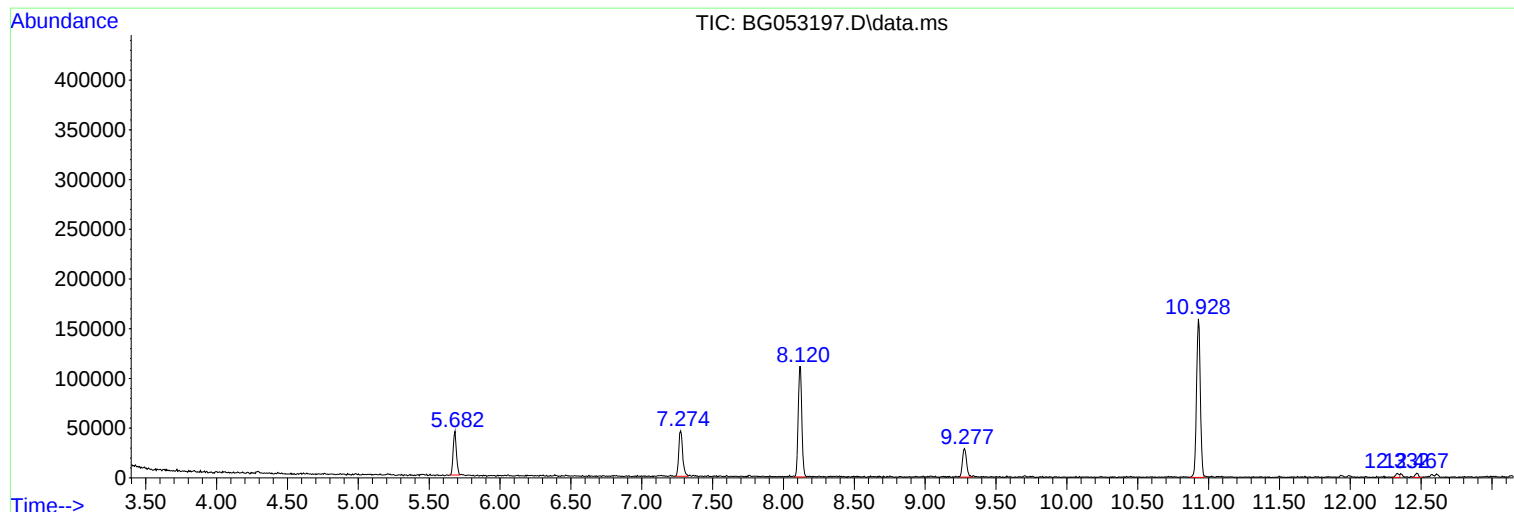

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
Data File : BG053197.D
Acq On : 19 Apr 2022 16:01
Operator : CG/JU
Sample : N2462-03 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
Data File : BG053197.D
Acq On : 19 Apr 2022 16:01
Operator : CG/JU
Sample : N2462-03 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------