
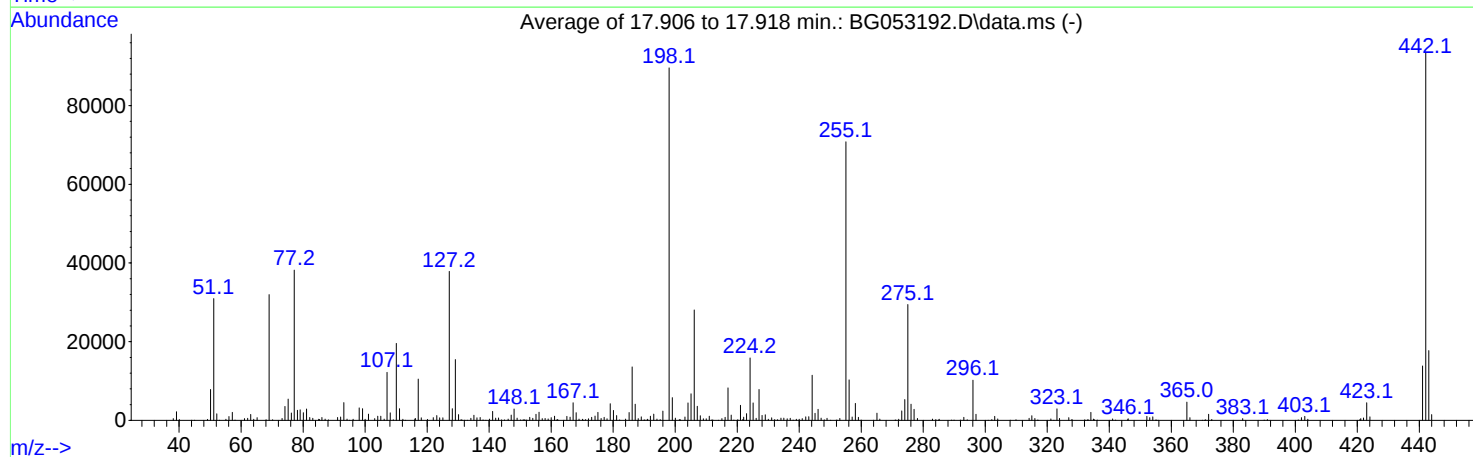


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
 Data File : BG053192.D
 Acq On : 19 Apr 2022 11:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

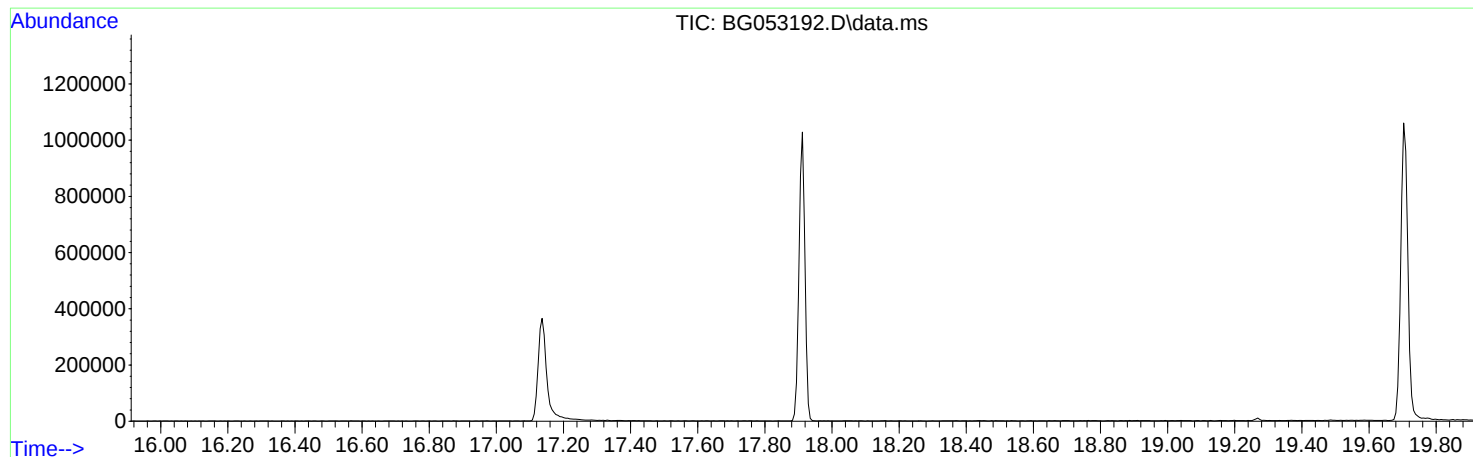




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	30949	PASS
68	69	0.00	2	0.5	173	PASS
69	198	0.00	100	35.7	31987	PASS
70	69	0.00	2	0.5	155	PASS
127	198	10	80	42.3	37859	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89605	PASS
199	198	5	9	6.4	5760	PASS
275	198	10	60	32.9	29459	PASS
365	198	1	100	5.2	4651	PASS
441	198	0.01	100	15.4	13815	PASS
442	442	50	100	100.0	93501	PASS
443	442	15	24	19.0	17723	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
Data File : BG053192.D
Acq On : 19 Apr 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 20 06:41:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

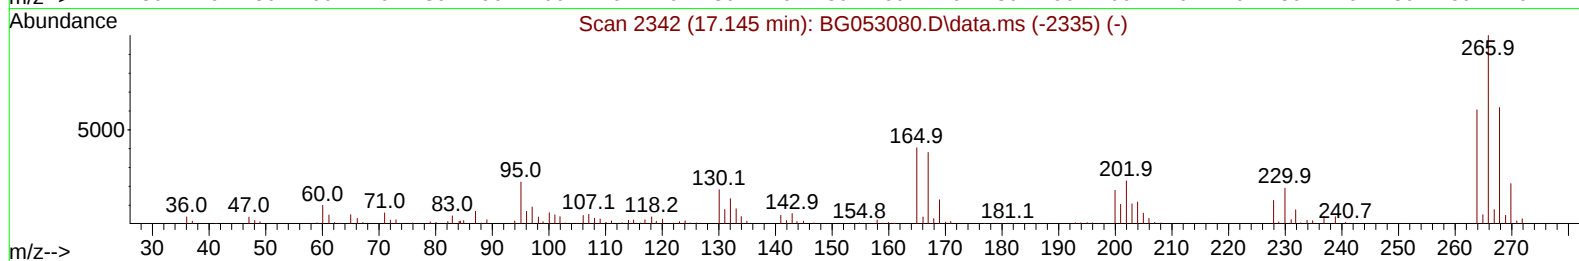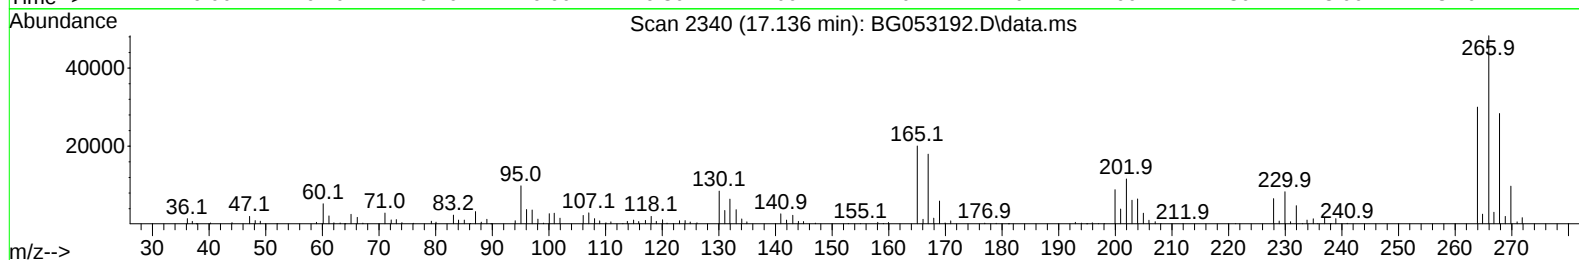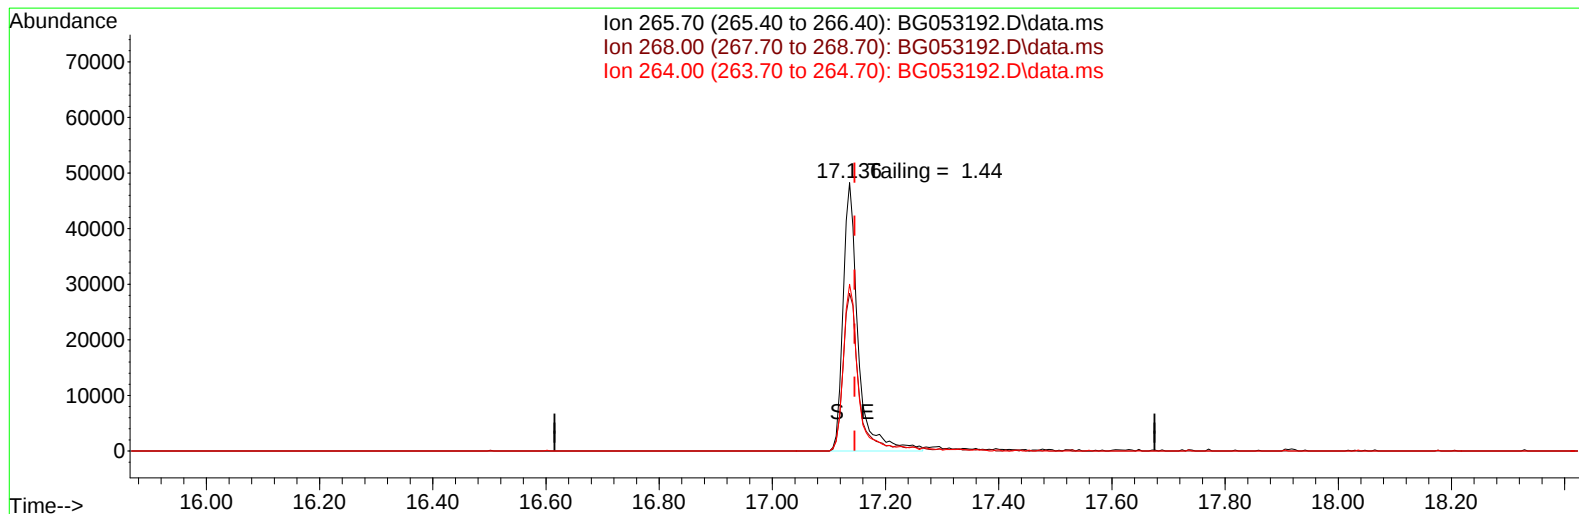

TIC: BG053192.D\data.ms

(70) Pentachlorophenol (C)

17.136min (-0.009) 17375.65 ng




response 89738

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	58.76
264.00	56.60	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041922\
Data File : BG053192.D
Acq On : 19 Apr 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 20 06:41:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

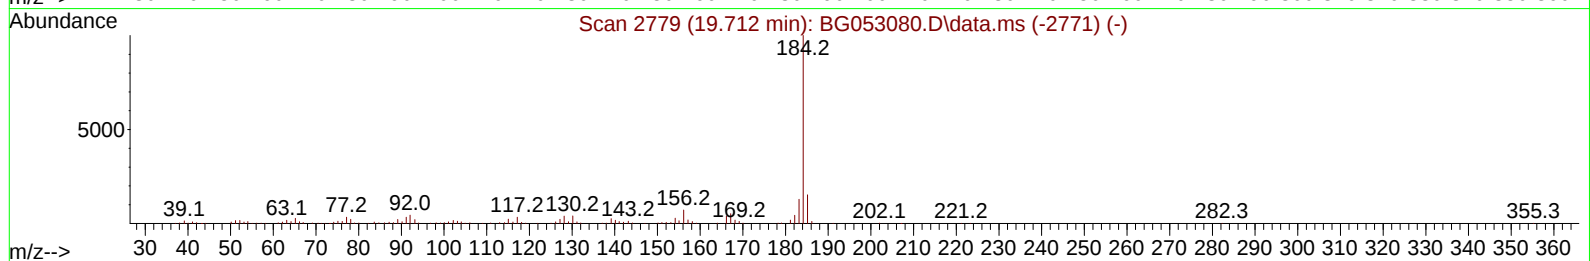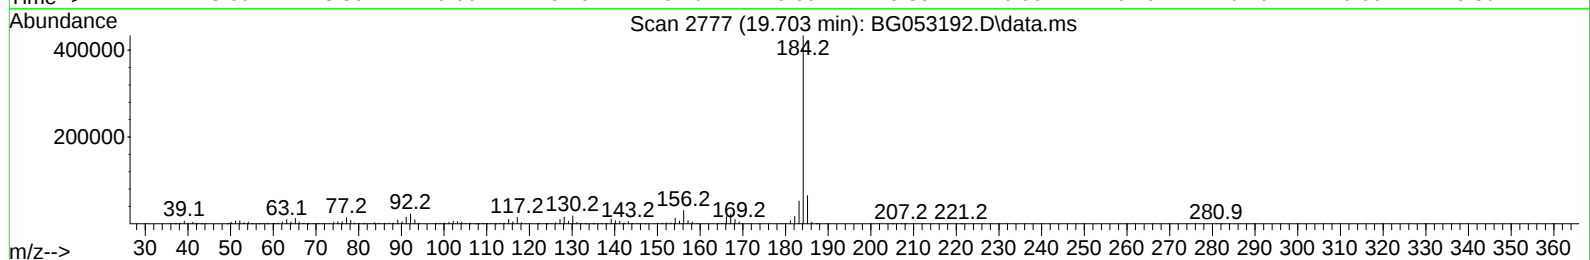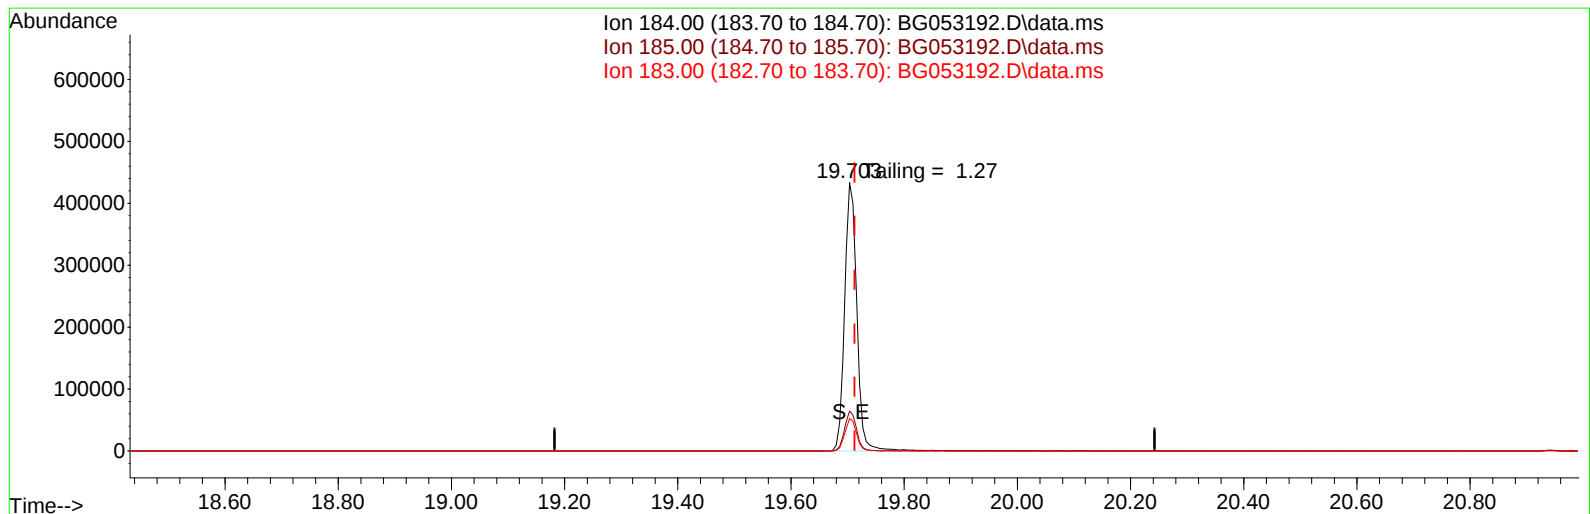

TIC: BG053192.D\data.ms

(77) Benzidine

19.703min (-0.009) 385893.91 ng

response 649600

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.95
183.00	11.80	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2022	BNA_G	BG053192.D
Compound Name	Response	Retention Time
DDT	355724	20.943
DDD	7284	20.496
DDE	1117	19.997
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8401	364125	2.31

Instrument :
BNA_G
ClientSampleId :
DFTPP