
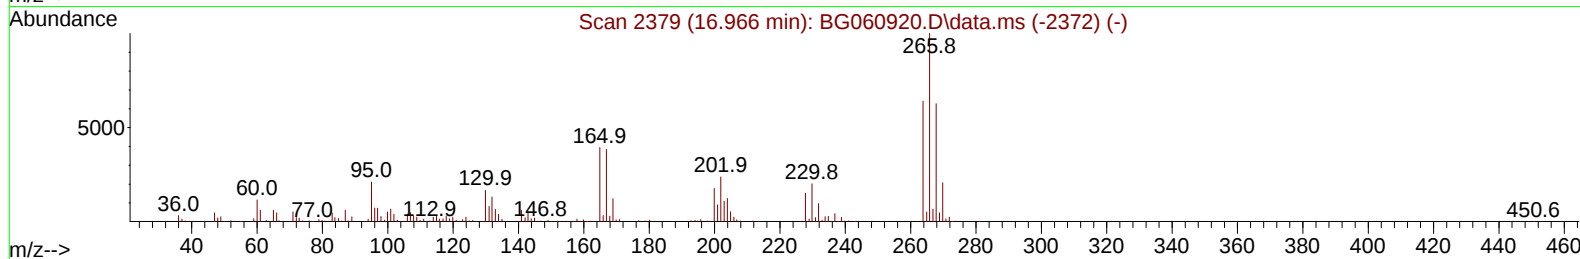
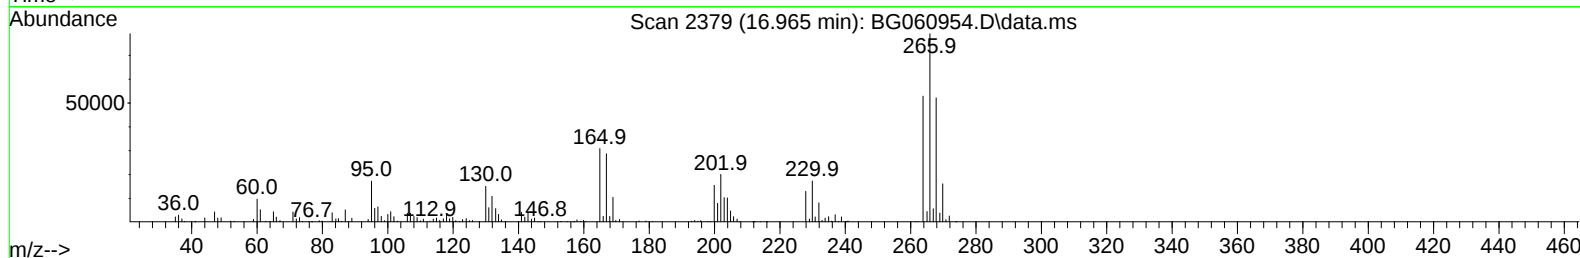


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041924\
Data File : BG060954.D
Acq On : 19 Apr 2024 9:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 12:18:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

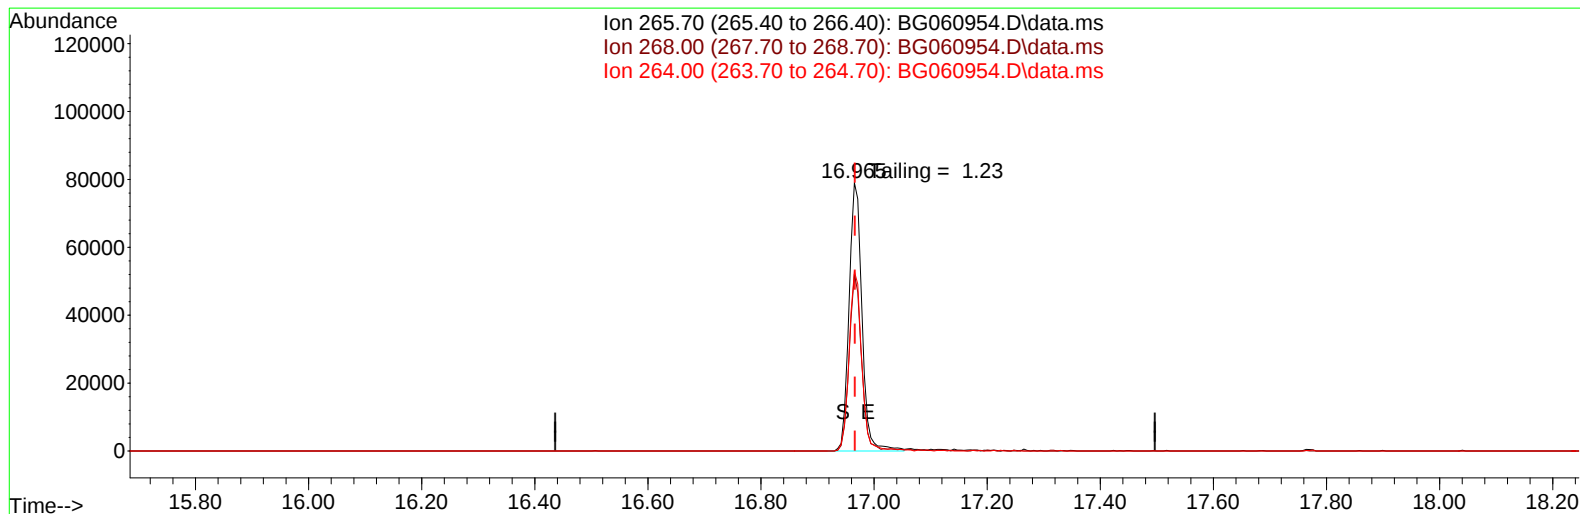

TIC: BG060954.D\data.ms

(70) Pentachlorophenol (C)




16.965min (-0.001) 16833.54 ng

response 125624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	65.92
264.00	64.00	66.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041924\
Data File : BG060954.D
Acq On : 19 Apr 2024 9:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 12:18:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

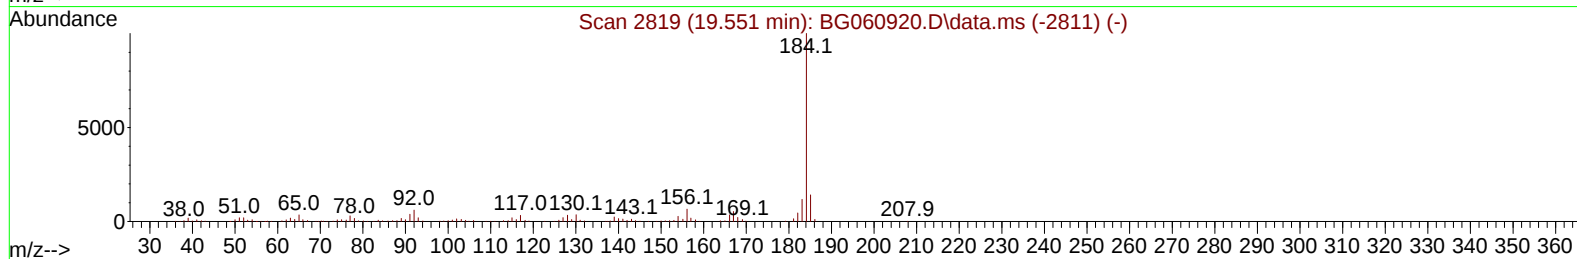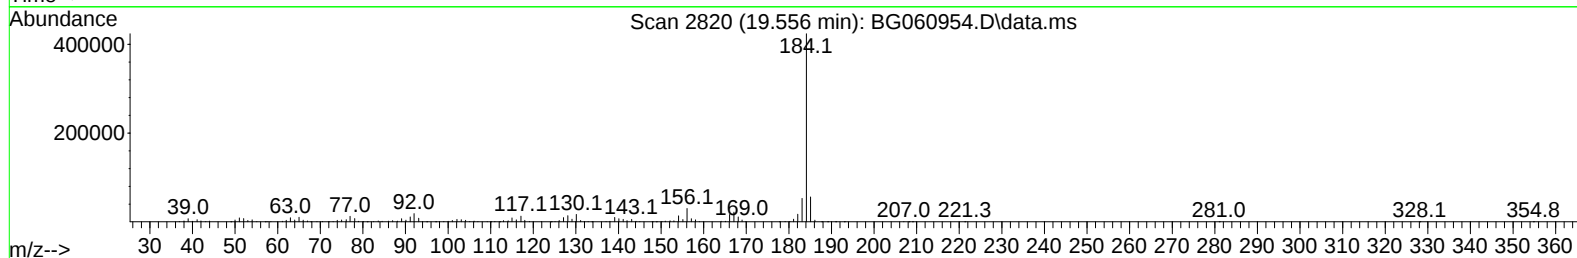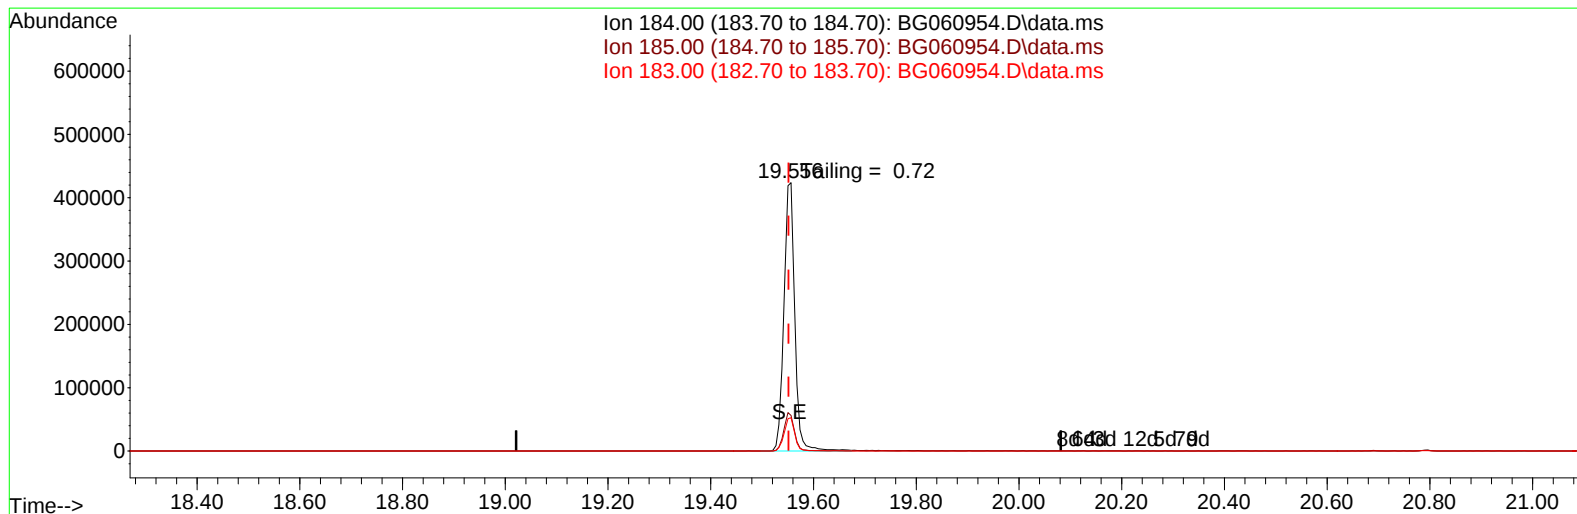

TIC: BG060954.D\data.ms

(77) Benzidine

19.556min (+ 0.005) 233524.91 ng m

response 633564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.23
183.00	11.80	12.43
0.00	0.00	0.00