
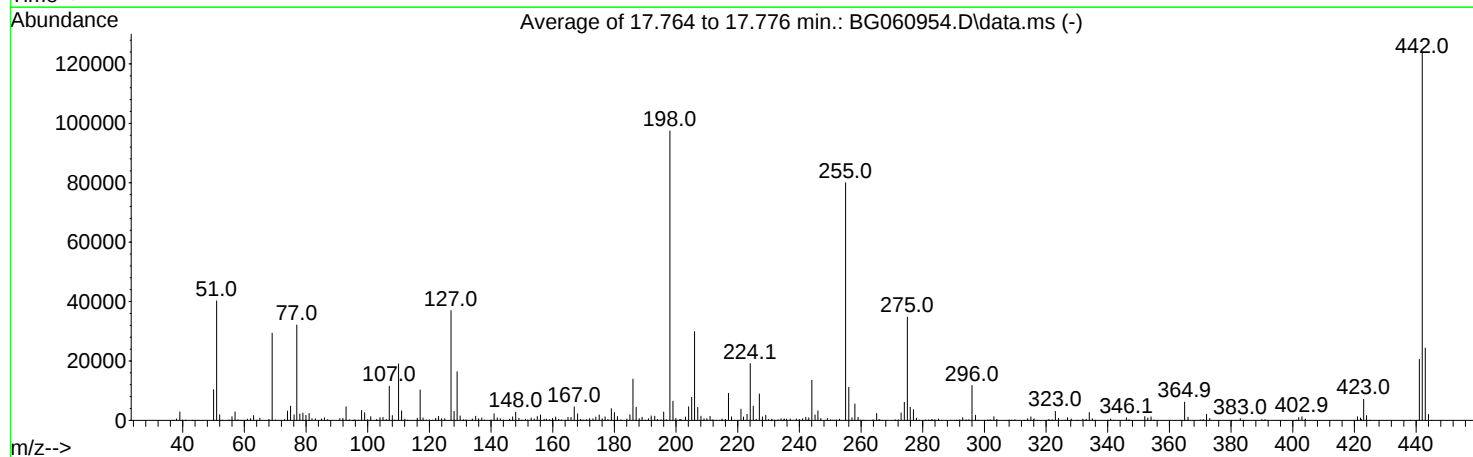


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041924\
Data File : BG060954.D
Acq On : 19 Apr 2024 9:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 18 02:02:19 2024

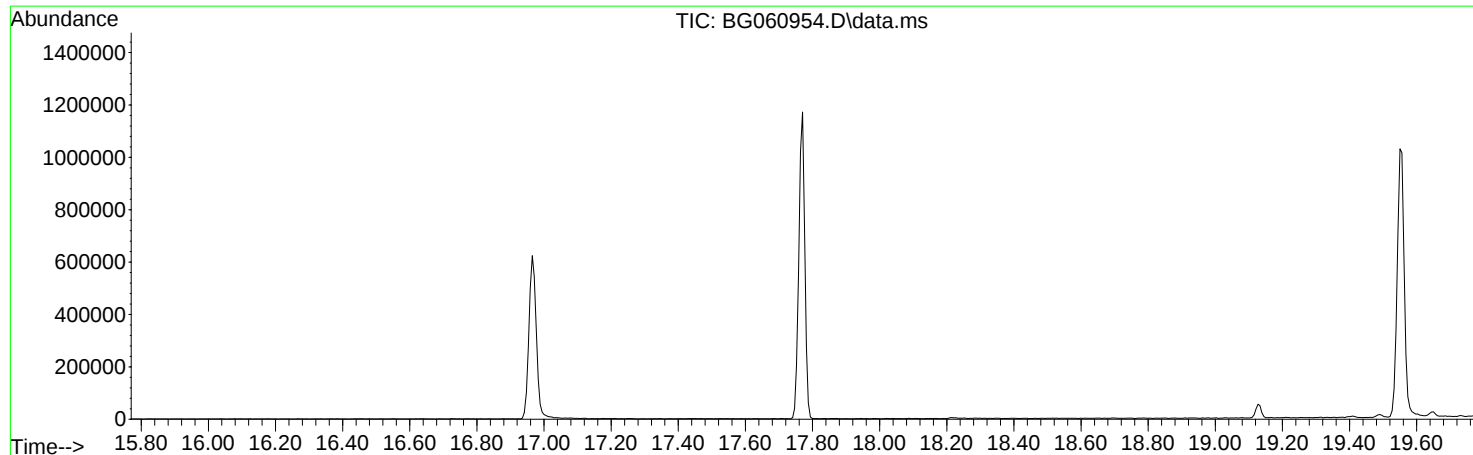




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	40224	PASS
68	69	0.00	2	1.2	339	PASS
69	198	0.00	100	30.1	29363	PASS
70	69	0.00	2	0.5	136	PASS
127	198	10	80	37.9	36944	PASS
197	198	0.00	2	0.3	273	PASS
198	198	100	100	100.0	97451	PASS
199	198	5	9	6.6	6476	PASS
275	198	10	60	35.7	34757	PASS
365	198	1	100	6.3	6136	PASS
441	198	0.01	100	21.1	20565	PASS
442	442	50	100	100.0	123848	PASS
443	442	15	24	19.7	24368	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041924\
Data File : BG060954.D
Acq On : 19 Apr 2024 9:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 12:18:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

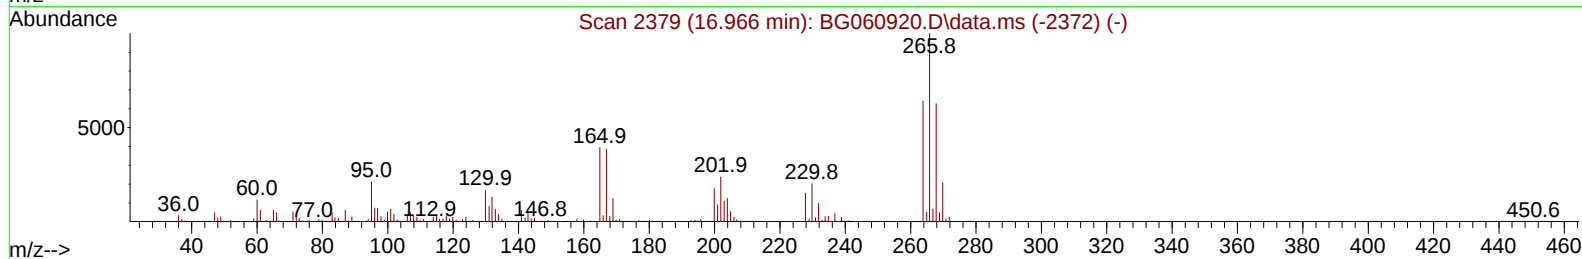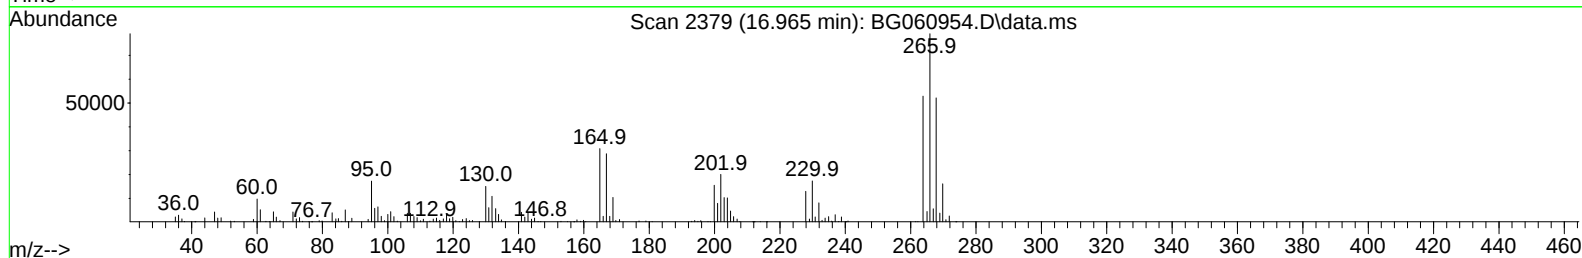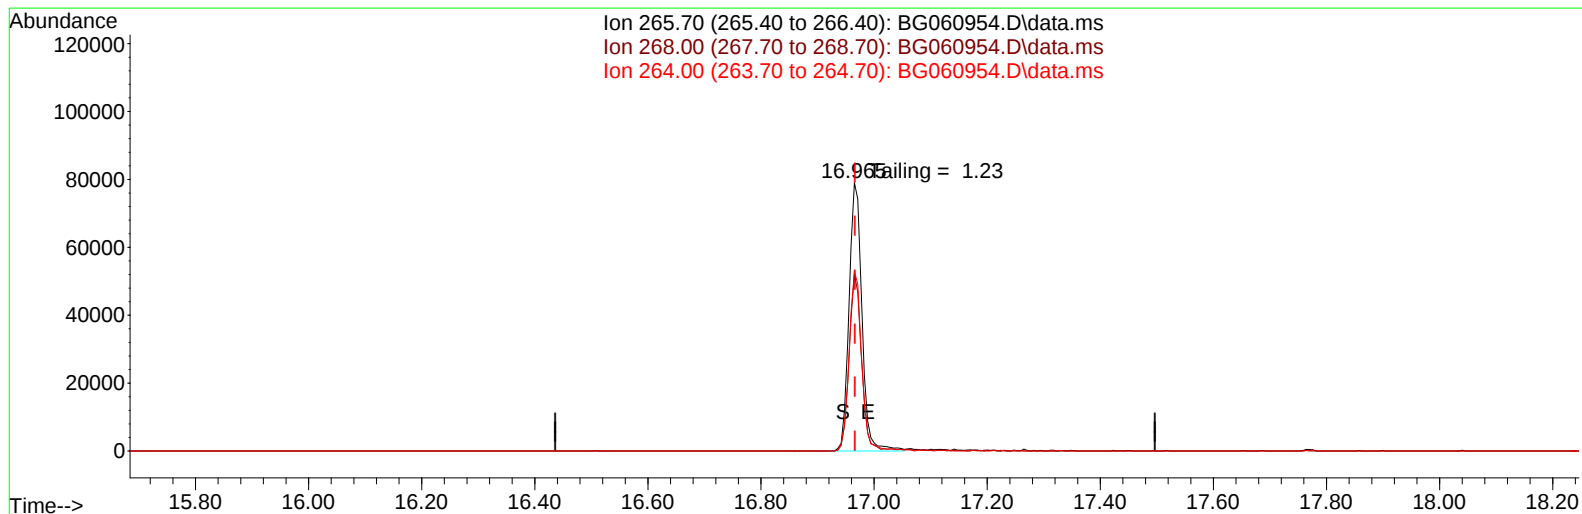

TIC: BG060954.D\data.ms

(70) Pentachlorophenol (C)

16.965min (-0.001) 16833.54 ng




response 125624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	65.92
264.00	64.00	66.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041924\
Data File : BG060954.D
Acq On : 19 Apr 2024 9:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 12:18:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

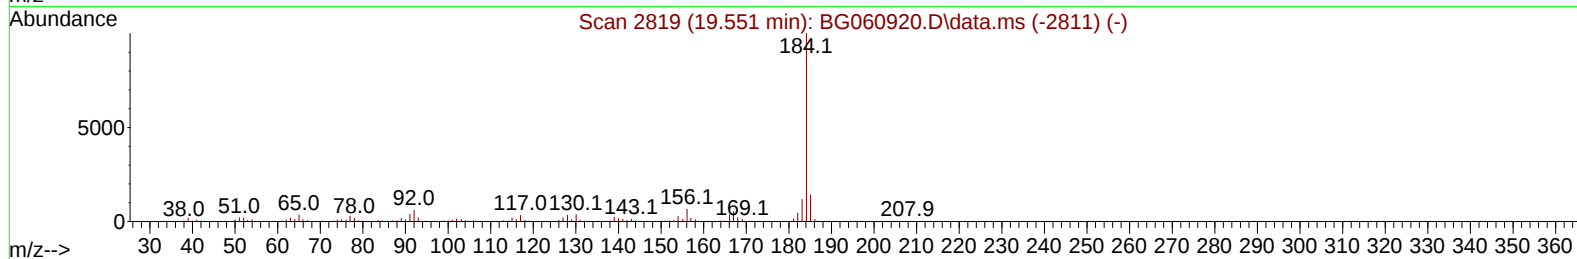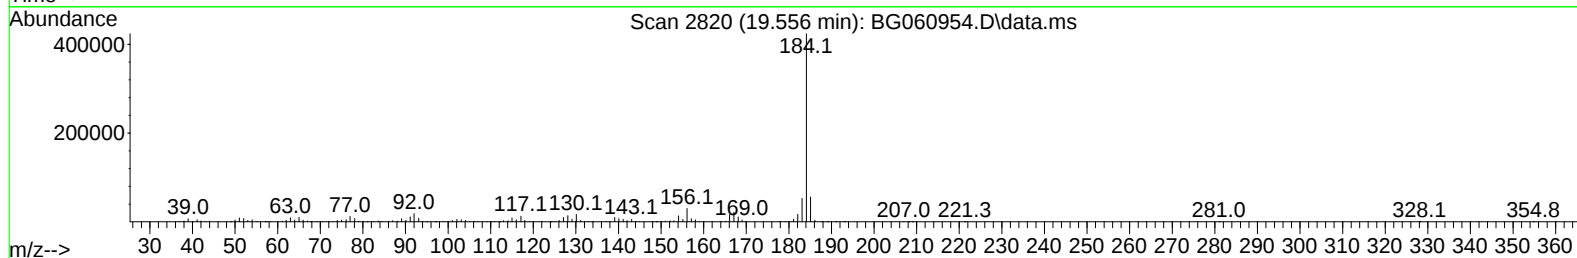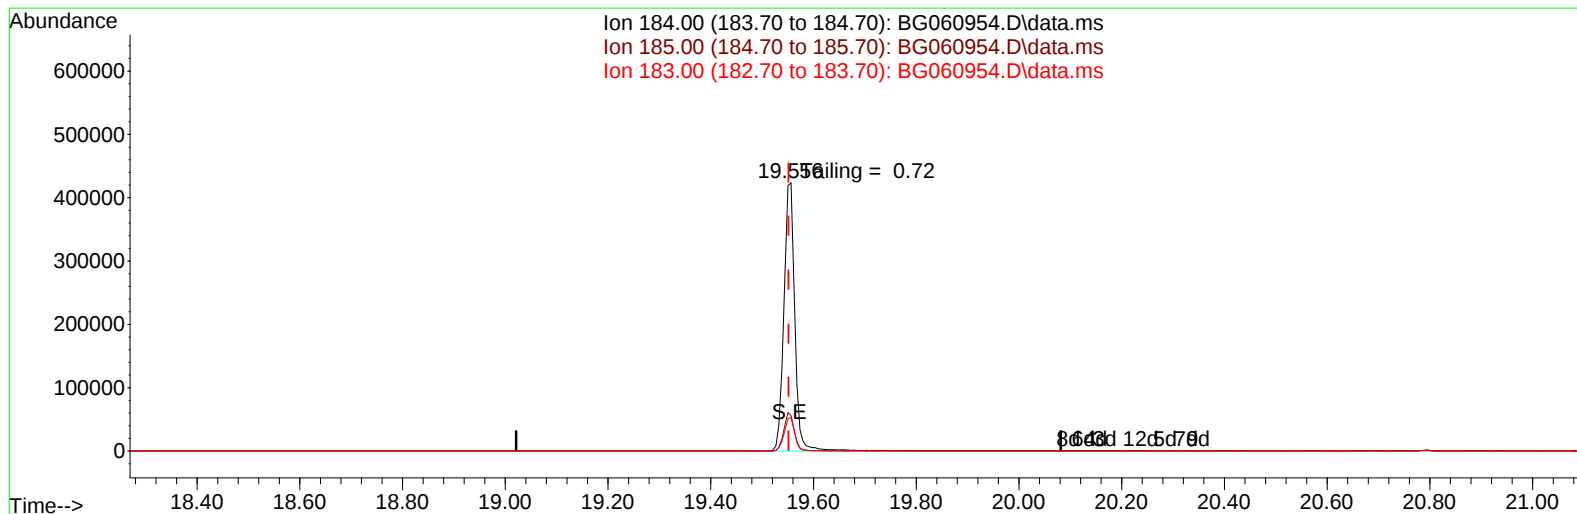

TIC: BG060954.D\data.ms

(77) Benzidine

19.556min (+ 0.005) 233524.91 ng m

response 633564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.23
183.00	11.80	12.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2024	BNA_G	<u>BG060954.D</u>
Compound Name	Response	Retention Time
DDT	369577	20.79
DDD	11175	20.349
DDE	1458	19.844
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12633	382210	3.31

Instrument :
BNA_G
ClientSampleId :
DFTPP