
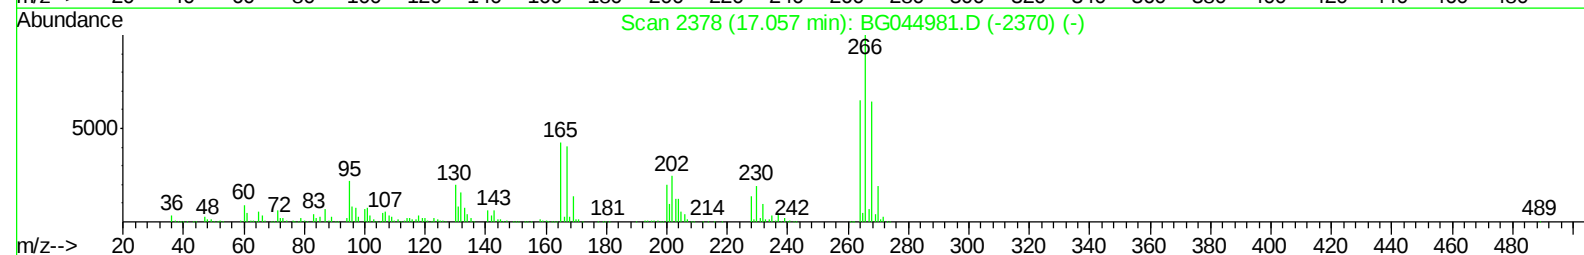
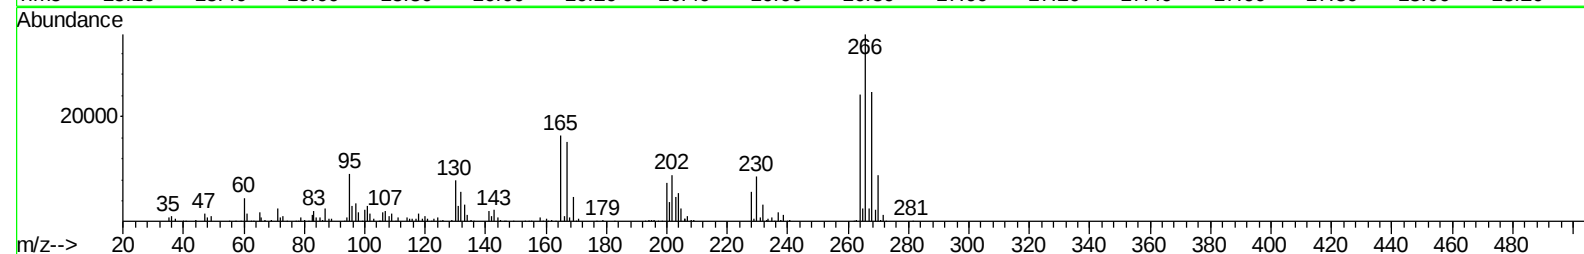


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG042020\
 Data File : BG045089.D
 Acq On : 20 Apr 2020 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 05:46:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 20 11:57:28 2020
 Response via : Initial Calibration

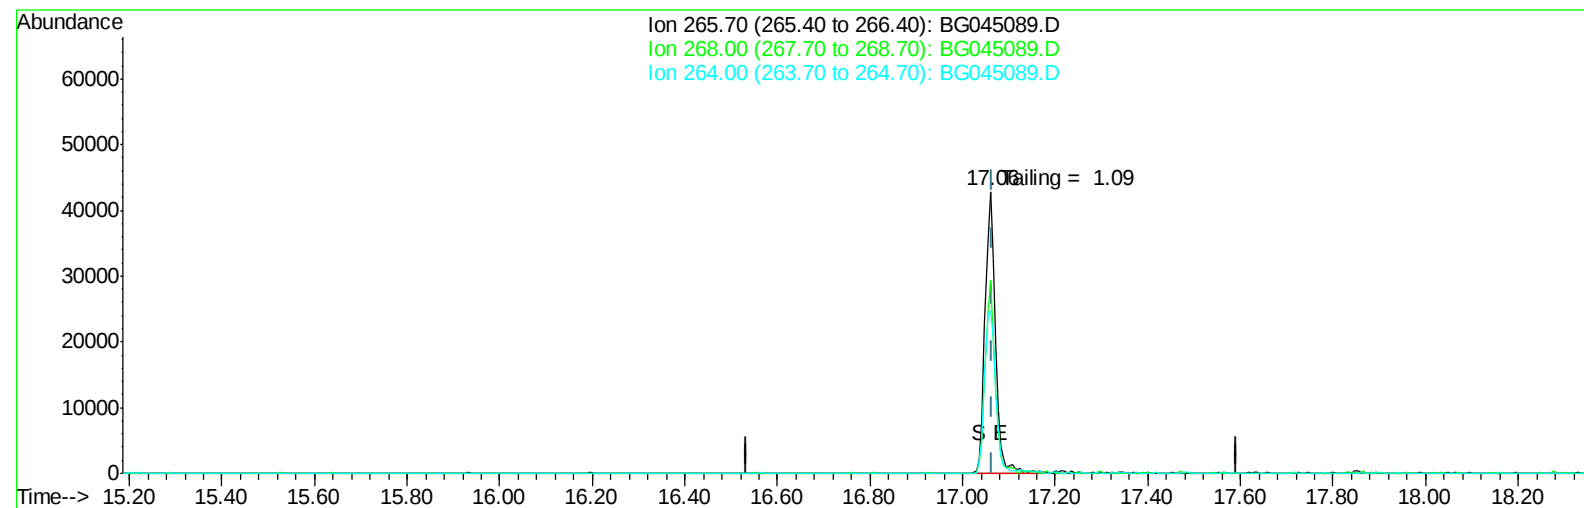




TIC: BG045089.D

(70) Pentachlorophenol (C)
 16.196min (-0.867) 109.65ng
 response 63

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	0.00#
264.00	65.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG042020\
 Data File : BG045089.D
 Acq On : 20 Apr 2020 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 05:46:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 20 11:57:28 2020
 Response via : Initial Calibration

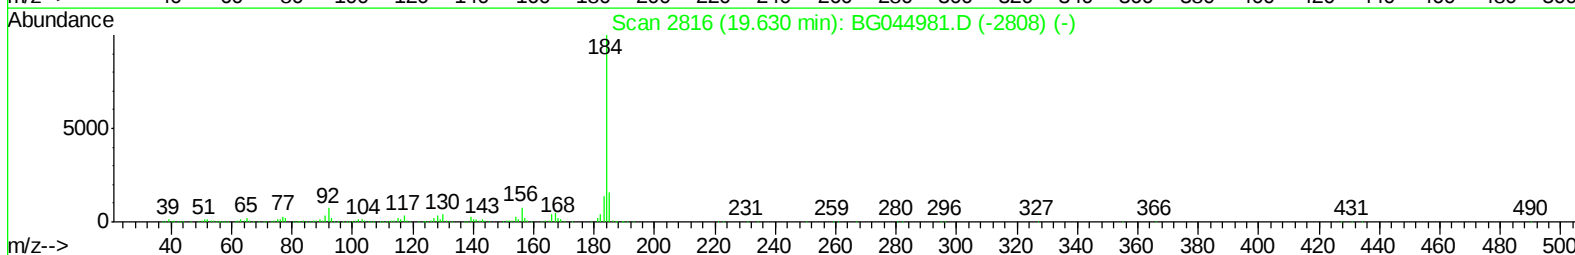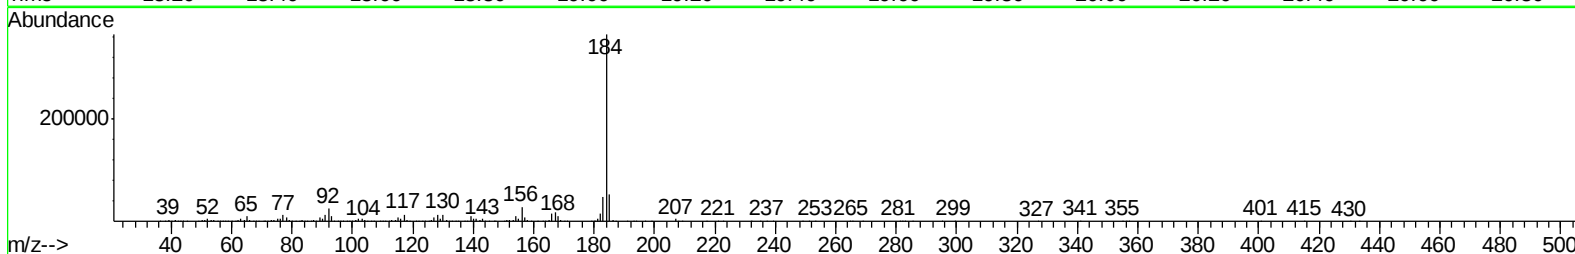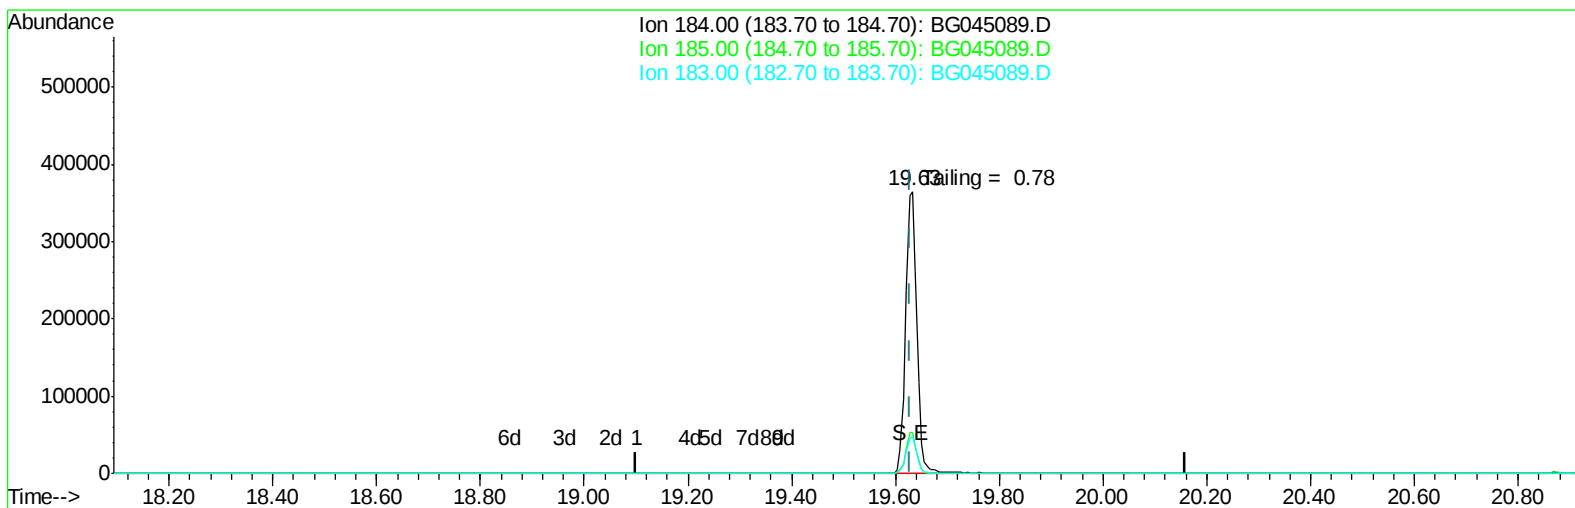

TIC: BG045089.D

(77) Benzidine

19.104min (-0.527) 5.55ng

response 83

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	126.38#
183.00	14.10	0.00#
0.00	0.00	0.00