


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042020\
 Data File : BG045089.D
 Acq On : 20 Apr 2020 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 20 11:57:28 2020

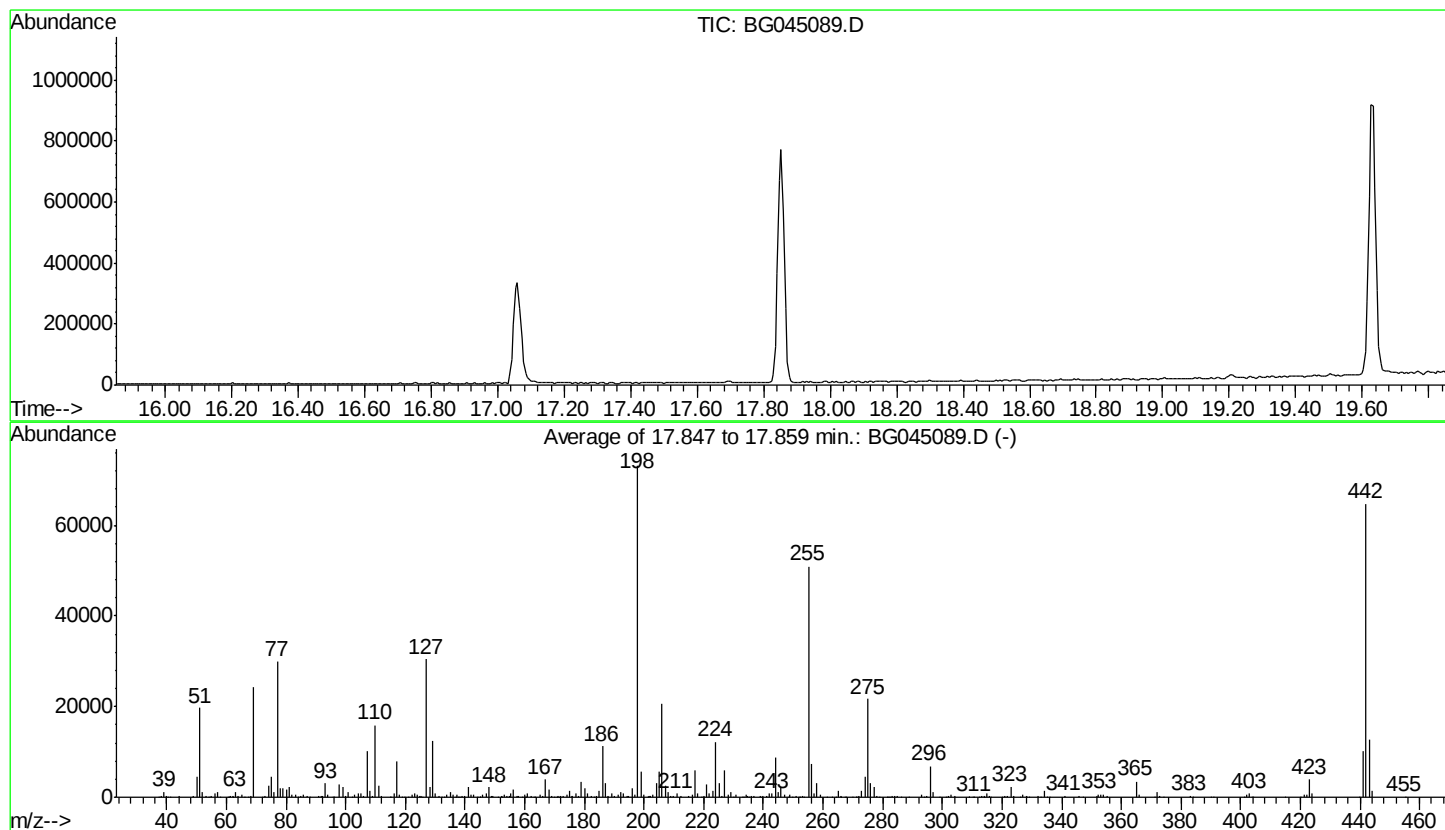

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	19744	PASS
68	69	0.00	2	0.9	220	PASS
69	198	0.00	100	33.3	24369	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	30485	PASS
197	198	0.00	2	0.8	598	PASS
198	198	100	100	100.0	73157	PASS
199	198	5	9	7.8	5683	PASS
275	198	10	60	29.7	21696	PASS
365	198	1	100	4.6	3392	PASS
441	198	0.01	100	14.1	10319	PASS
442	198	50	100	88.5	64736	PASS
443	442	15	24	19.7	12730	PASS