
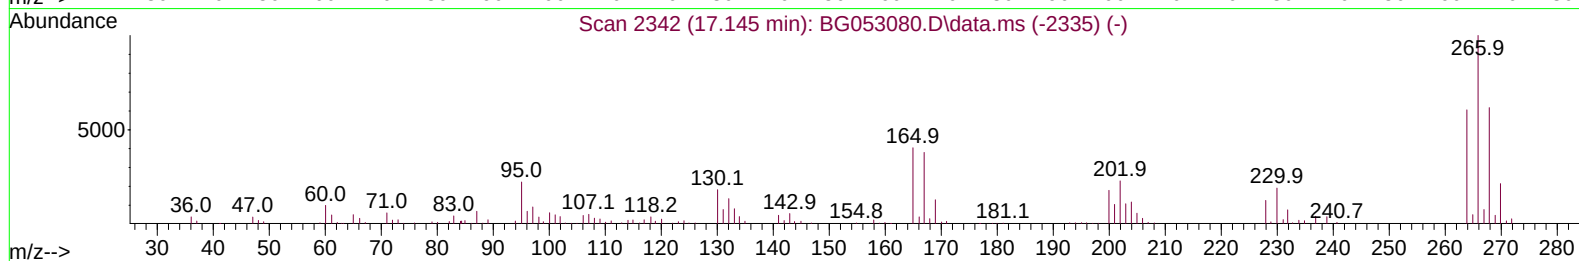
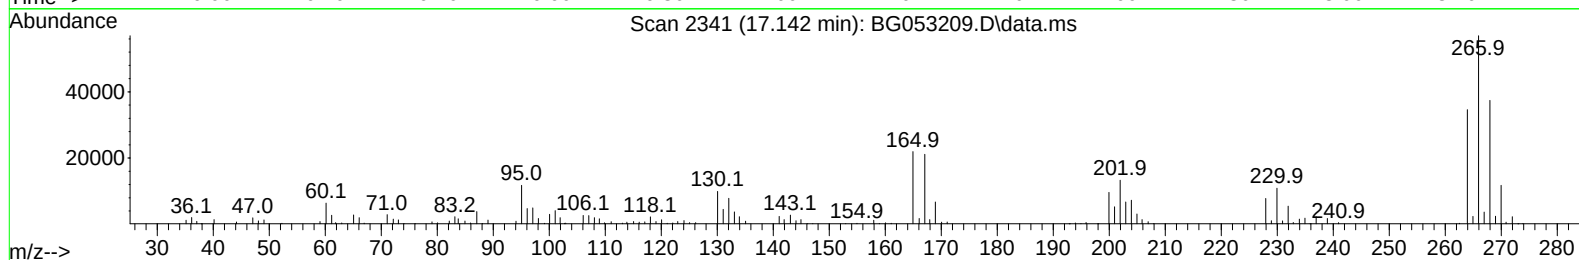


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053209.D
Acq On : 20 Apr 2022 9:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 18:40:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

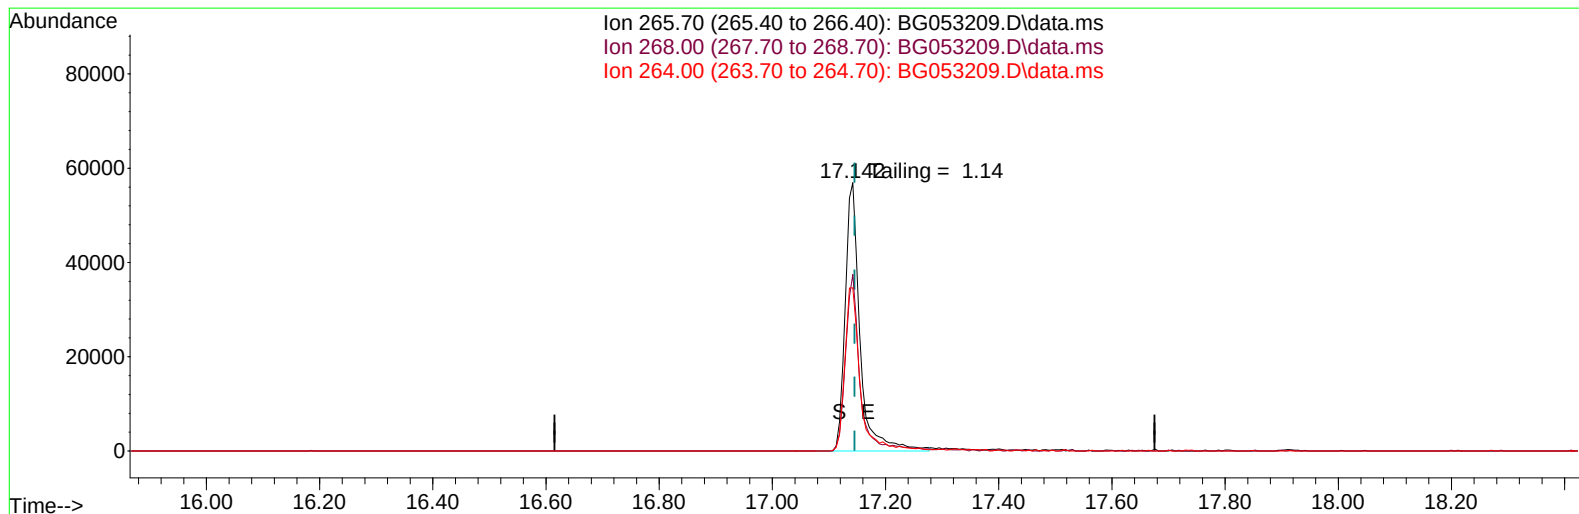

TIC: BG053209.D\data.ms

(70) Pentachlorophenol (C)




17.142min (-0.003) 23091.91 ng

response 103674

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.75
264.00	56.60	60.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053209.D
Acq On : 20 Apr 2022 9:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 18:40:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

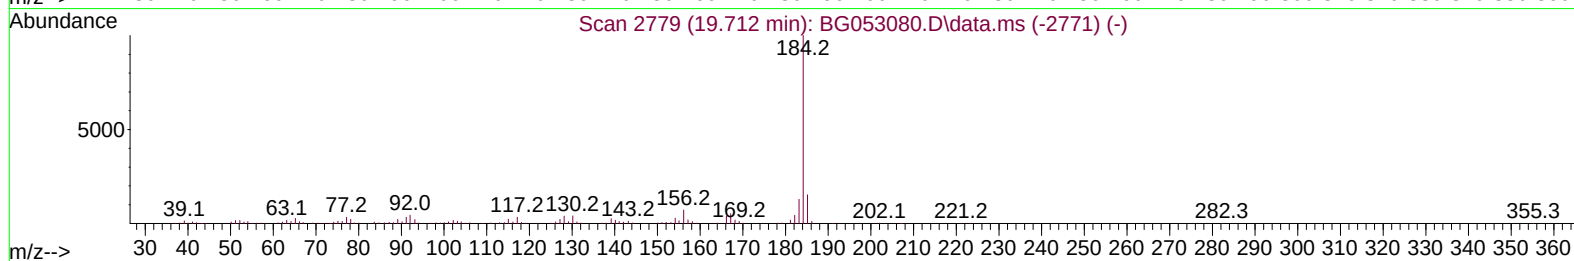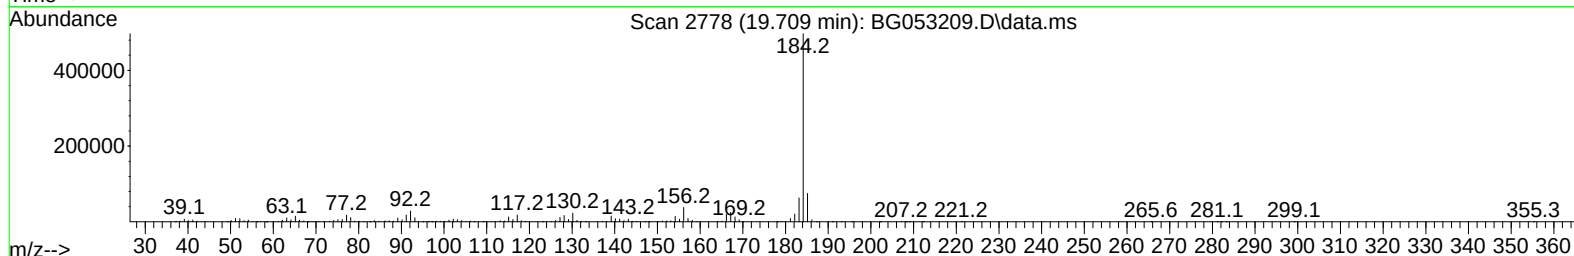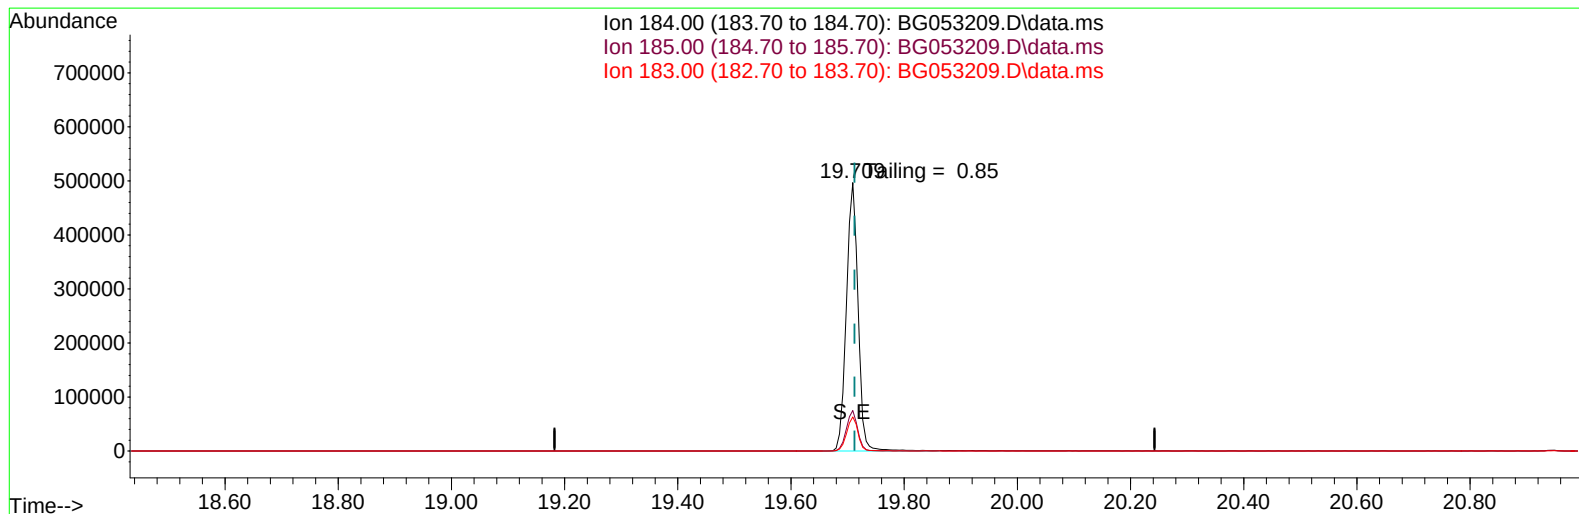

TIC: BG053209.D\data.ms

(77) Benzidine

19.709min (-0.003) 444892.11 ng

response 710835

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.08
183.00	11.80	12.74
0.00	0.00	0.00