
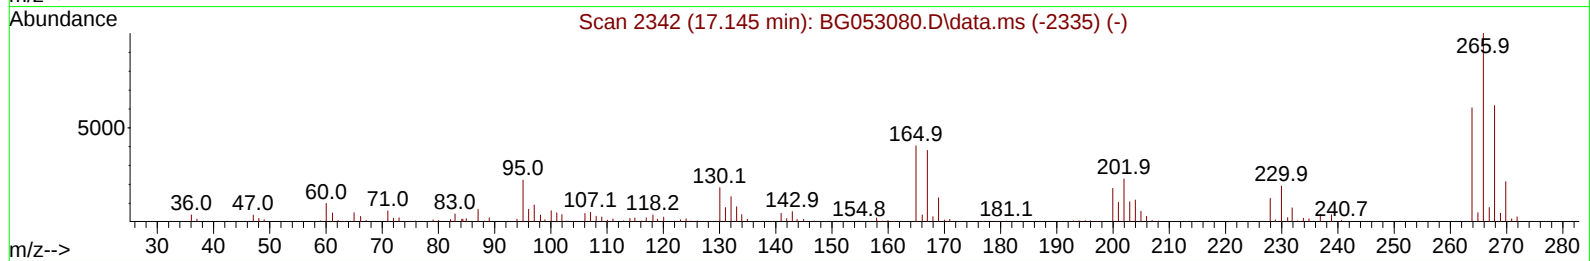
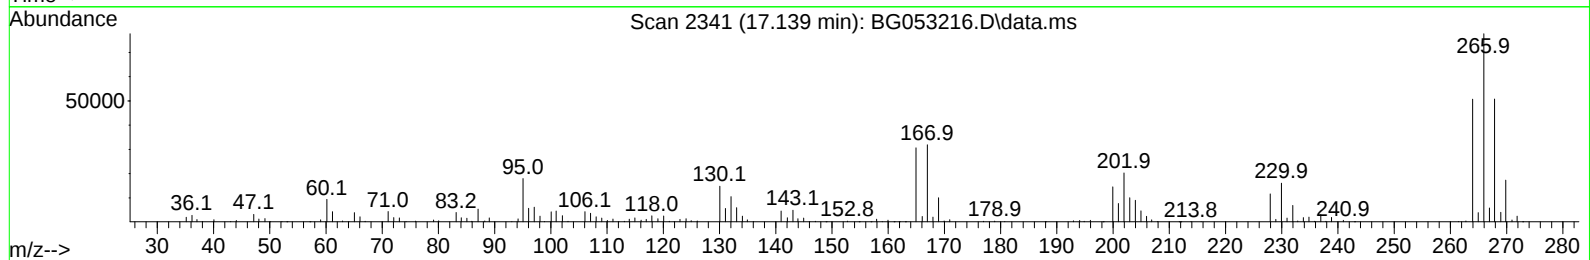


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053216.D
Acq On : 20 Apr 2022 15:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 15:54:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

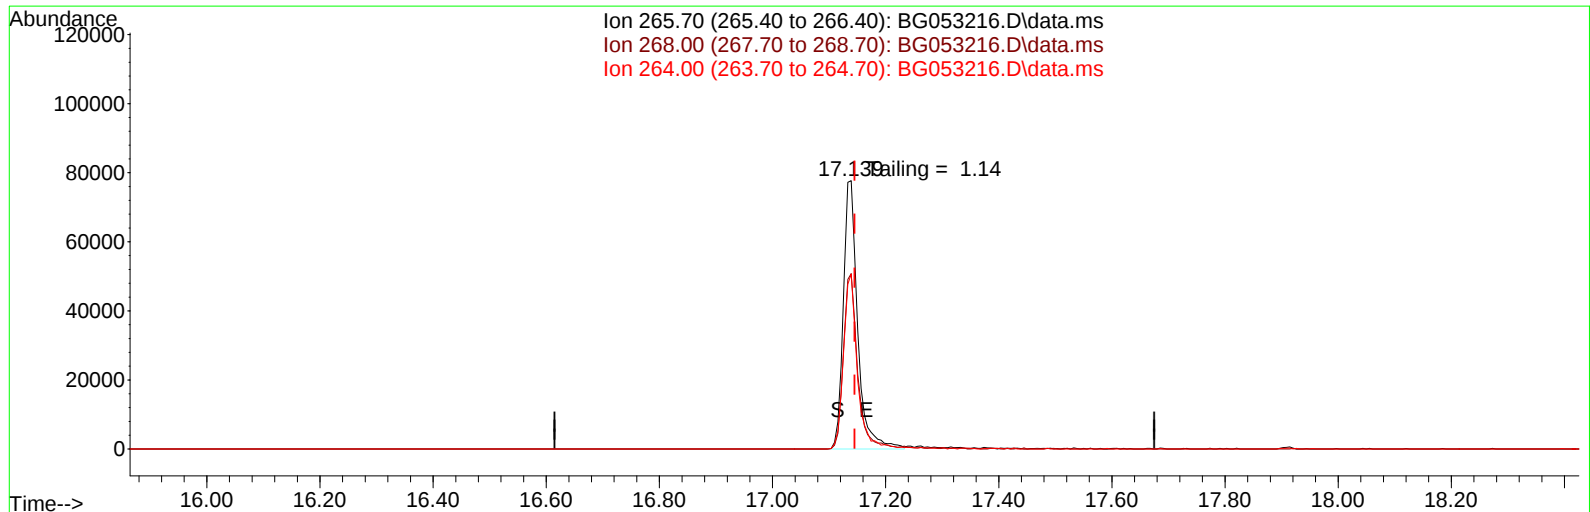

TIC: BG053216.D\data.ms

(70) Pentachlorophenol (C)




17.139min (-0.006) 282842.98 ng

response 137282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.36
264.00	56.60	65.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
 Data File : BG053216.D
 Acq On : 20 Apr 2022 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 15:54:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

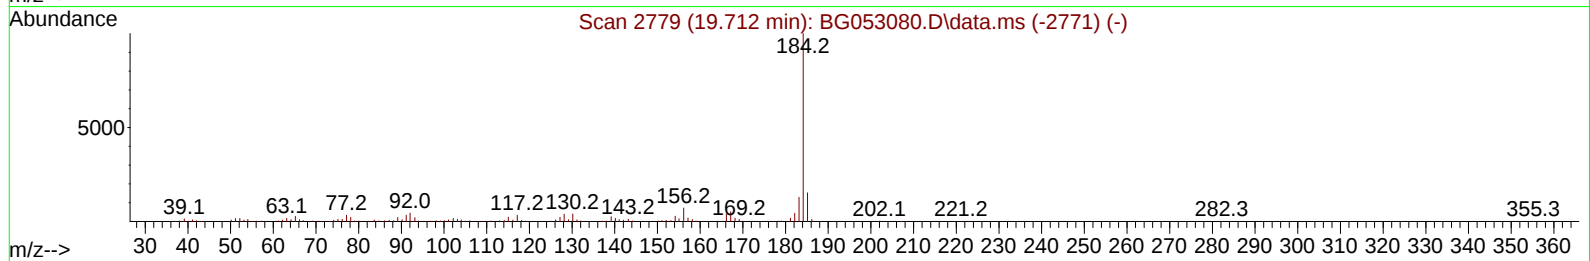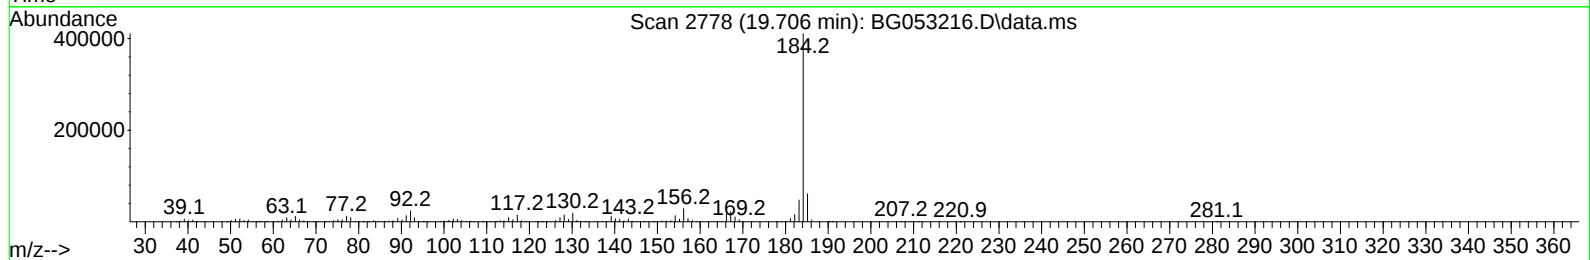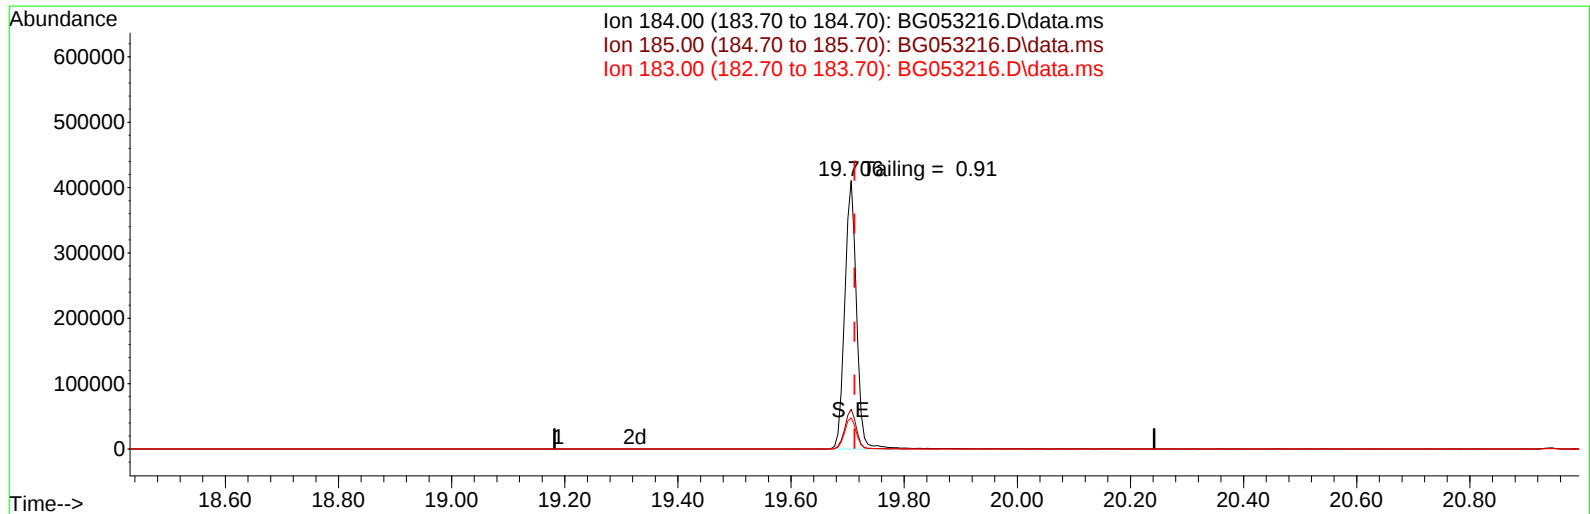

TIC: BG053216.D\data.ms

(77) Benzidine

19.706min (-0.006) 3171.48 ng m

response 590611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.83
183.00	11.80	11.60
0.00	0.00	0.00