

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
 Data File : BG053227.D
 Acq On : 20 Apr 2022 22:27
 Operator : CG/JU
 Sample : N2451-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-1120

Quant Time: Apr 21 06:05:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.116	152	36381	20.000	ng	0.00
21) Naphthalene-d8	10.924	136	141034	20.000	ng	-0.01
39) Acenaphthene-d10	14.737	164	98416	20.000	ng	-0.01
64) Phenanthrene-d10	17.480	188	228746	20.000	ng	#-0.01
76) Chrysene-d12	21.763	240	226772	20.000	ng	-0.01
86) Perylene-d12	25.064	264	233956	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.684	112	232705	109.645	ng	0.00
7) Phenol-d6	7.276	99	339466	103.721	ng	0.00
23) Nitrobenzene-d5	9.274	82	247064	71.129	ng	-0.01
42) 2,4,6-Tribromophenol	16.223	330	164592	105.120	ng	-0.01
45) 2-Fluorobiphenyl	13.362	172	529120	74.135	ng	0.00
79) Terphenyl-d14	20.083	244	965490	71.906	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053227.D
Acq On : 20 Apr 2022 22:27
Operator : CG/JU
Sample : N2451-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-1120

Quant Time: Apr 21 06:05:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration




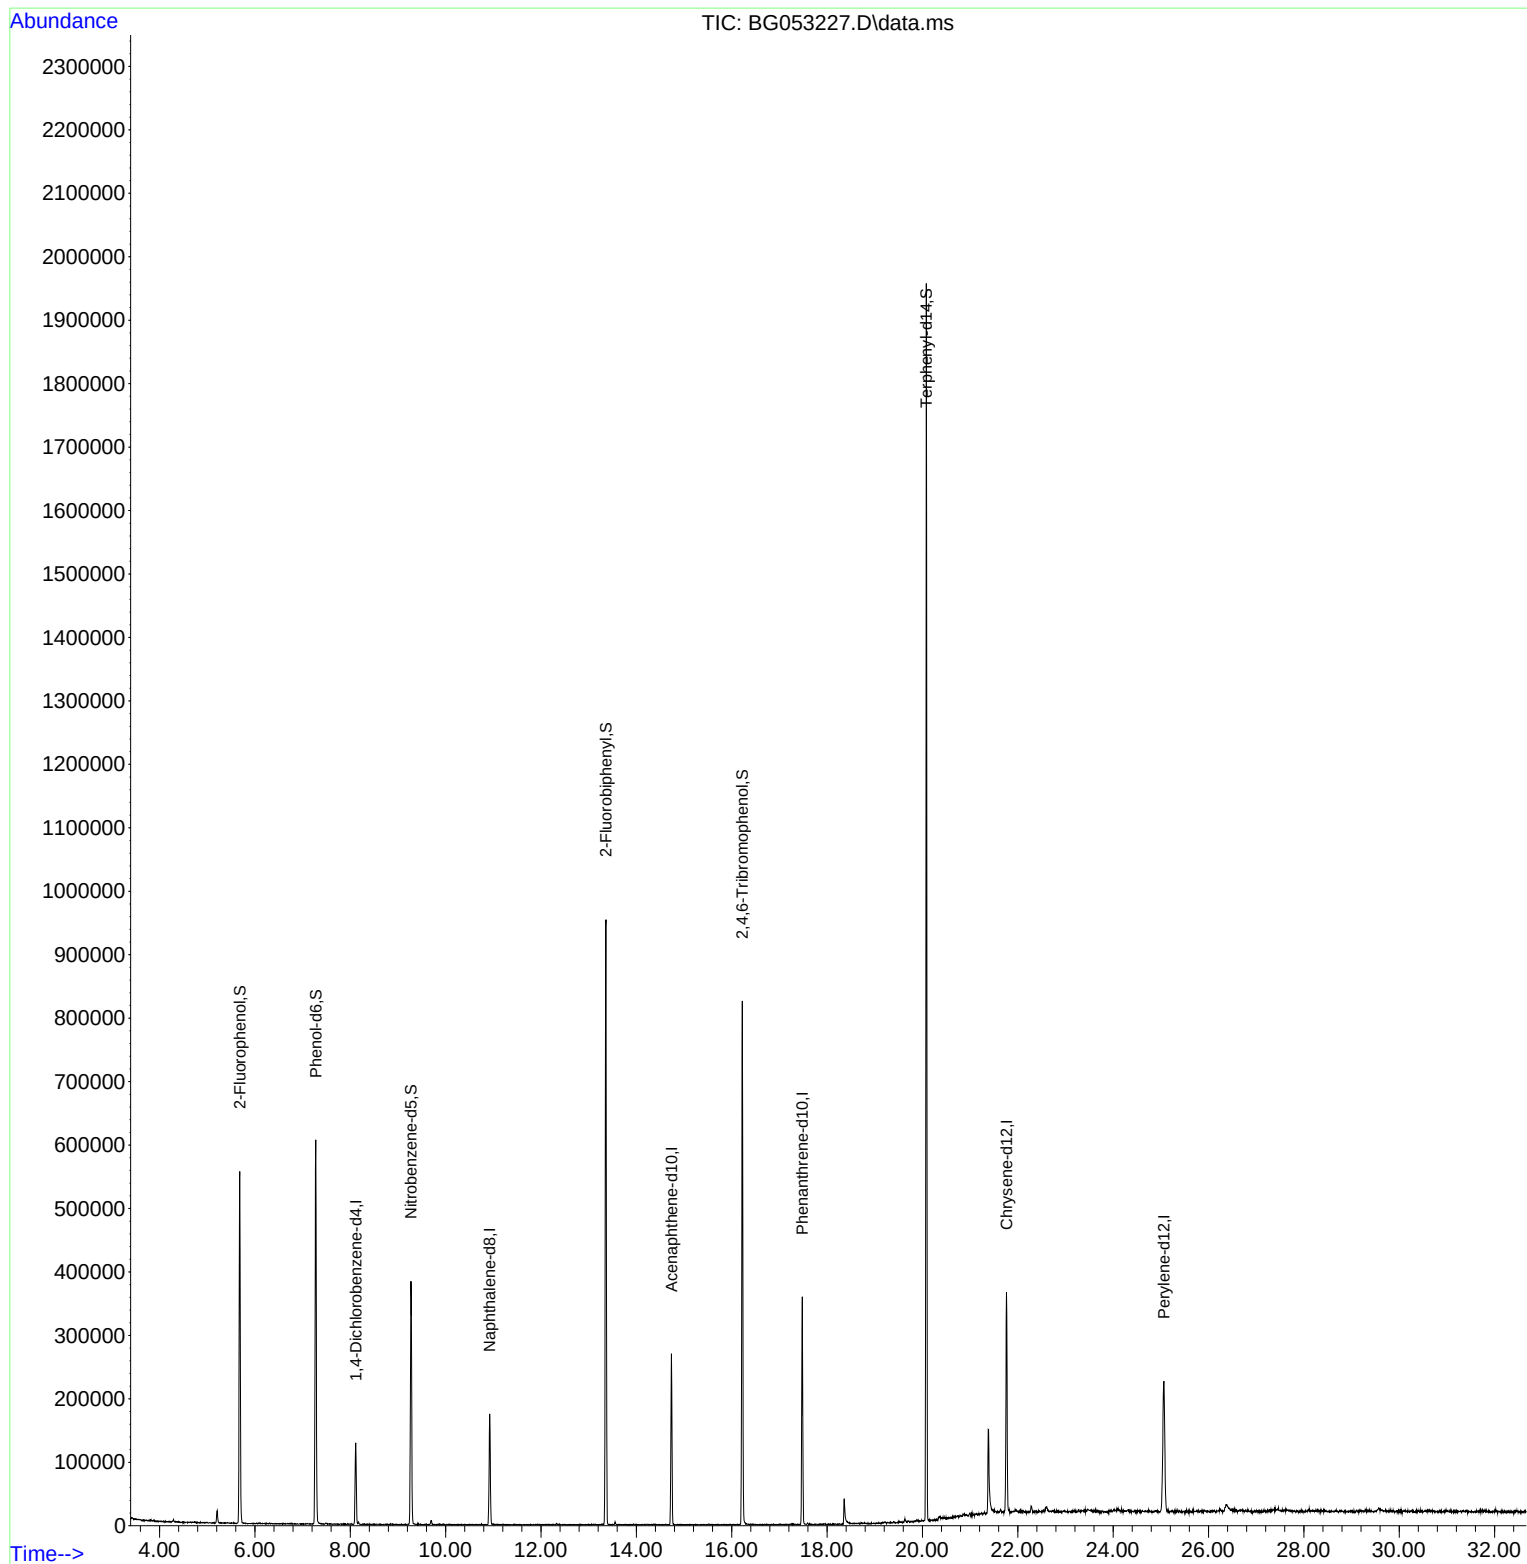


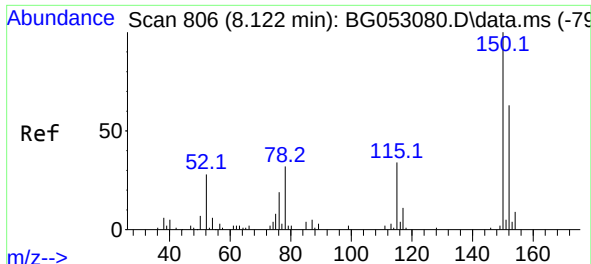

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.116 min Scan# 805
Delta R.T. -0.006 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27




Instrument :
BNA_G
ClientSampleId :
SB-1120


Tgt Ion:152 Resp: 36381
Ion Ratio Lower Upper
152 100
150 155.5 114.6 172.0
115 53.3 45.9 68.9

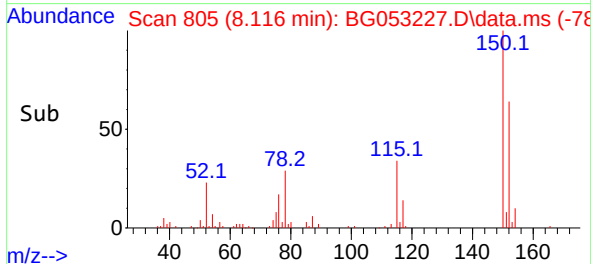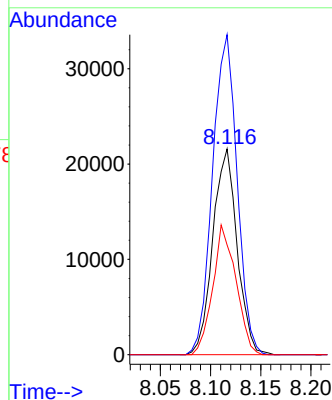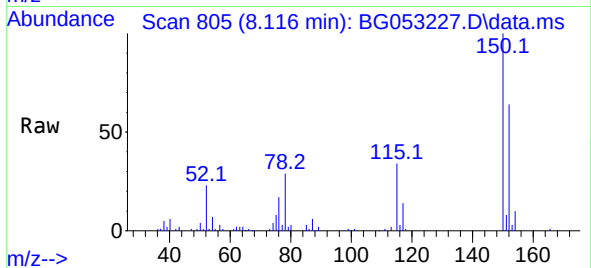

#5
2-Fluorophenol
Concen: 109.645 ng
RT: 5.684 min Scan# 391
Delta R.T. 0.000 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27

Tgt Ion:112 Resp: 232705
Ion Ratio Lower Upper
112 100
64 66.9 48.0 72.0
63 38.9 26.5 39.7


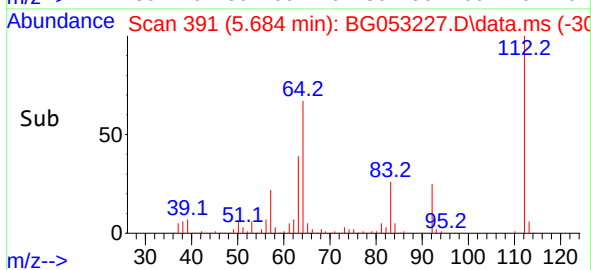
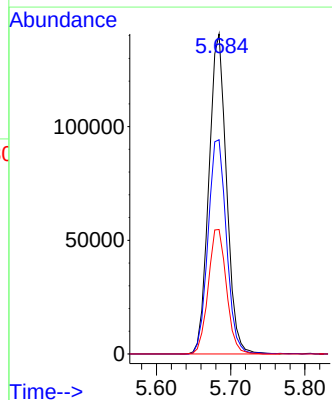
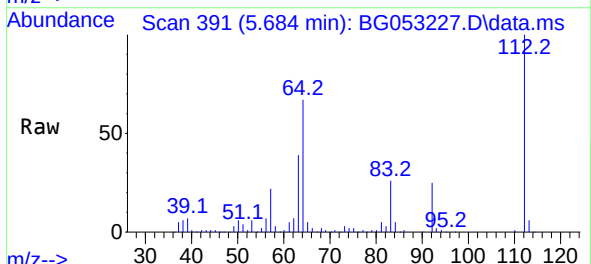




#7
Phenol-d6
Concen: 103.721 ng
RT: 7.276 min Scan# 60
Delta R.T. -0.005 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27




Instrument :
BNA_G
ClientSampleId :
SB-1120


Tgt Ion: 99 Resp: 339466
Ion Ratio Lower Upper
99 100
42 20.5 14.7 22.1
71 42.5 29.2 43.8

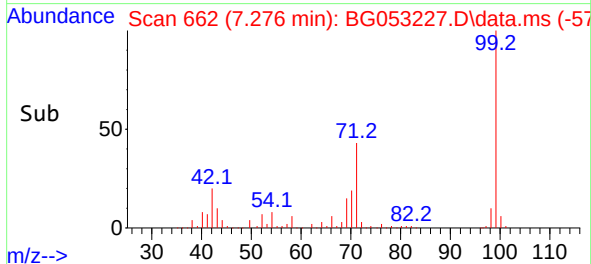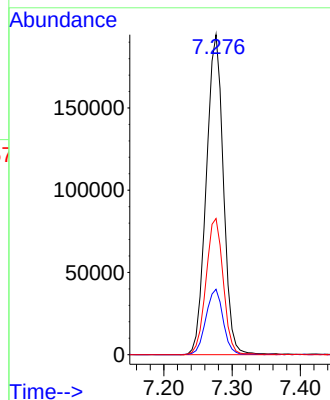

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.924 min Scan# 1283
Delta R.T. -0.012 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27

Tgt Ion: 136 Resp: 141034
Ion Ratio Lower Upper
136 100
137 11.6 9.4 14.2
54 9.5 6.4 9.6
68 7.2 5.0 7.6


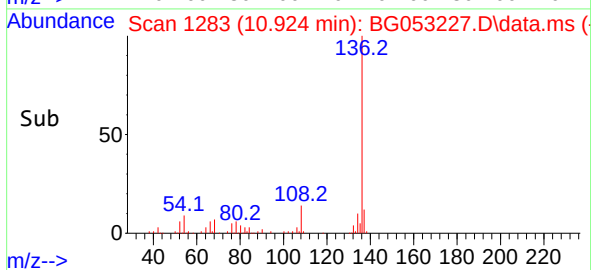
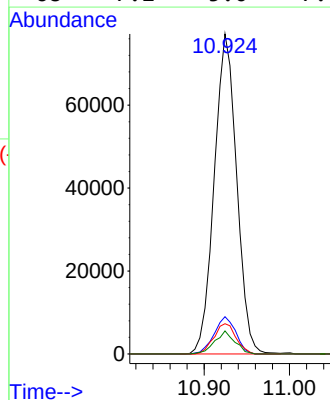
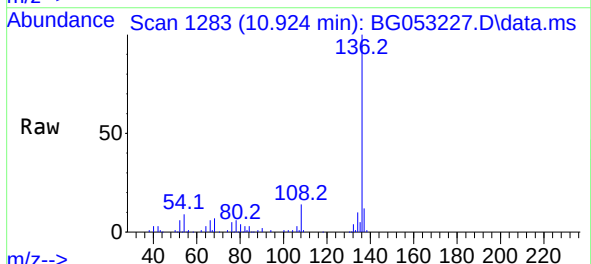




#23
Nitrobenzene-d5
Concen: 71.129 ng
RT: 9.274 min Scan# 1002
Delta R.T. -0.011 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27




Instrument :
BNA_G
ClientSampleId :
SB-1120


Tgt Ion: 82 Resp: 247064
Ion Ratio Lower Upper
82 100
128 35.0 31.3 46.9
54 49.9 37.8 56.8

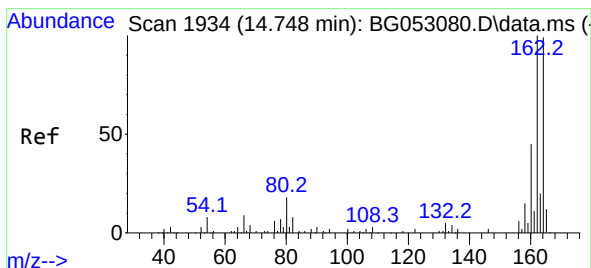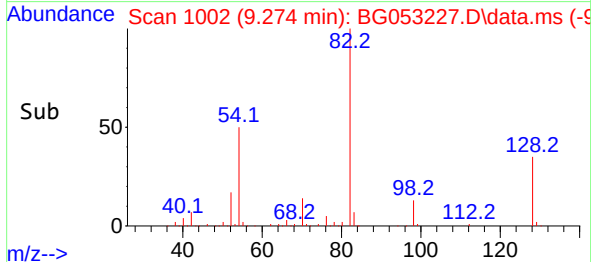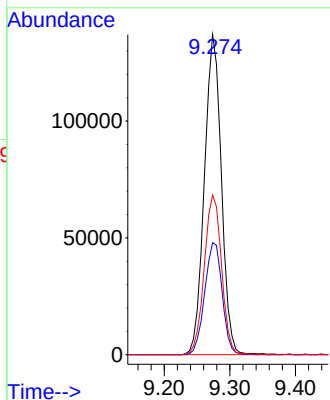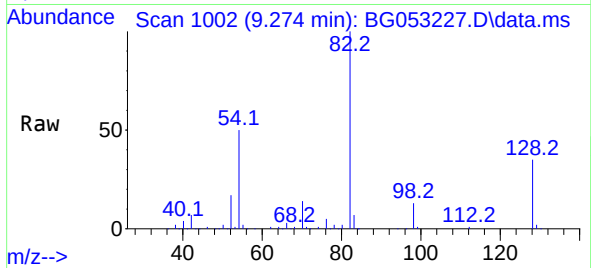

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.737 min Scan# 1932
Delta R.T. -0.011 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27


Tgt Ion:164 Resp: 98416
Ion Ratio Lower Upper
164 100
162 103.1 80.0 120.0
160 43.0 38.8 58.2

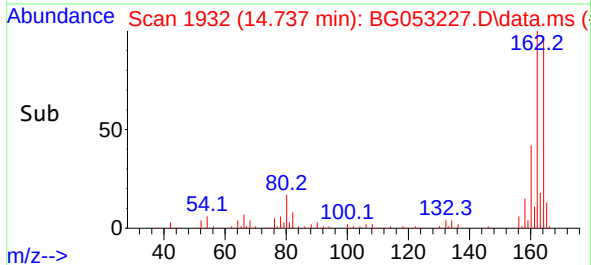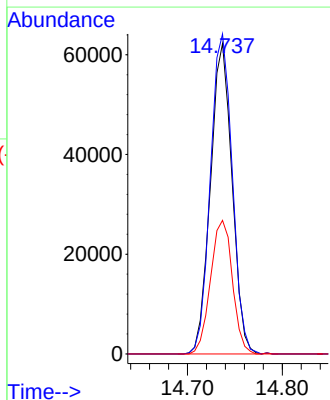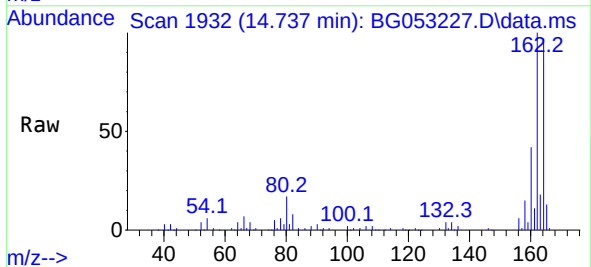



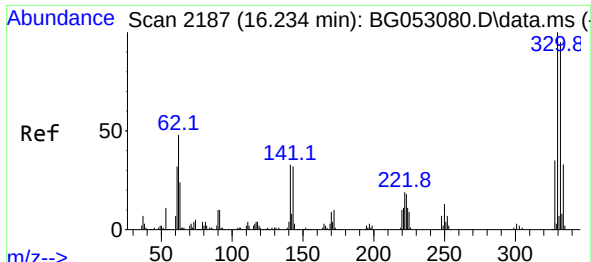


#42
2,4,6-Tribromophenol
Concen: 105.120 ng
RT: 16.223 min Scan# 2185
Delta R.T. -0.011 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27

Instrument :
BNA_G
ClientSampleId :
SB-1120



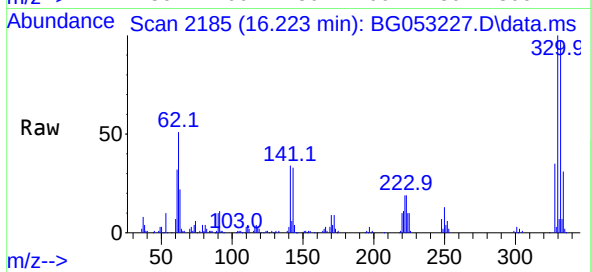



Tgt Ion:330 Resp: 164592
Ion Ratio Lower Upper
330 100
332 96.2 75.8 113.6
141 33.6 24.6 36.8

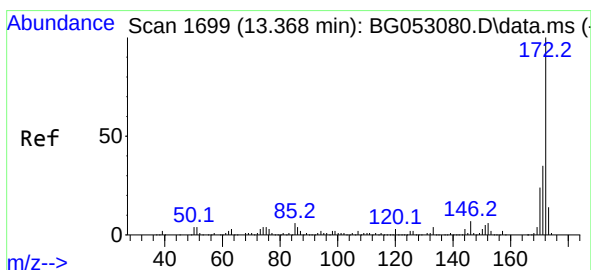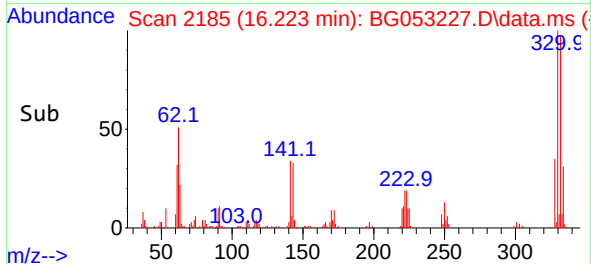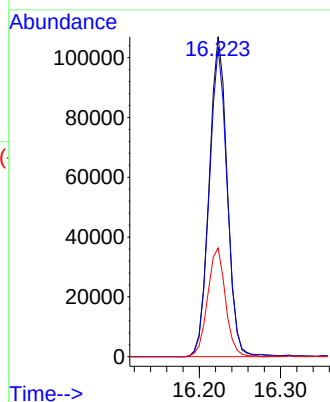

#45
2-Fluorobiphenyl
Concen: 74.135 ng
RT: 13.362 min Scan# 1698
Delta R.T. -0.005 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27

Tgt Ion:172 Resp: 529120
Ion Ratio Lower Upper
172 100
171 35.3 28.3 42.5
170 23.2 18.0 27.0


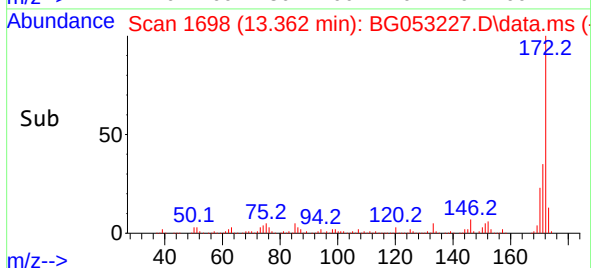
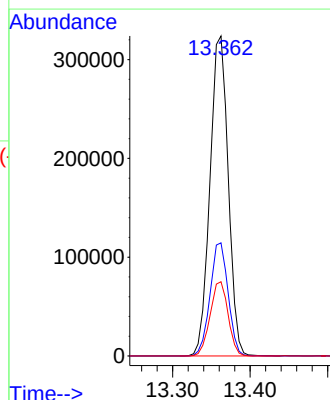
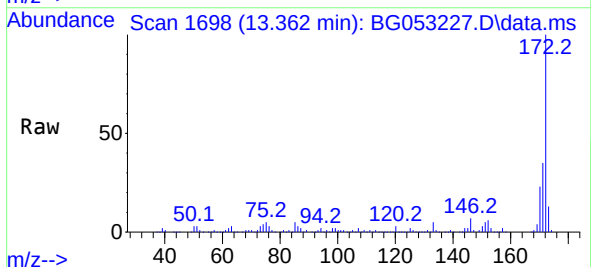




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.480 min Scan# 21
Delta R.T. -0.011 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27




Instrument :
BNA_G
ClientSampleId :
SB-1120


Tgt Ion:188 Resp: 228746
Ion Ratio Lower Upper
188 100
94 6.4 5.7 8.5
80 6.8 7.2 10.8#

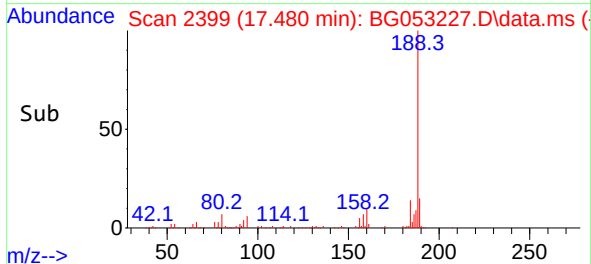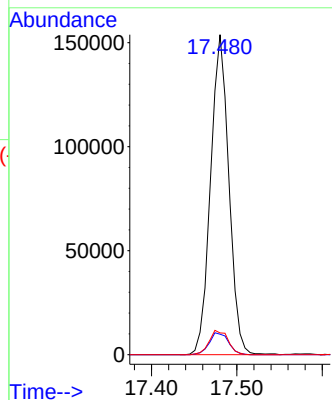

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.763 min Scan# 3128
Delta R.T. -0.011 min
Lab File: BG053227.D
Acq: 20 Apr 2022 22:27


Tgt Ion:240 Resp: 226772
Ion Ratio Lower Upper
240 100
120 6.6 5.4 8.0
236 25.2 19.8 29.6

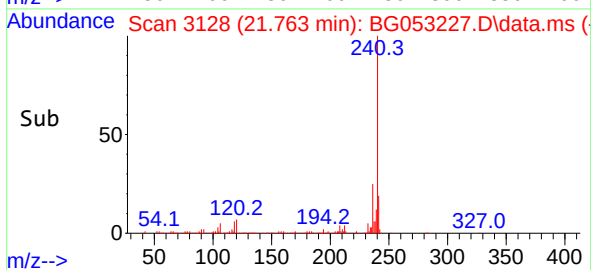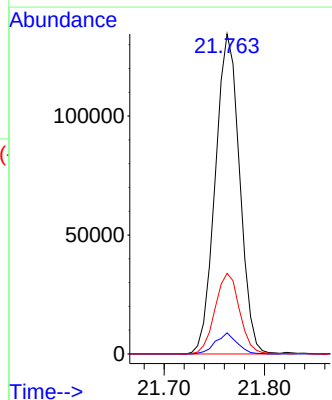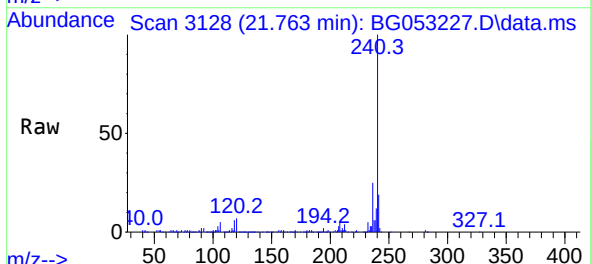



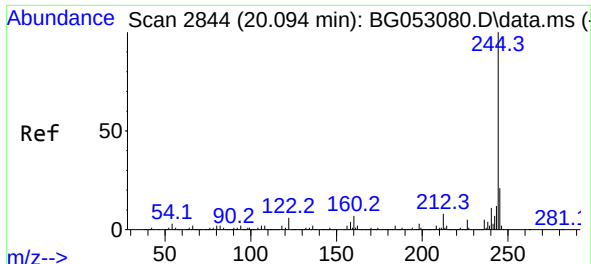


#79
 Terphenyl-d14
 Concen: 71.906 ng
 RT: 20.083 min Scan# 21
 Delta R.T. -0.011 min
 Lab File: BG053227.D
 Acq: 20 Apr 2022 22:27

Instrument :
 BNA_G
 ClientSampleId :
 SB-1120



Tgt Ion:244 Resp: 965490
 Ion Ratio Lower Upper
 244 100
 212 7.6 5.4 8.2
 122 6.5 5.8 8.6

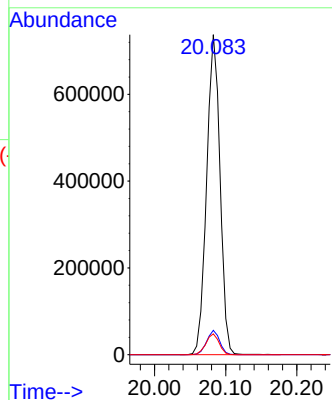

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.064 min Scan# 3690
 Delta R.T. -0.011 min
 Lab File: BG053227.D
 Acq: 20 Apr 2022 22:27

Tgt Ion:264 Resp: 233956
 Ion Ratio Lower Upper
 264 100
 260 22.8 18.2 27.2
 265 20.8 15.1 22.7

