

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
 Data File : BG053229.D
 Acq On : 20 Apr 2022 23:44
 Operator : CG/JU
 Sample : N2432-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FB220414

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.206	303	309	315	rBV2	59677	95288	3.33%	0.922%
2	5.682	383	390	402	rVB	262725	449338	15.71%	4.350%
3	7.274	654	661	668	rBV	159977	283556	9.92%	2.745%
4	8.114	797	804	811	rBV	132641	224911	7.86%	2.177%
5	9.277	991	1002	1017	rBV	443064	822056	28.75%	7.958%
6	10.922	1273	1282	1290	rBV	162432	302137	10.57%	2.925%
7	13.360	1688	1697	1704	rBV	1175858	1795663	62.79%	17.383%
8	14.735	1923	1931	1939	rBV	259808	418509	14.63%	4.051%
9	16.221	2177	2184	2194	rBV	896497	1400163	48.96%	13.554%
10	17.478	2392	2398	2407	rBV	337996	519556	18.17%	5.030%
11	20.086	2835	2842	2849	rVB	2124820	2859654	100.00%	27.683%
12	21.760	3121	3127	3134	rBV2	344881	585178	20.46%	5.665%
13	25.062	3678	3689	3699	rBV	192533	573893	20.07%	5.556%




Sum of corrected areas: 10329902

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053229.D
Acq On : 20 Apr 2022 23:44
Operator : CG/JU
Sample : N2432-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB220414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

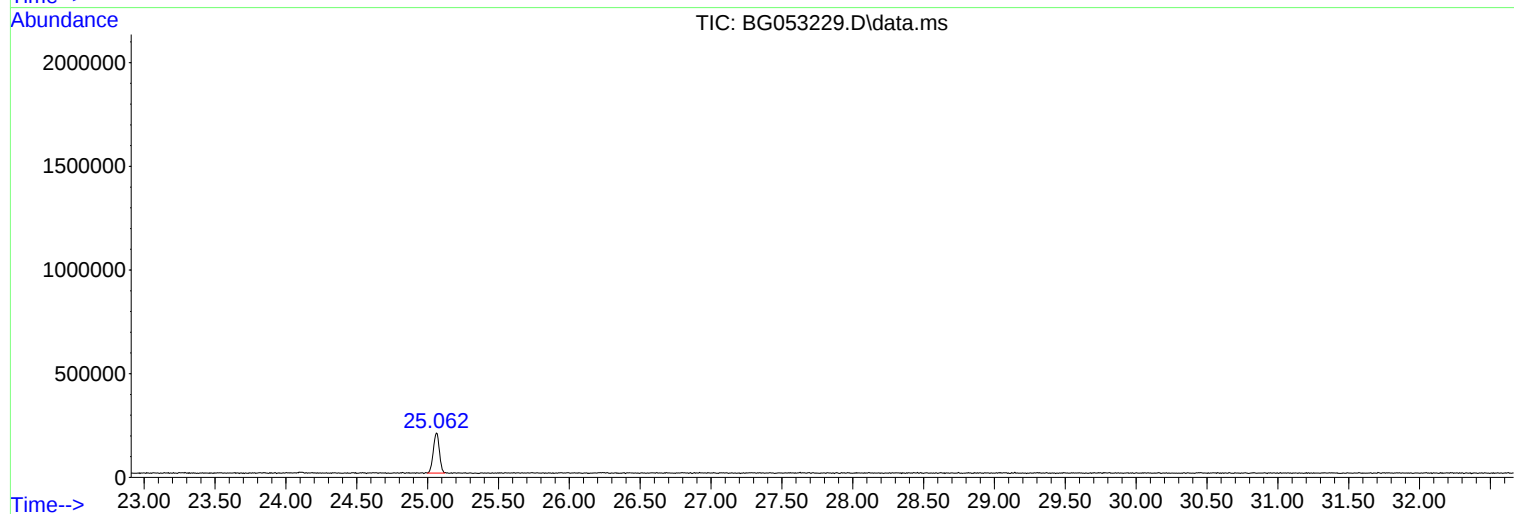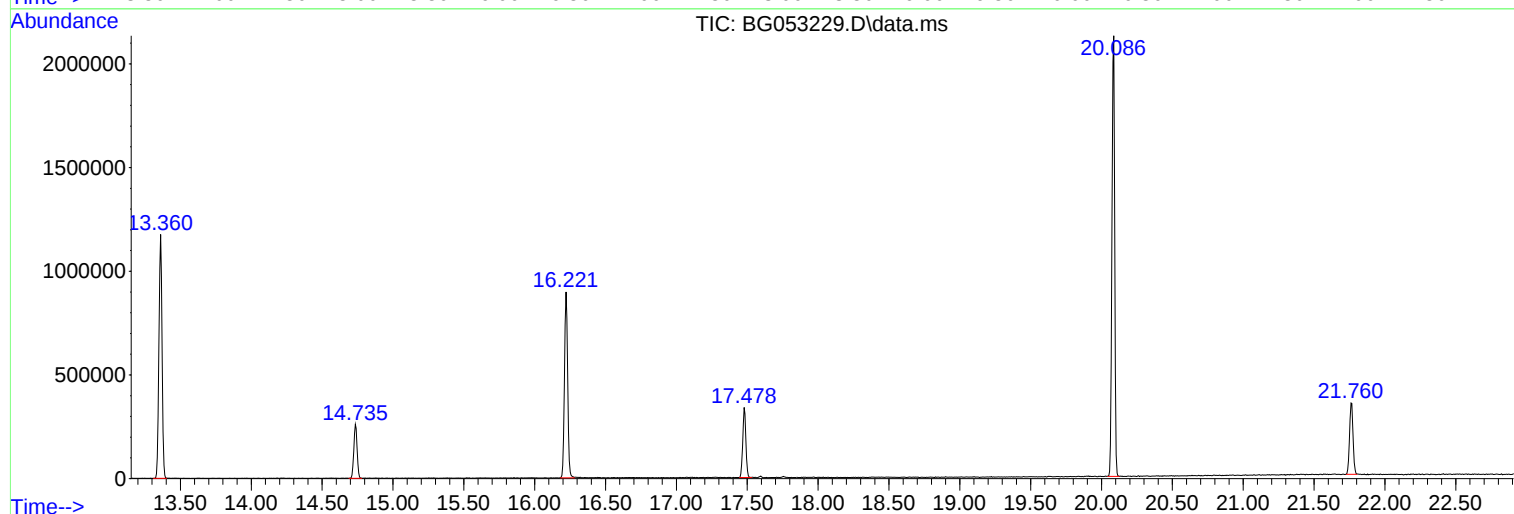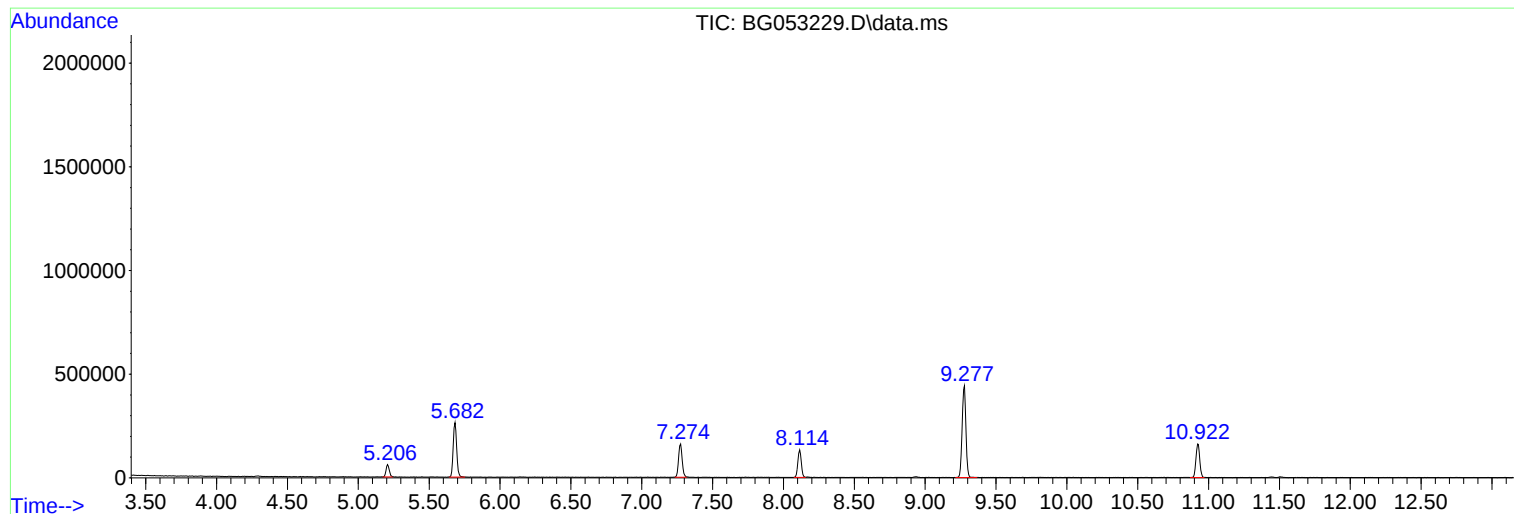

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053229.D
Acq On : 20 Apr 2022 23:44
Operator : CG/JU
Sample : N2432-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB220414










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.206	8.47 ng	95288	1,4-Dichlorobenzene-d4	8.114

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64	
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	37	
3	2-Nonanone, 9-hydroxy-	158	C9H18O2	025368-56-3	36	
4	4-Hydroxy-3-hexanone	116	C6H12O2	004984-85-4	25	
5	1,2-Butanediol	90	C4H10O2	000584-03-2	25	

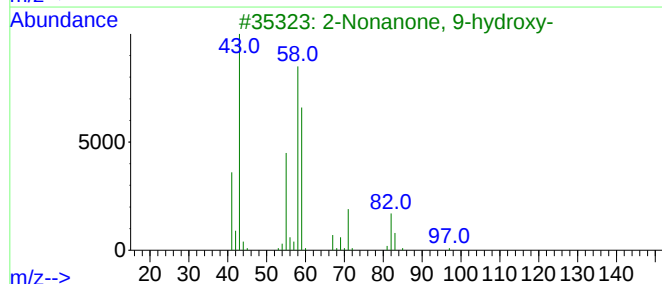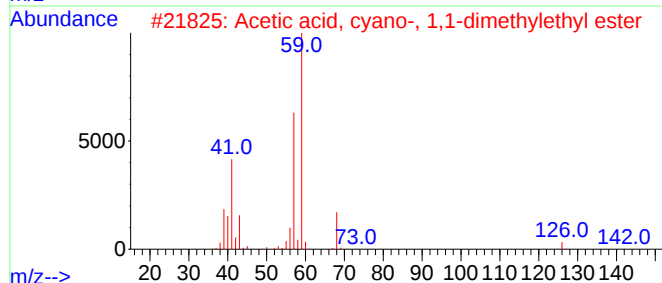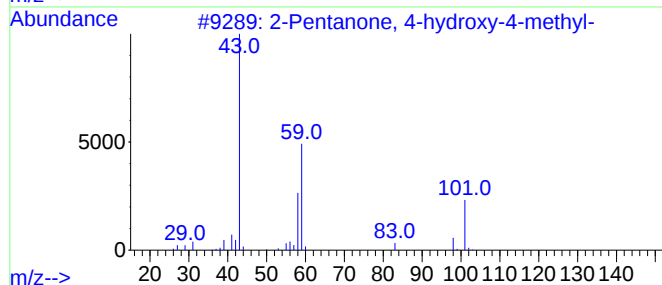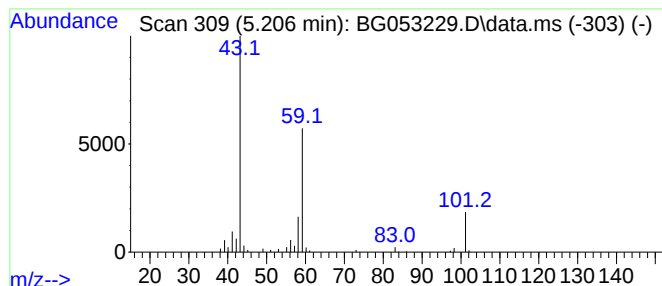

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053229.D
Acq On : 20 Apr 2022 23:44
Operator : CG/JU
Sample : N2432-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB220414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.206	8.5	ng	95288	1	8.114	224911	20.0