
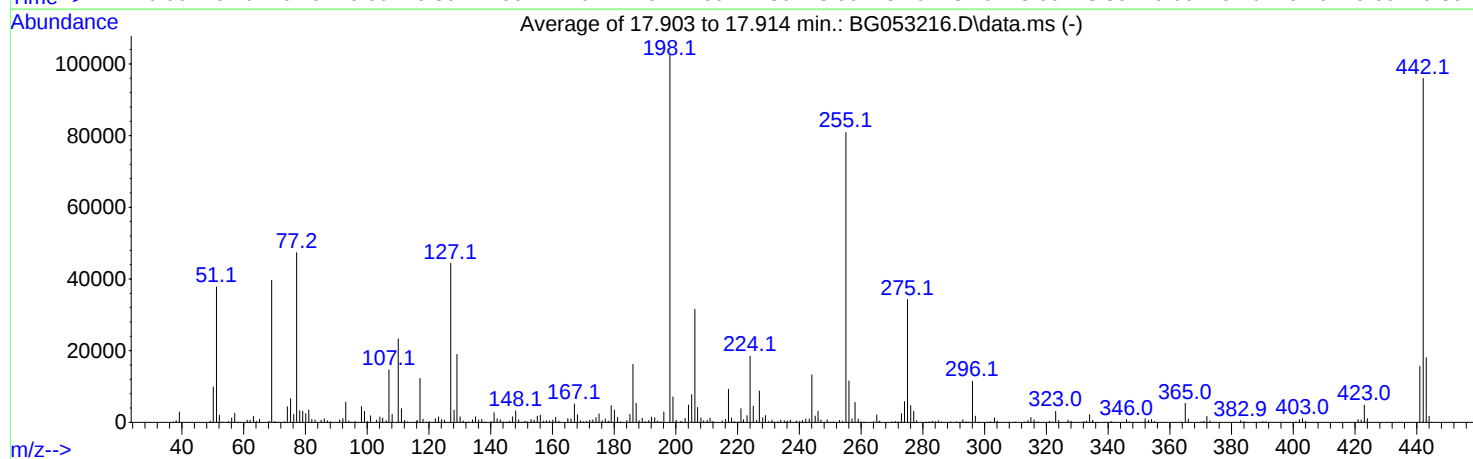


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
 Data File : BG053216.D
 Acq On : 20 Apr 2022 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

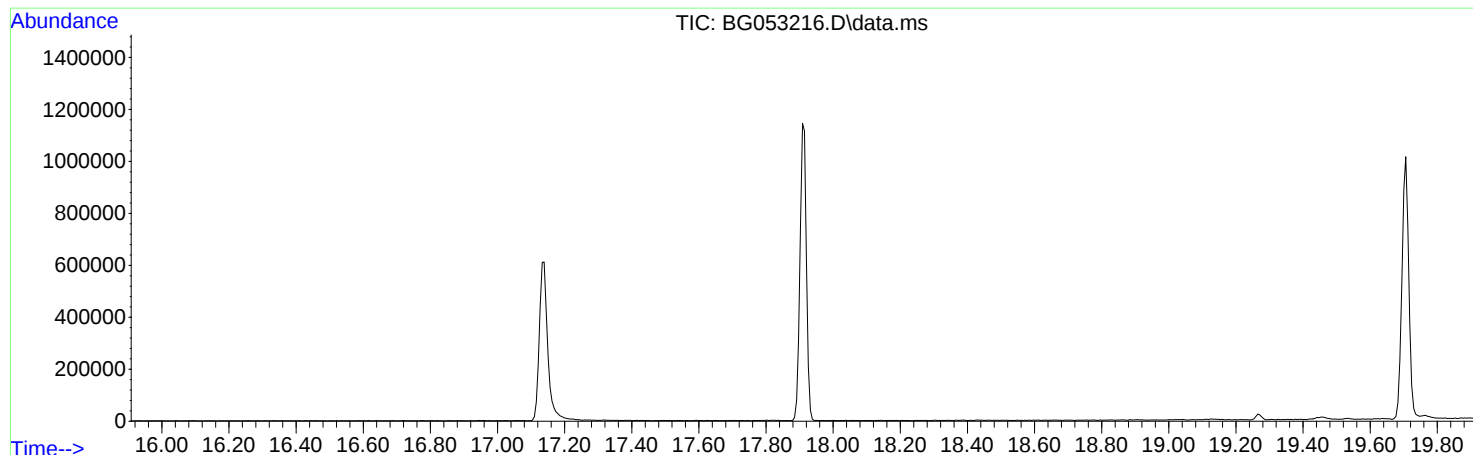




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	37779	PASS
68	69	0.00	2	0.8	308	PASS
69	198	0.00	100	38.6	39589	PASS
70	69	0.00	2	0.4	164	PASS
127	198	10	80	43.2	44363	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102621	PASS
199	198	5	9	6.9	7118	PASS
275	198	10	60	33.4	34296	PASS
365	198	1	100	5.2	5295	PASS
441	198	0.01	100	15.2	15609	PASS
442	442	50	100	100.0	95971	PASS
443	442	15	24	18.8	18057	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
 Data File : BG053216.D
 Acq On : 20 Apr 2022 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 20 15:54:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

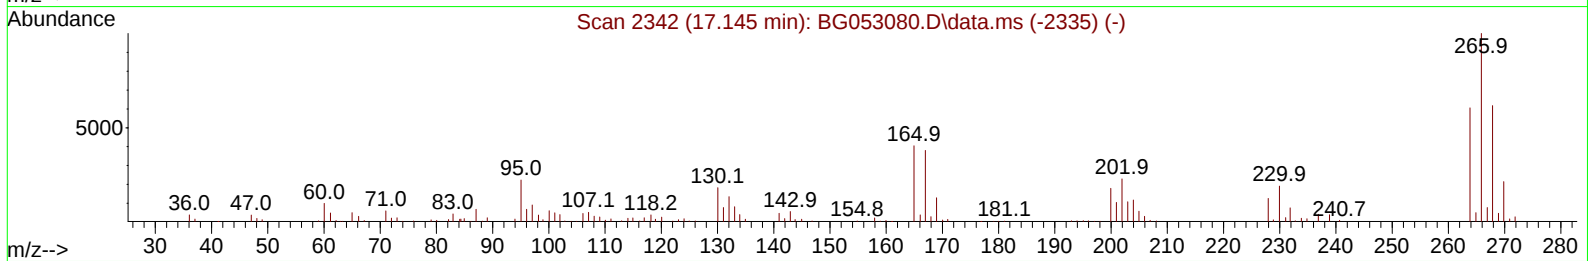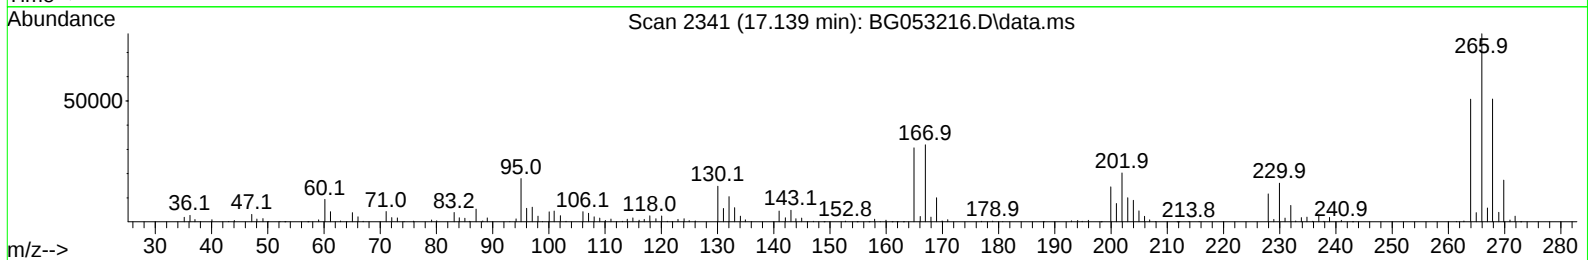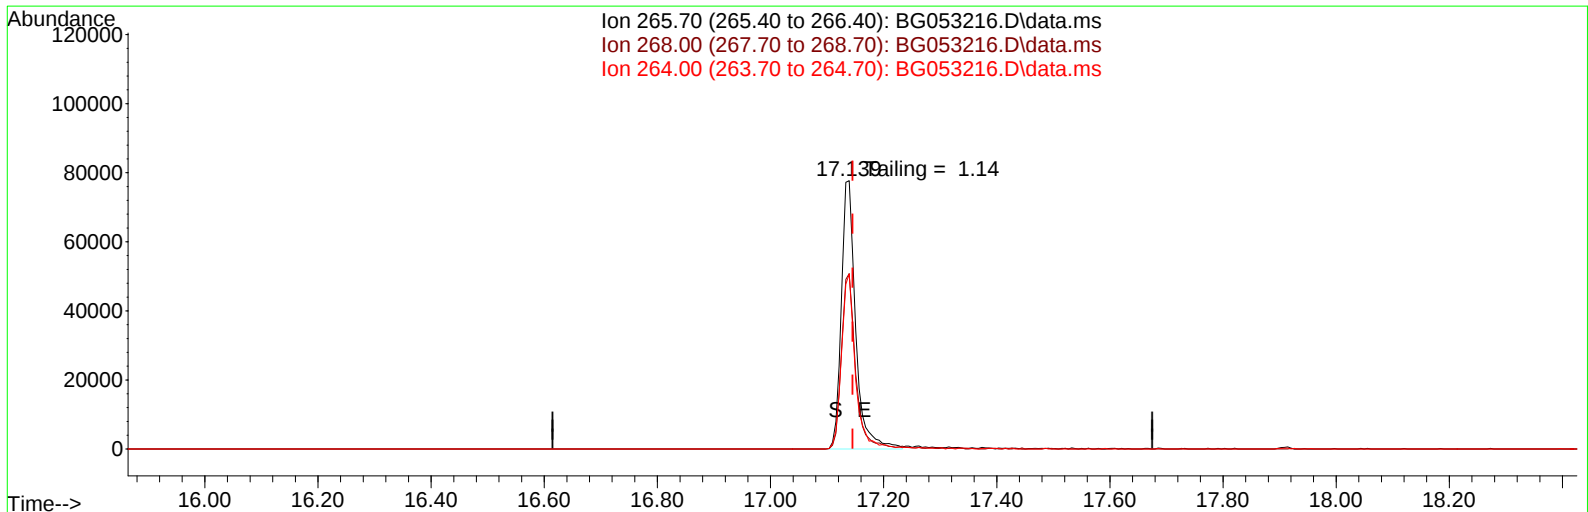

TIC: BG053216.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.006) 282842.98 ng




response 137282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.36
264.00	56.60	65.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042022\
Data File : BG053216.D
Acq On : 20 Apr 2022 15:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 20 15:54:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

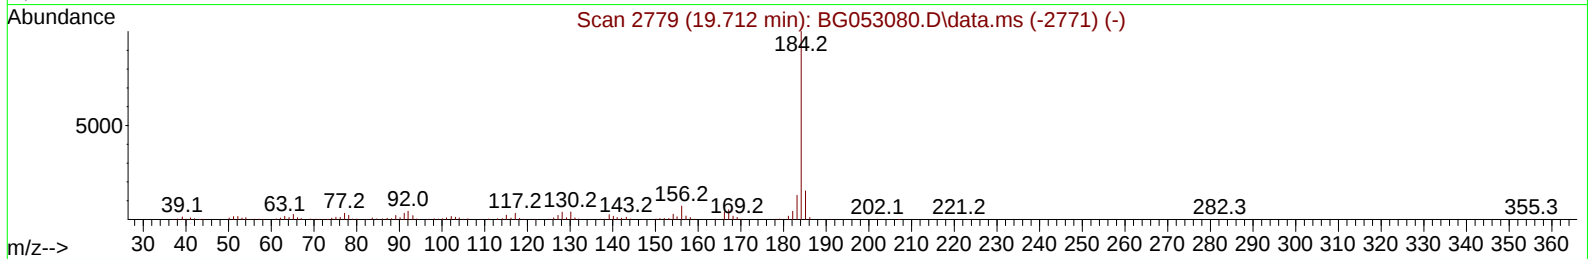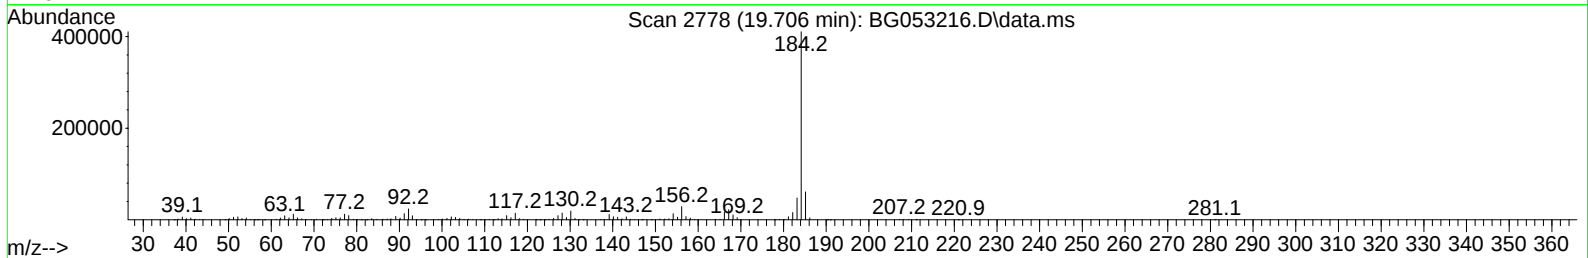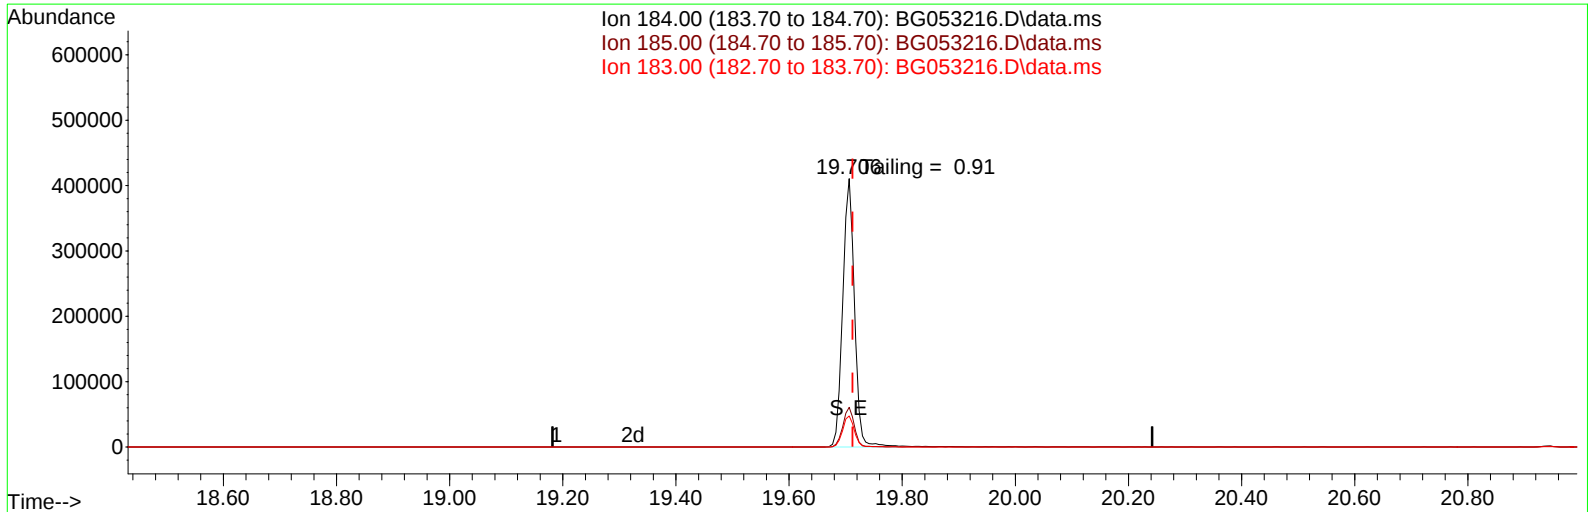

TIC: BG053216.D\data.ms

(77) Benzidine

19.706min (-0.006) 3171.48 ng m

response 590611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.83
183.00	11.80	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/20/2022	BNA_G	<u>BG053216.D</u>
Compound Name	Response	Retention Time
DDT	402614	20.946
DDD	6804	20.499
DDE	415	19.994
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7219	409833	1.76

Instrument :
BNA_G
ClientSampleId :
DFTPP