


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG042120\
 Data File : BG045105.D
 Acq On : 21 Apr 2020 10:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 22 12:56:37 2020

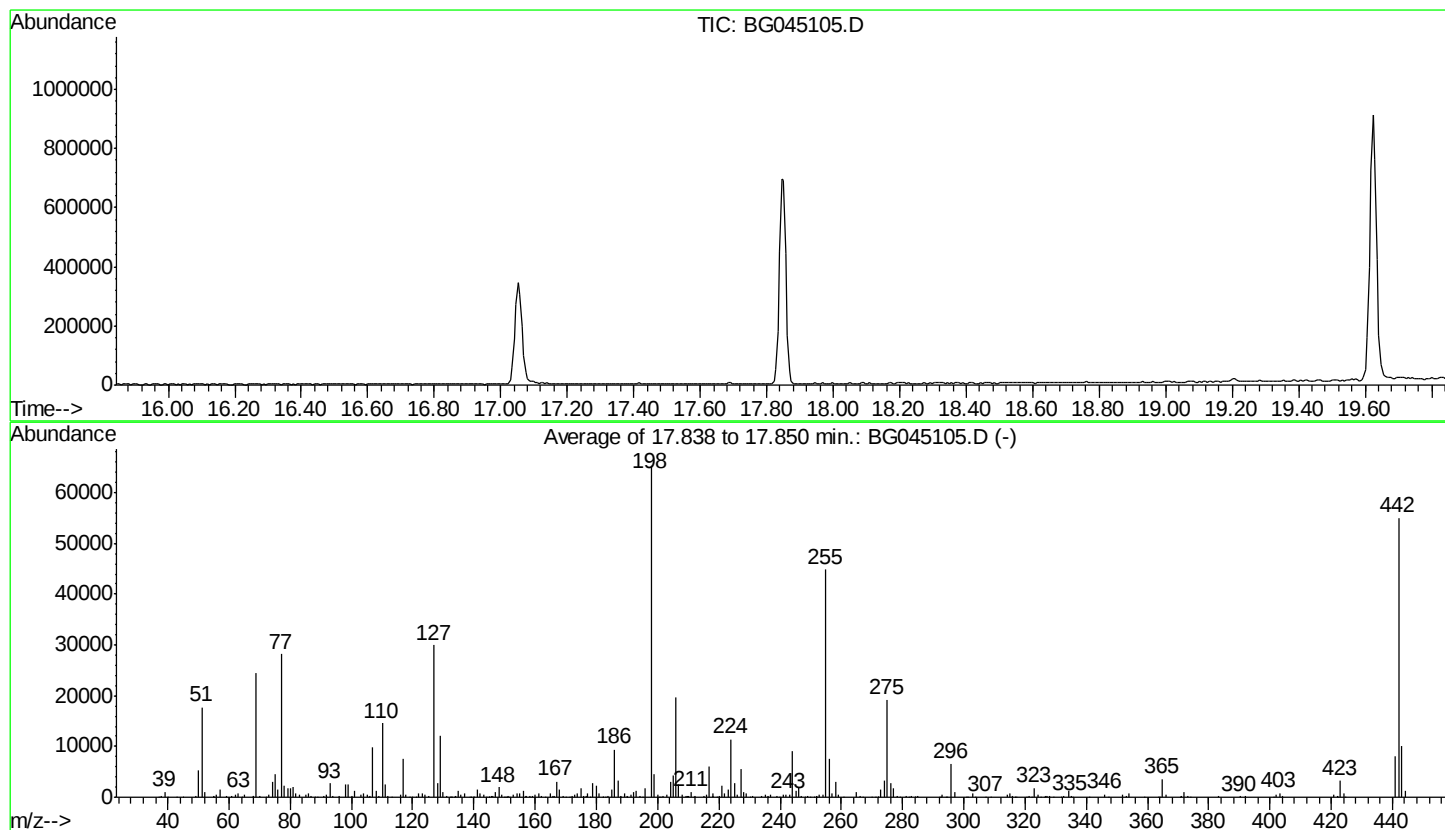

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	17671	PASS
68	69	0.00	2	1.4	340	PASS
69	198	0.00	100	37.3	24381	PASS
70	69	0.00	2	0.9	228	PASS
127	198	10	80	45.9	29978	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65330	PASS
199	198	5	9	7.0	4562	PASS
275	198	10	60	29.4	19199	PASS
365	198	1	100	5.4	3543	PASS
441	198	0.01	100	12.4	8115	PASS
442	198	50	100	84.2	55024	PASS
443	442	15	24	18.5	10178	PASS