
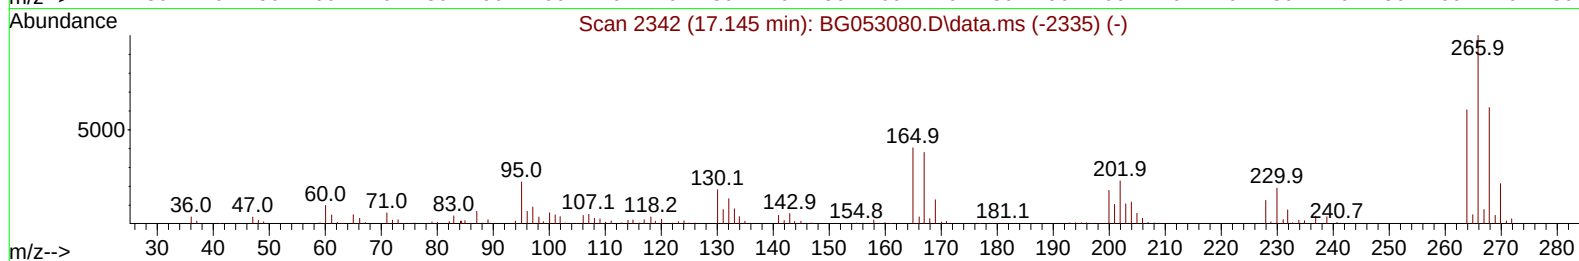
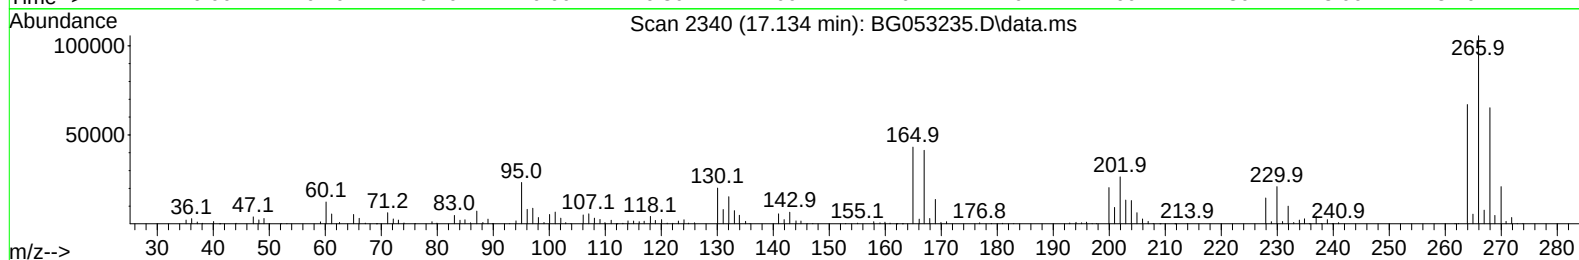


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042122\
Data File : BG053235.D
Acq On : 21 Apr 2022 10:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:27:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

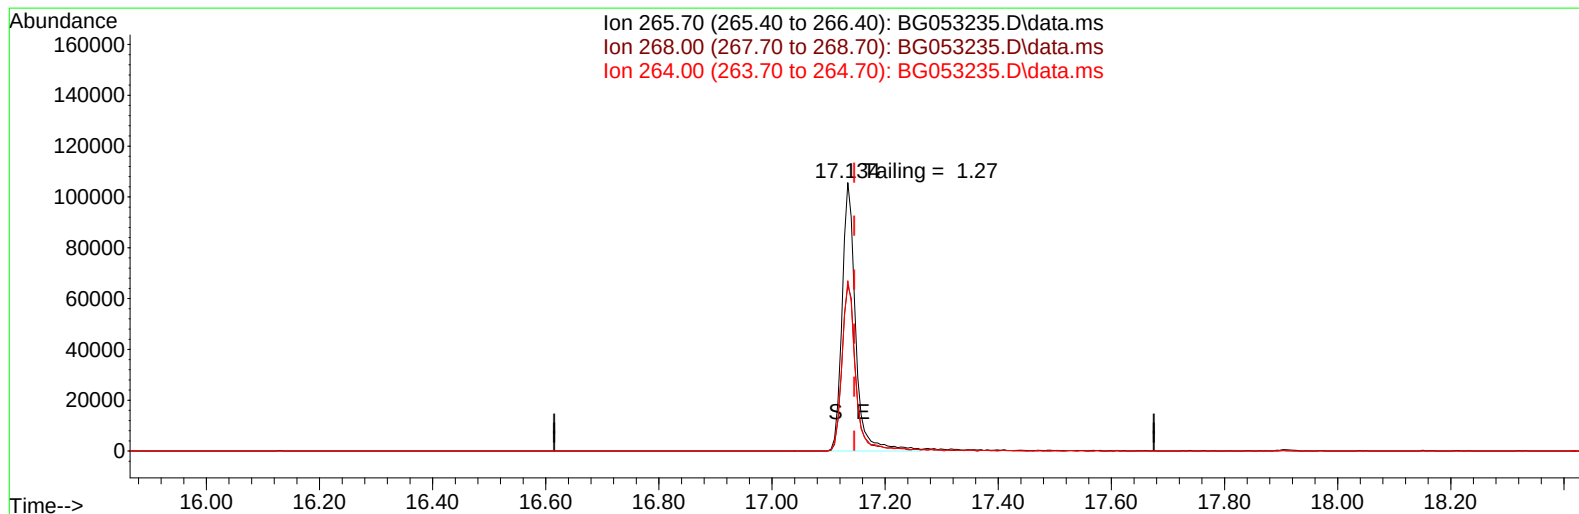

TIC: BG053235.D\data.ms

(70) Pentachlorophenol (C)




17.134min (-0.011) 24414.59 ng

response 175713

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.76
264.00	56.60	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042122\
Data File : BG053235.D
Acq On : 21 Apr 2022 10:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:27:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

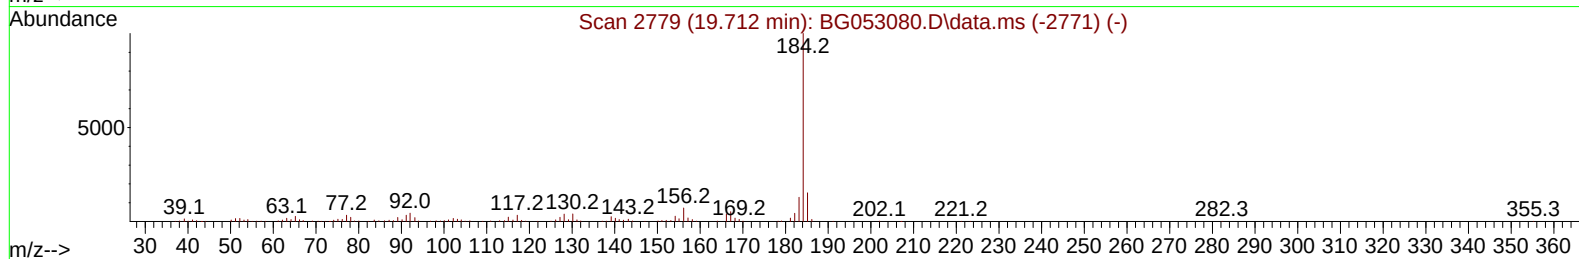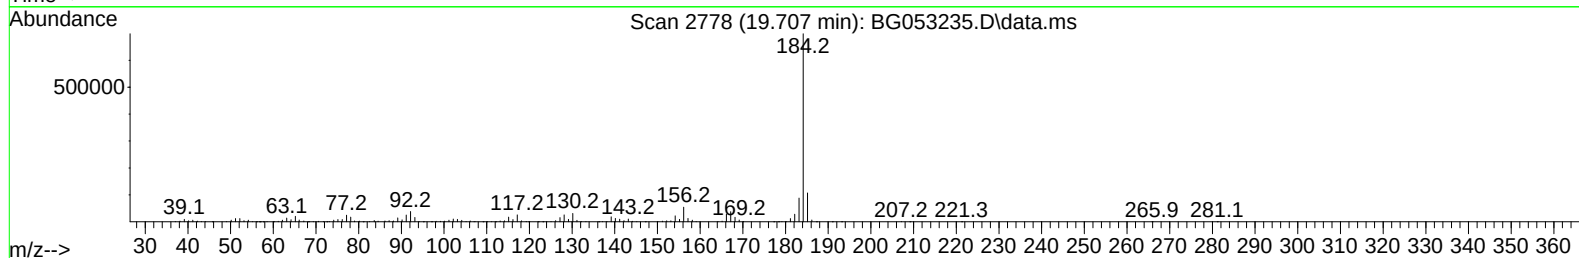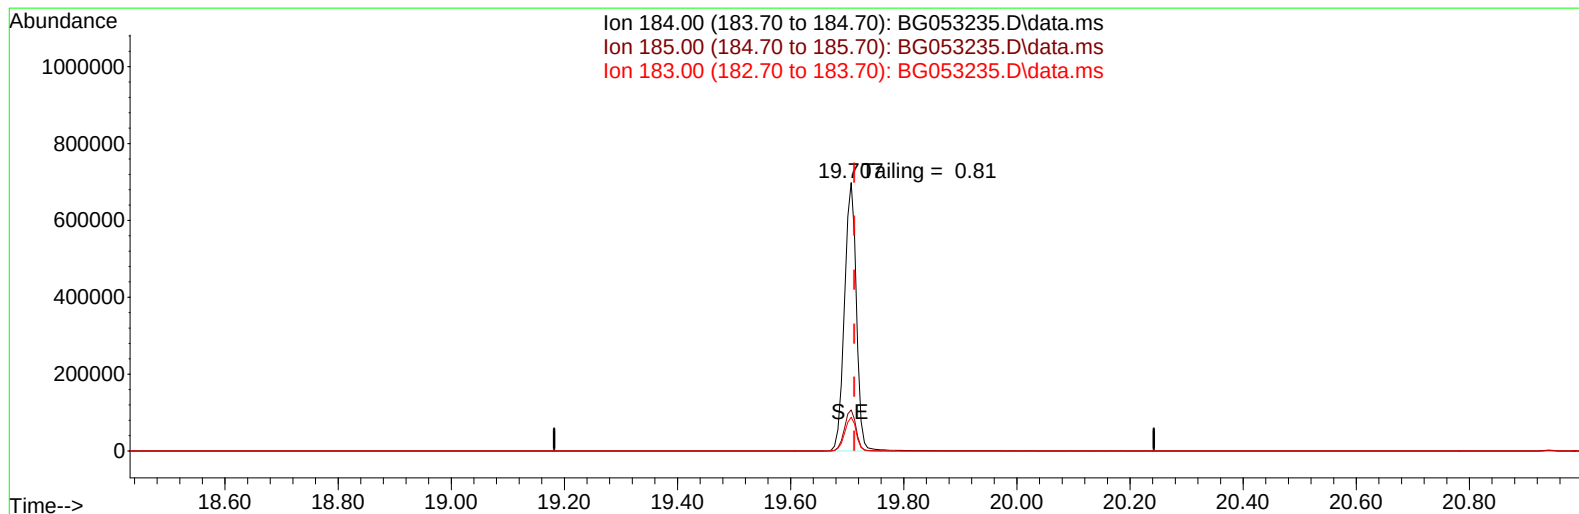

TIC: BG053235.D\data.ms

(77) Benzidine**19.707min (-0.005) 629280.19 ng****response 1023399**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.31
183.00	11.80	12.61
0.00	0.00	0.00