
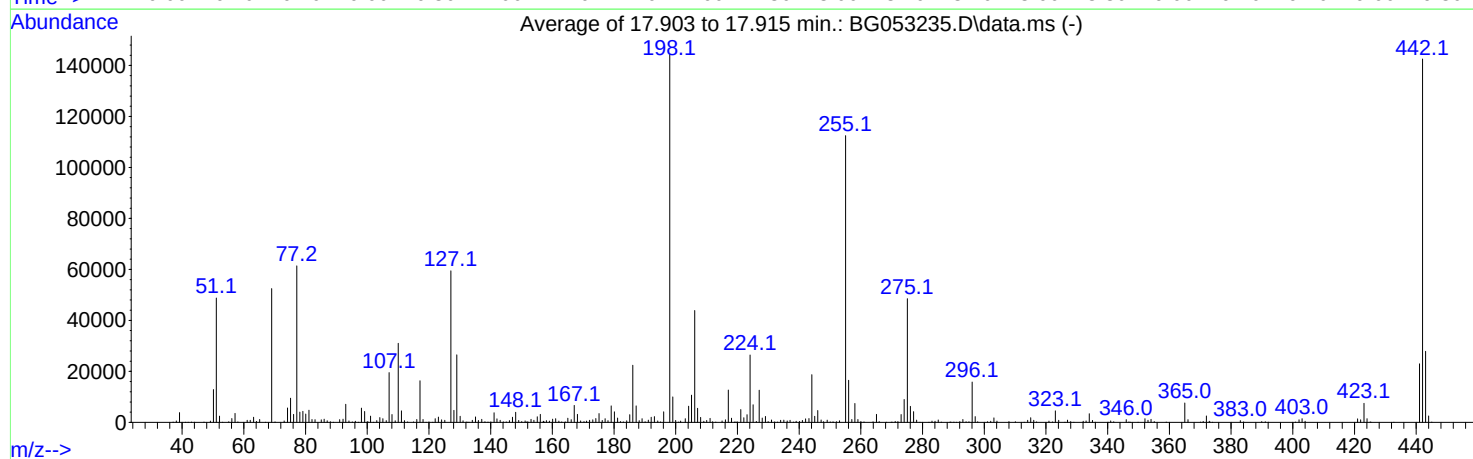


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042122\
 Data File : BG053235.D
 Acq On : 21 Apr 2022 10:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

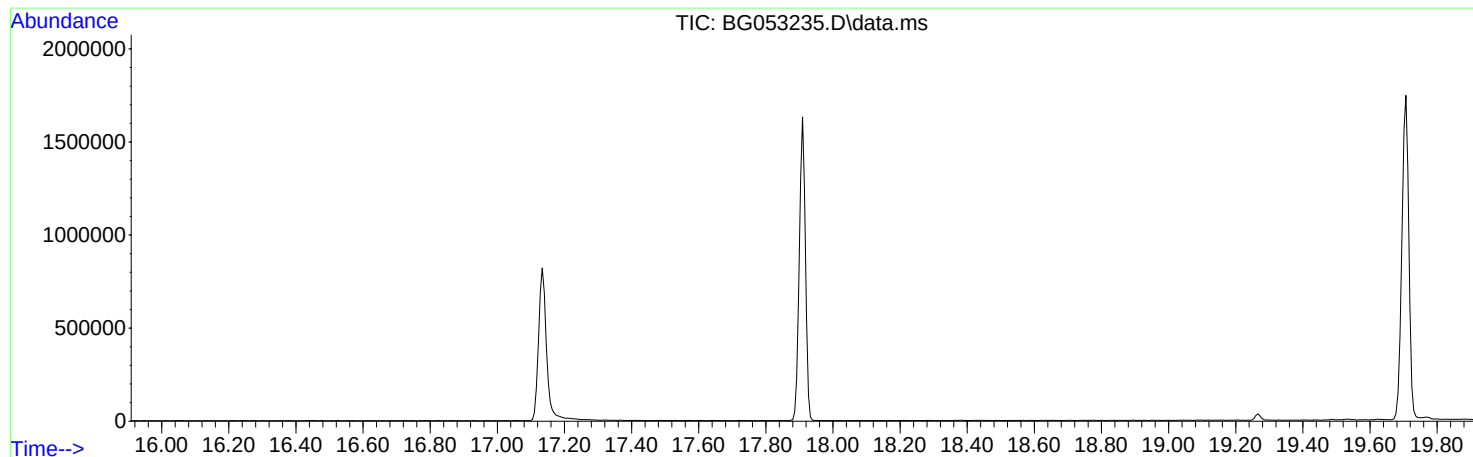




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	48783	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.4	52483	PASS
70	69	0.00	2	0.4	206	PASS
127	198	10	80	41.2	59464	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144301	PASS
199	198	5	9	6.9	9984	PASS
275	198	10	60	33.6	48525	PASS
365	198	1	100	5.2	7575	PASS
441	198	0.01	100	15.9	22971	PASS
442	442	50	100	100.0	142552	PASS
443	442	15	24	19.6	27888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042122\
Data File : BG053235.D
Acq On : 21 Apr 2022 10:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 22 07:27:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

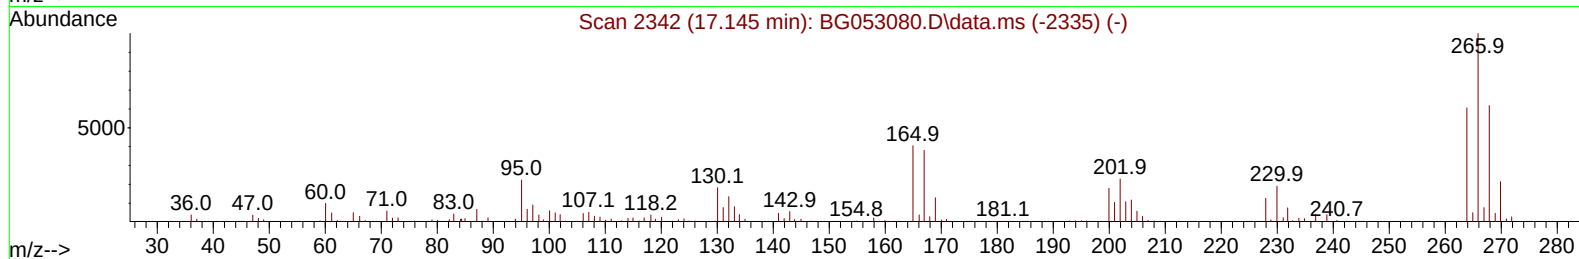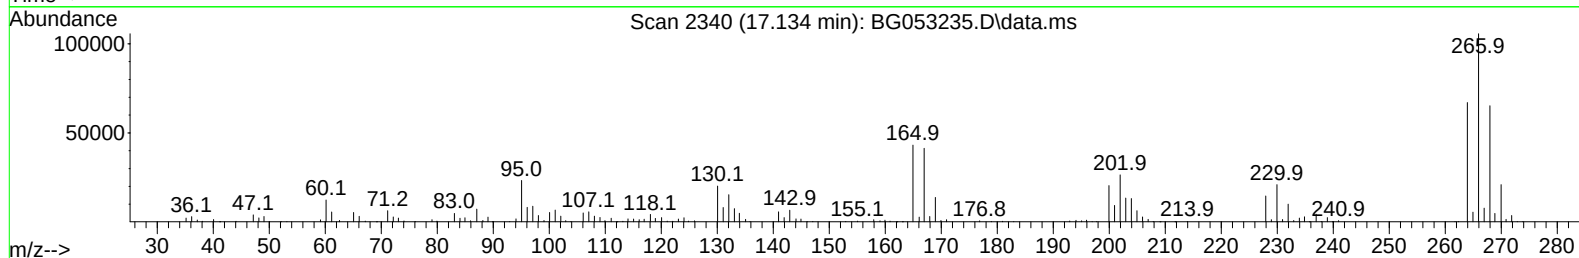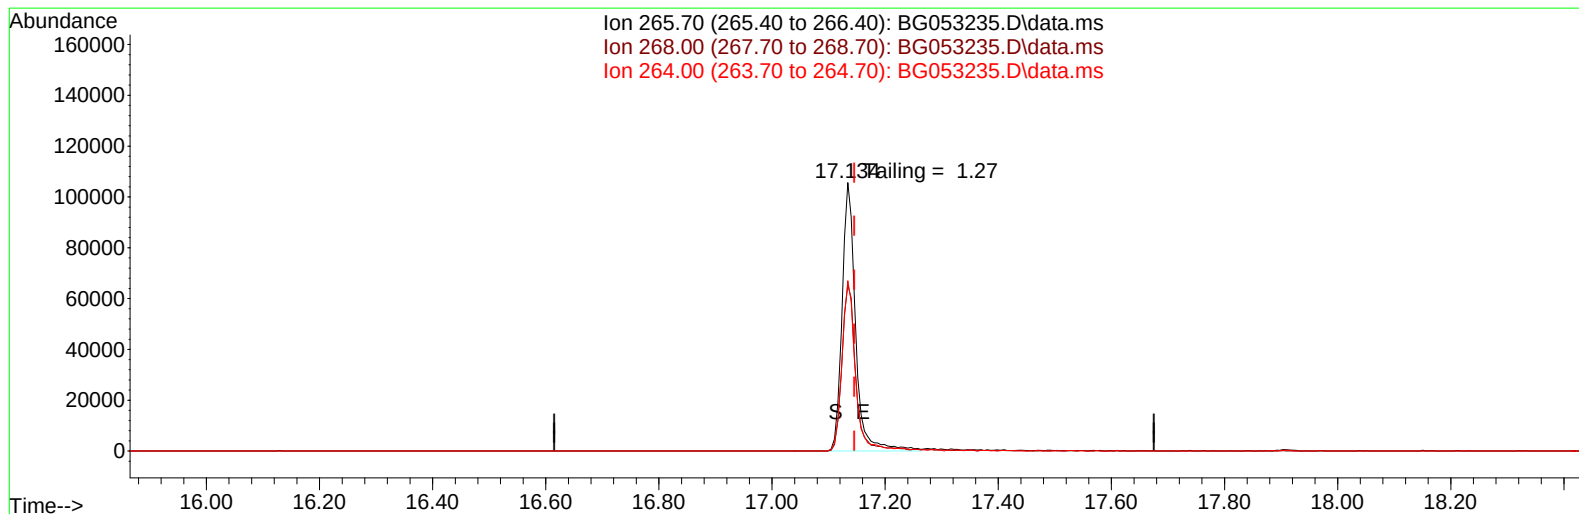

TIC: BG053235.D\data.ms

(70) Pentachlorophenol (C)

17.134min (-0.011) 24414.59 ng




response 175713

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.76
264.00	56.60	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042122\
 Data File : BG053235.D
 Acq On : 21 Apr 2022 10:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 22 07:27:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

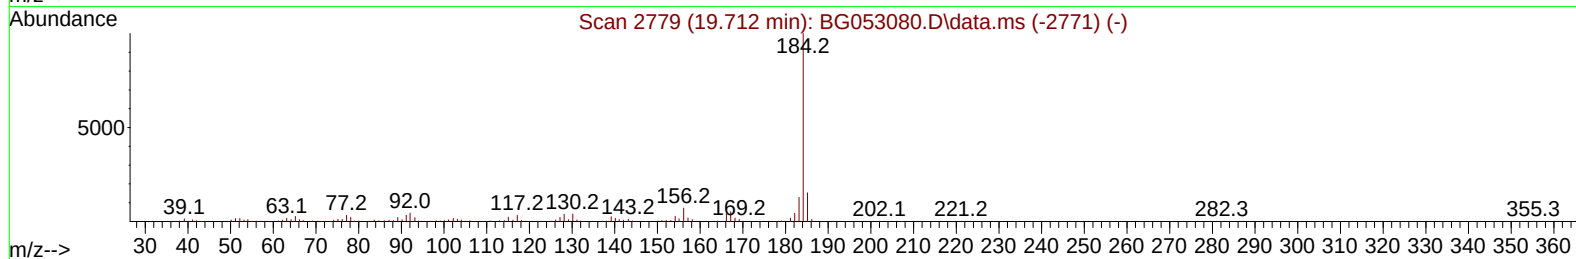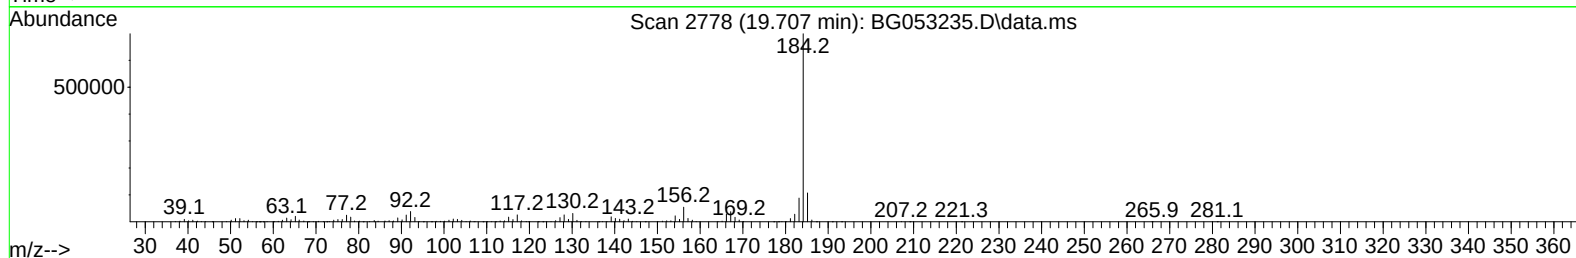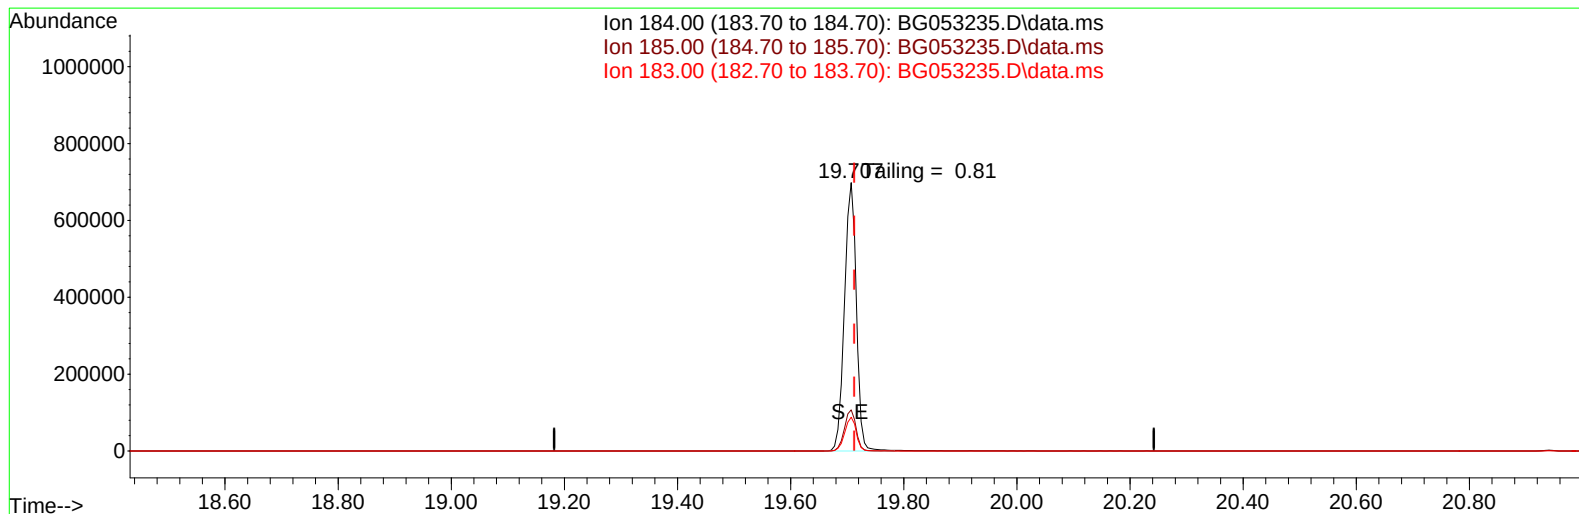

TIC: BG053235.D\data.ms

(77) Benzidine

19.707min (-0.005) 629280.19 ng

response 1023399

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.31
183.00	11.80	12.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/21/2022	BNA_G	<u>BG053235.D</u>
Compound Name	Response	Retention Time
DDT	532993	20.941
DDD	6648	20.494
DDE	463	20.001
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7111	540104	1.32

Instrument :
BNA_G
ClientSampleId :
DFTPP