


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042220\
 Data File : BG045121.D
 Acq On : 22 Apr 2020 11:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 22 12:56:37 2020

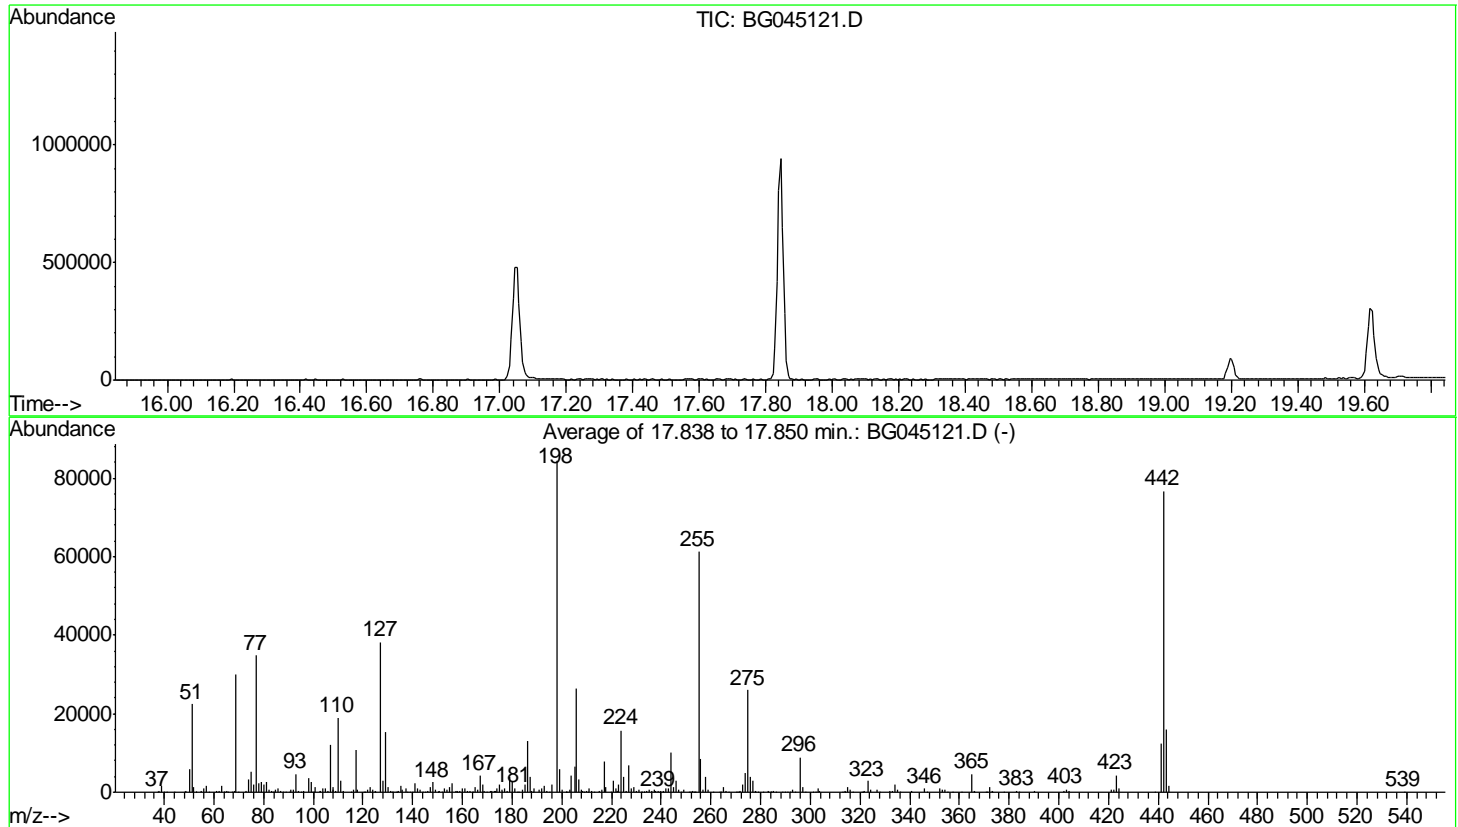

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	22460	PASS
68	69	0.00	2	0.9	269	PASS
69	198	0.00	100	35.6	30040	PASS
70	69	0.00	2	0.5	152	PASS
127	198	10	80	45.2	38186	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84426	PASS
199	198	5	9	6.9	5823	PASS
275	198	10	60	30.8	26010	PASS
365	198	1	100	5.5	4682	PASS
441	198	0.01	100	14.8	12465	PASS
442	198	50	100	90.7	76594	PASS
443	442	15	24	20.9	15978	PASS