
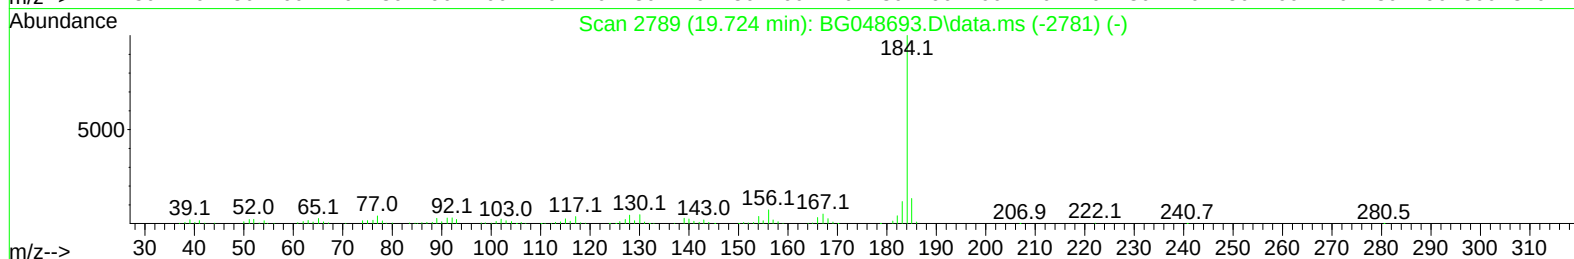
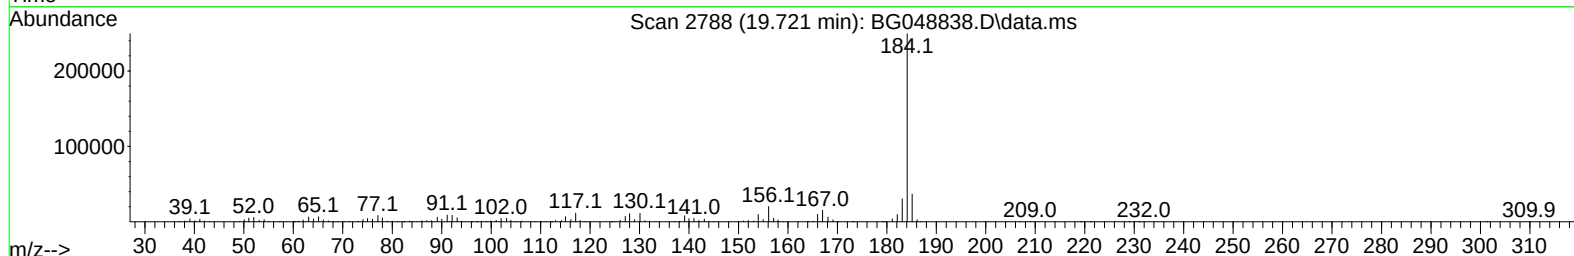


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042221\
 Data File : BG048838.D
 Acq On : 22 Apr 2021 8:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 11:44:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 17:33:30 2021
 Response via : Initial Calibration

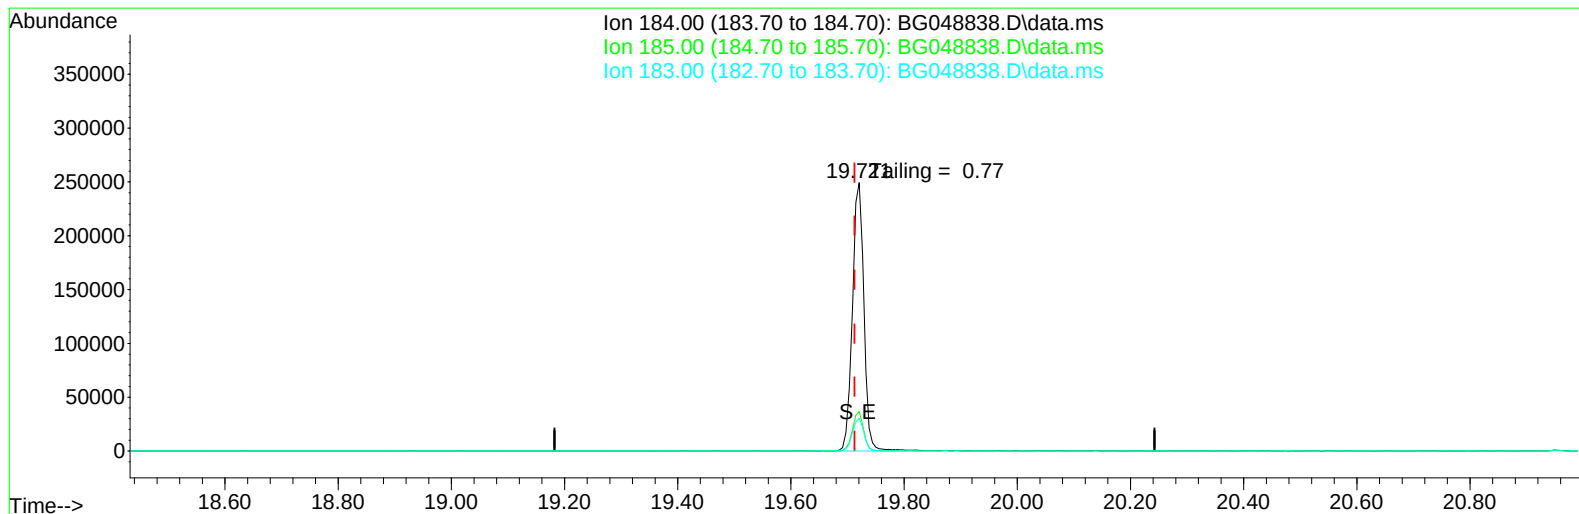

TIC: BG048838.D\data.ms

(77) Benzidine




19.721min (+ 0.008) 227336.38 ng

response 351896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.77
183.00	11.70	12.19
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042221\  
Data File : BG048838.D  
Acq On    : 22 Apr 2021    8:39  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 22 11:44:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

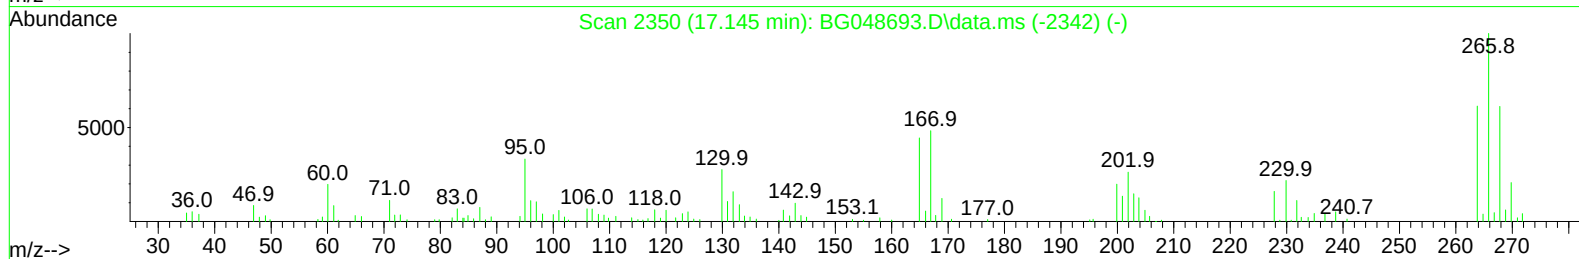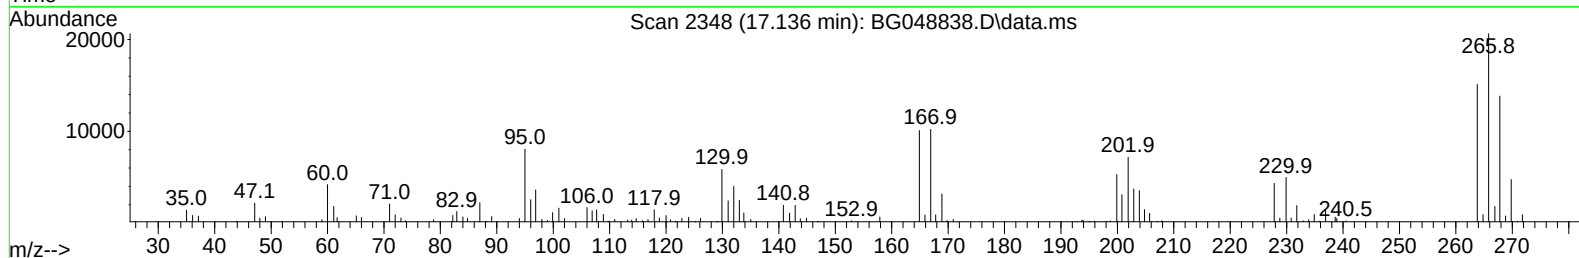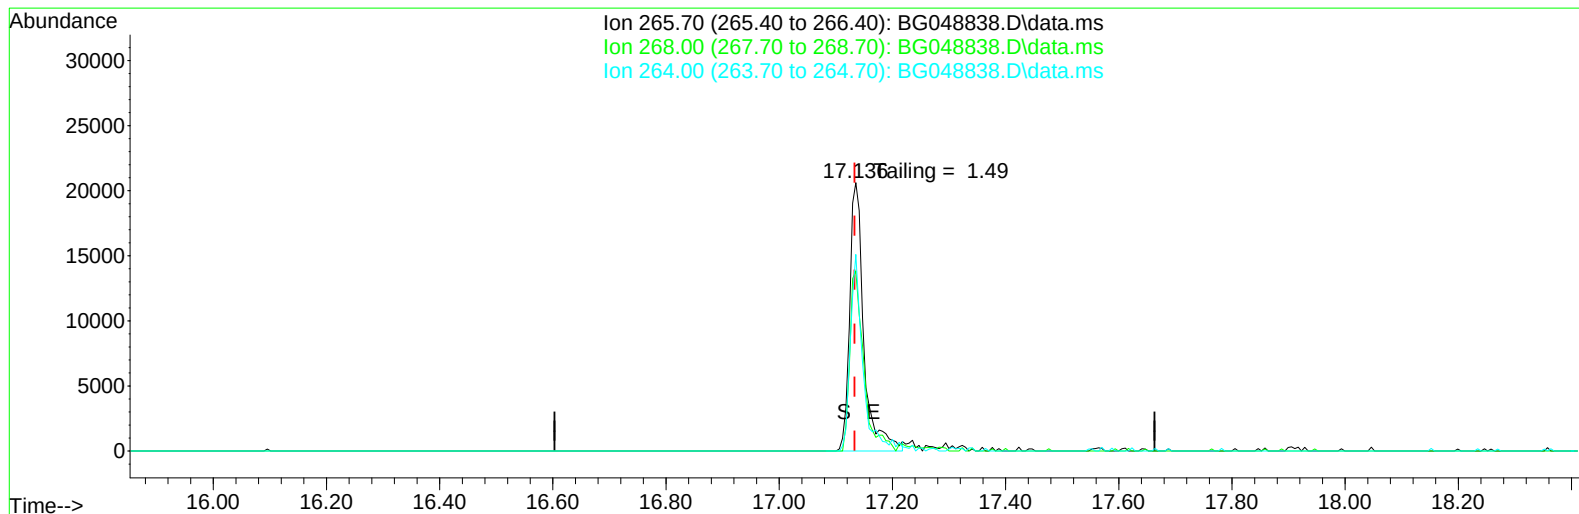

TIC: BG048838.D\data.ms

(70) Pentachlorophenol (C)

17.136min (+ 0.003) 104883.72 ng

response **35836**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.05
264.00	61.30	73.24
0.00	0.00	0.00