
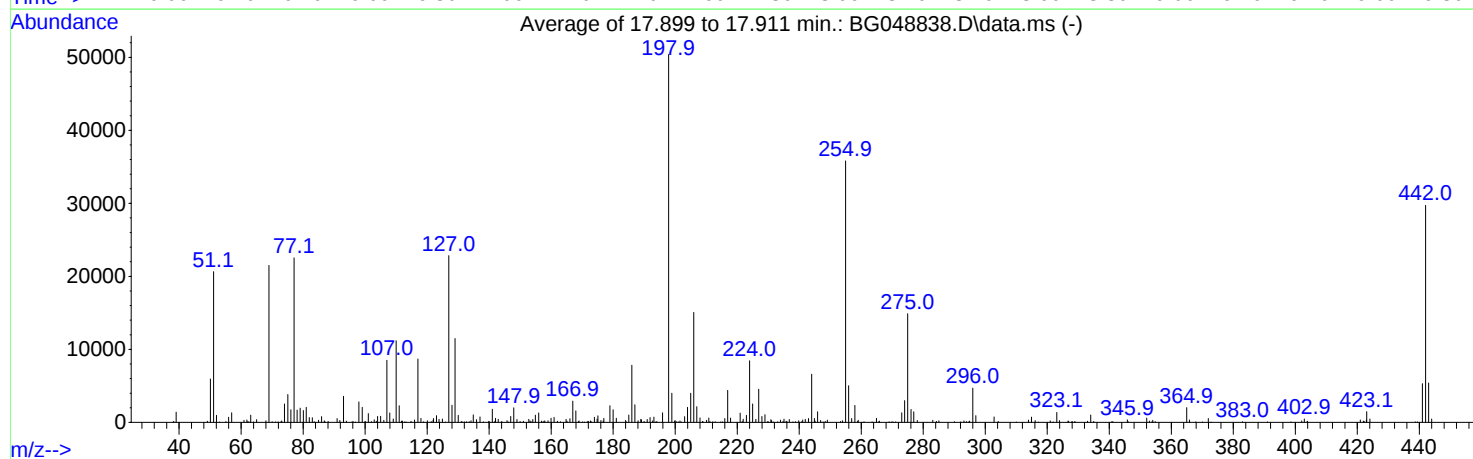


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042221\
 Data File : BG048838.D
 Acq On : 22 Apr 2021 8:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 17:33:30 2021

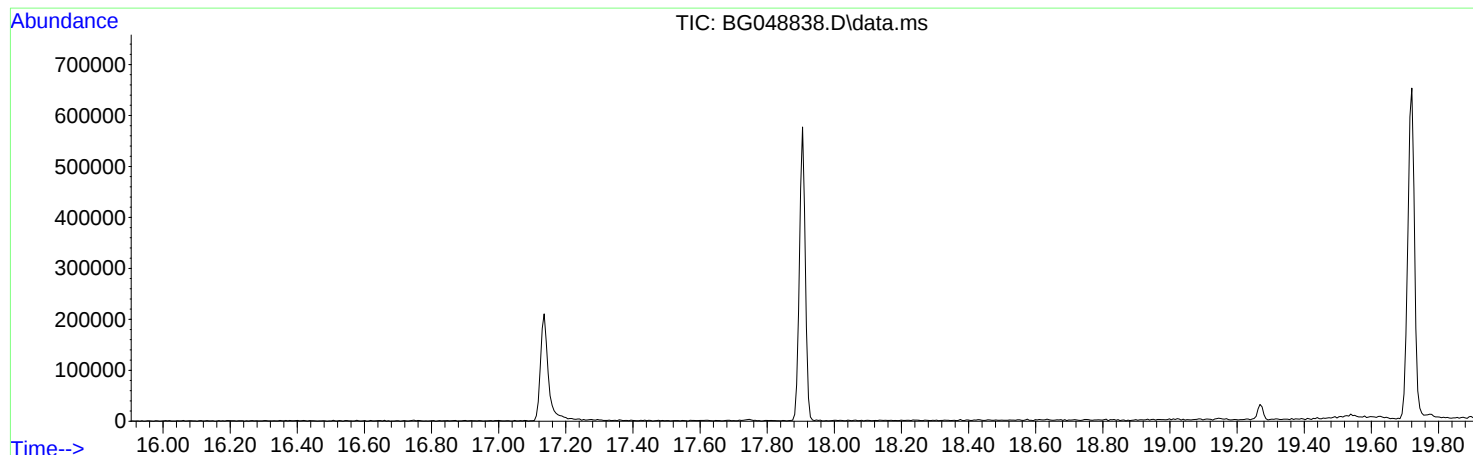




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	20654	PASS
68	69	0.00	2	1.1	228	PASS
69	198	0.00	100	42.7	21507	PASS
70	69	0.00	2	0.4	79	PASS
127	198	10	80	45.3	22835	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50389	PASS
199	198	5	9	7.9	3993	PASS
275	198	10	60	29.6	14890	PASS
365	198	1	100	4.0	2029	PASS
441	198	0.01	100	10.5	5306	PASS
442	198	50	100	59.0	29720	PASS
443	442	15	24	18.2	5402	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042221\
Data File : BG048838.D
Acq On : 22 Apr 2021 8:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 22 11:44:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

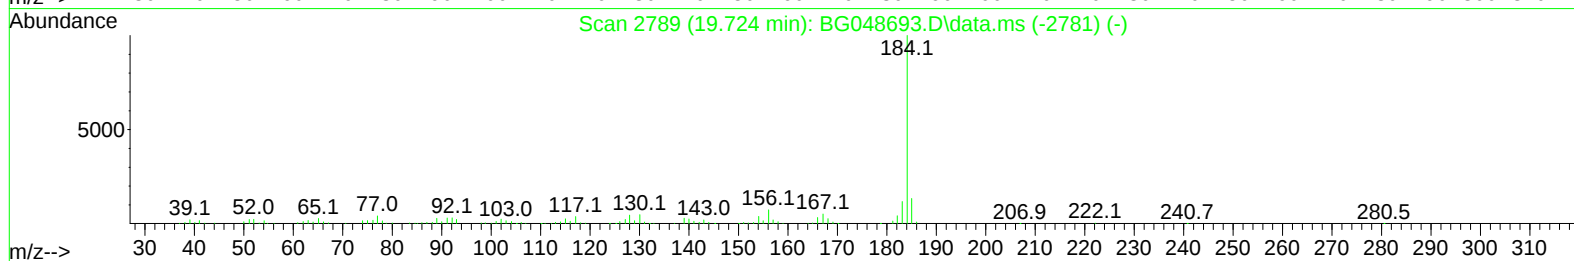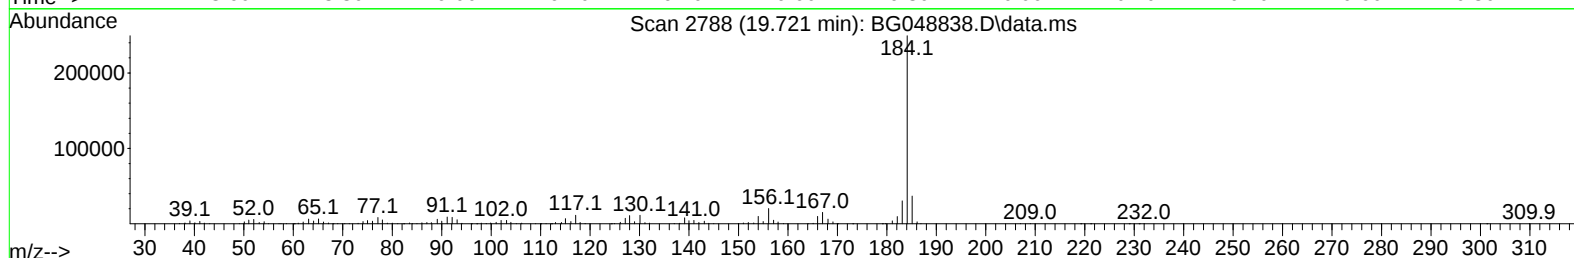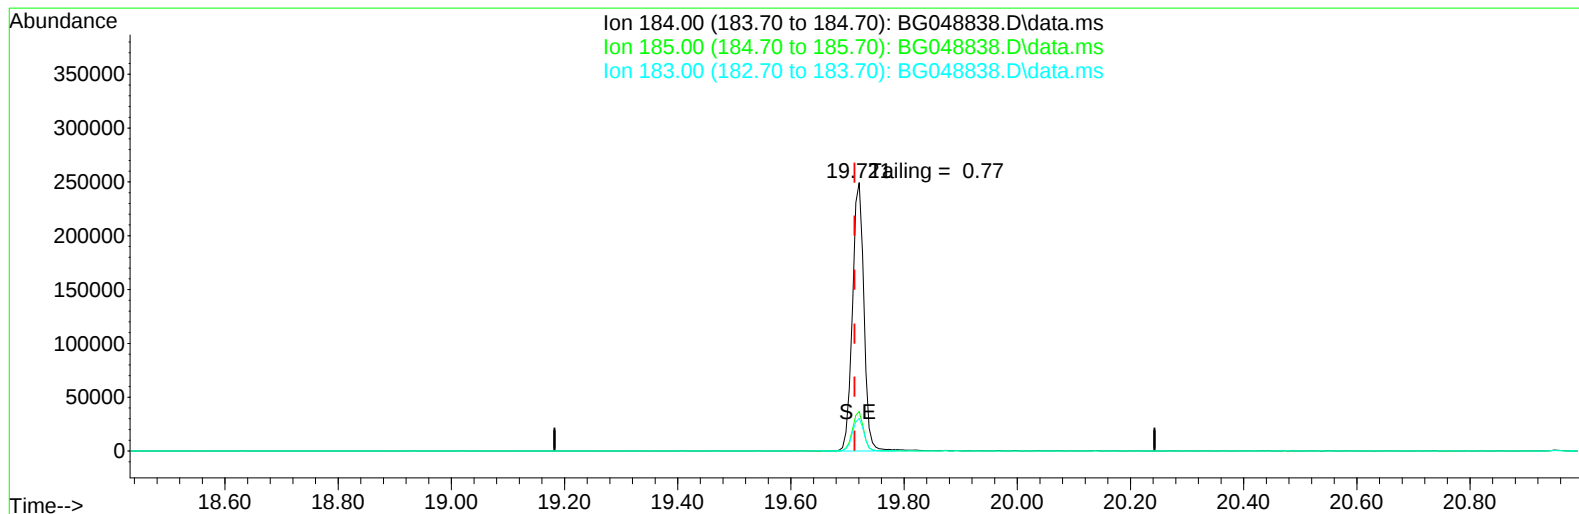

TIC: BG048838.D\data.ms

(77) Benzidine

19.721min (+ 0.008) 227336.38 ng




response 351896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.77
183.00	11.70	12.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042221\
Data File : BG048838.D
Acq On : 22 Apr 2021 8:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 22 11:44:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

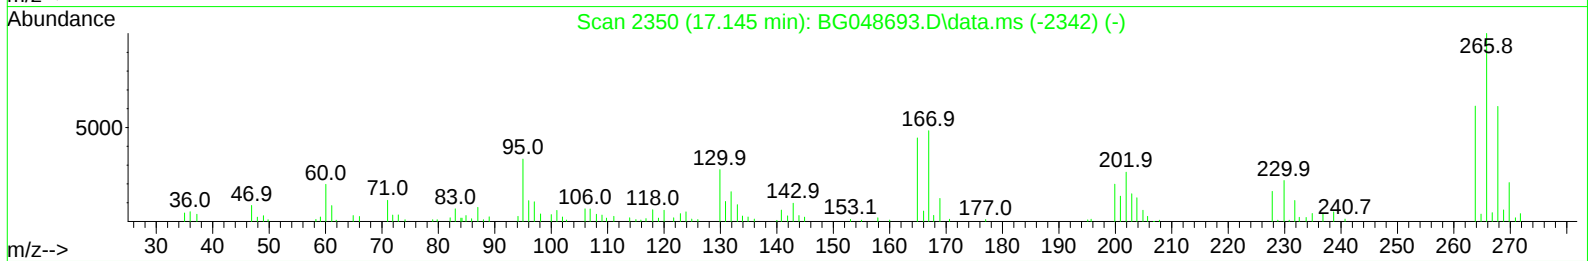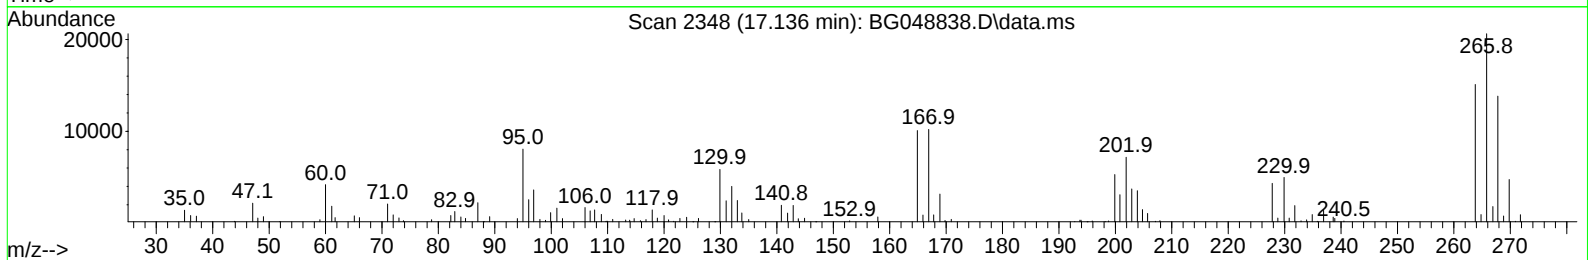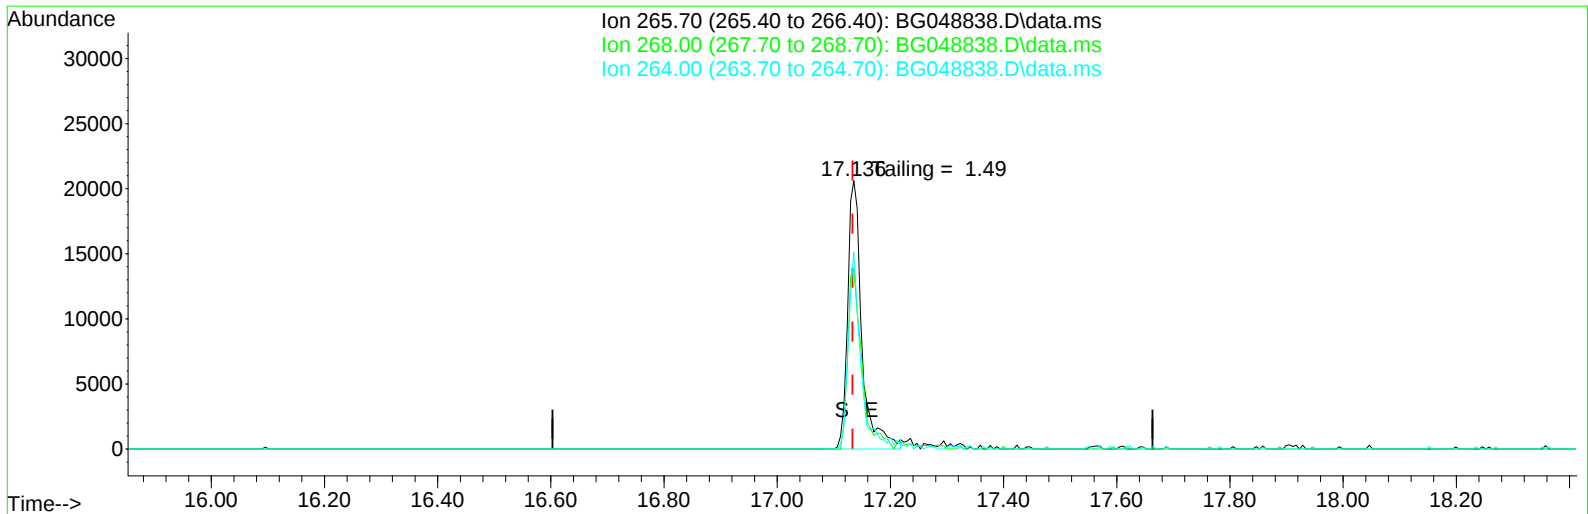

TIC: BG048838.D\data.ms

(70) Pentachlorophenol (C)

17.136min (+ 0.003) 104883.72 ng

response 35836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.05
264.00	61.30	73.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/22/2021	BNA_G	BG048838.D
Compound Name	Response	Retention Time
DDT	176983	20.95
DDD	6797	20.5
DDE	974	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7771	184754	4.21