
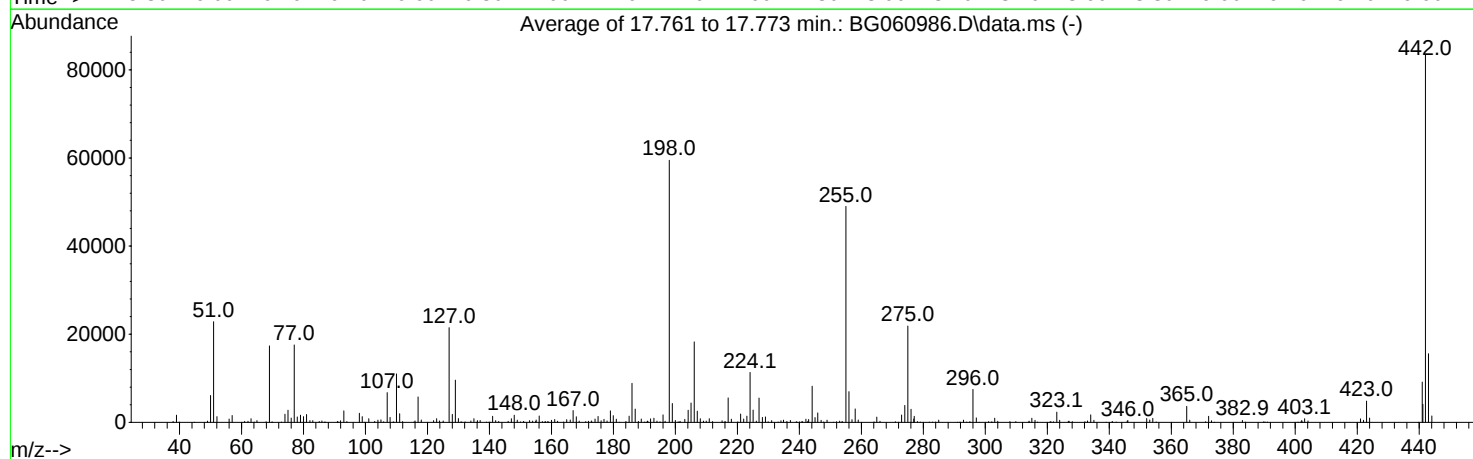


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042224\
Data File : BG060986.D
Acq On : 22 Apr 2024 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 22 04:22:00 2024

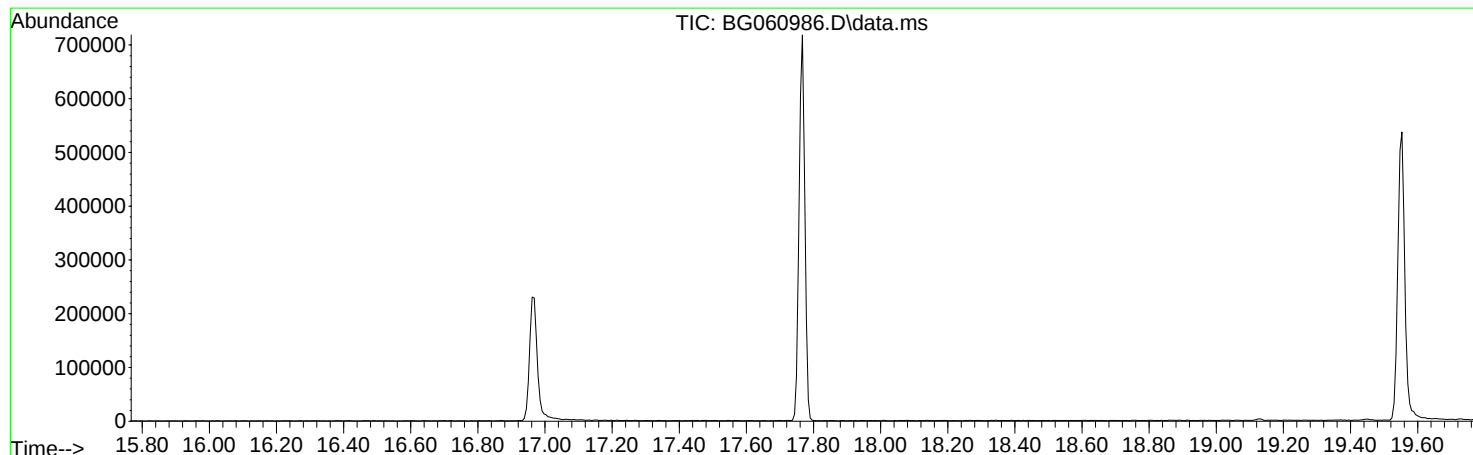




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	22826	PASS
68	69	0.00	2	0.8	145	PASS
69	198	0.00	100	29.2	17365	PASS
70	69	0.00	2	0.4	76	PASS
127	198	10	80	36.1	21484	PASS
197	198	0.00	2	0.4	250	PASS
198	198	100	100	100.0	59472	PASS
199	198	5	9	7.2	4294	PASS
275	198	10	60	36.8	21859	PASS
365	198	1	100	6.1	3646	PASS
441	198	0.01	100	15.4	9165	PASS
442	442	50	100	100.0	83475	PASS
443	442	15	24	18.6	15561	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042224\
Data File : BG060986.D
Acq On : 22 Apr 2024 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 06:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

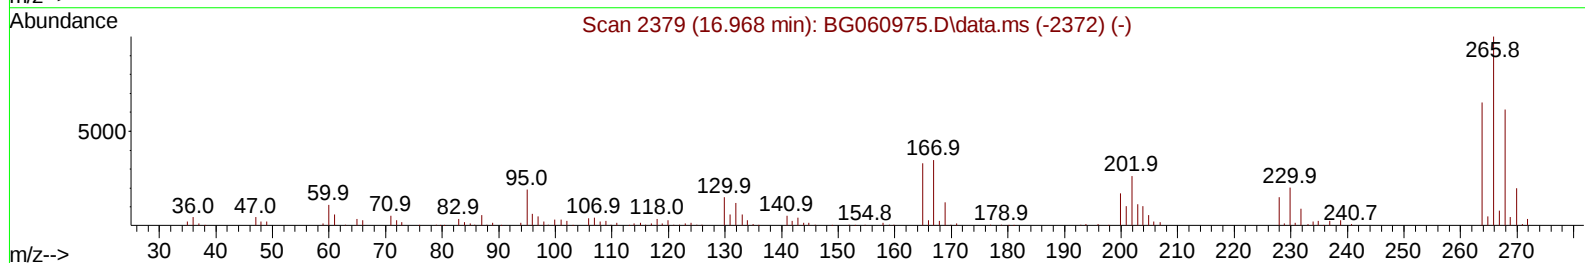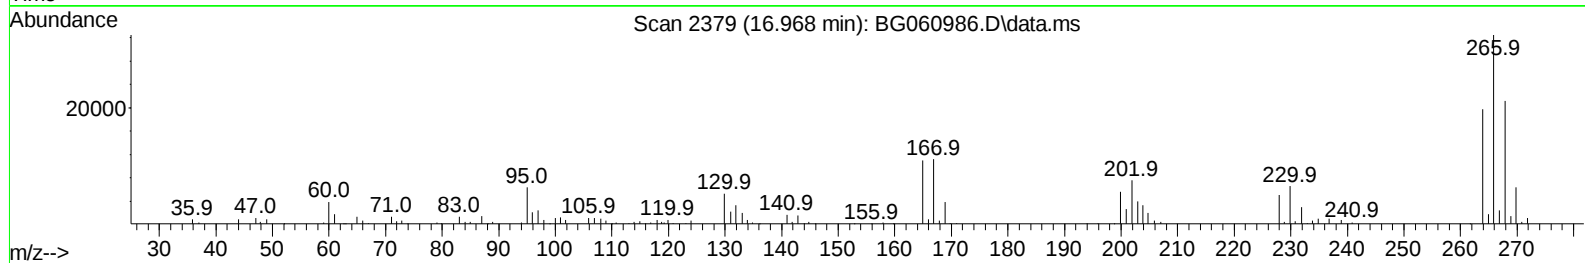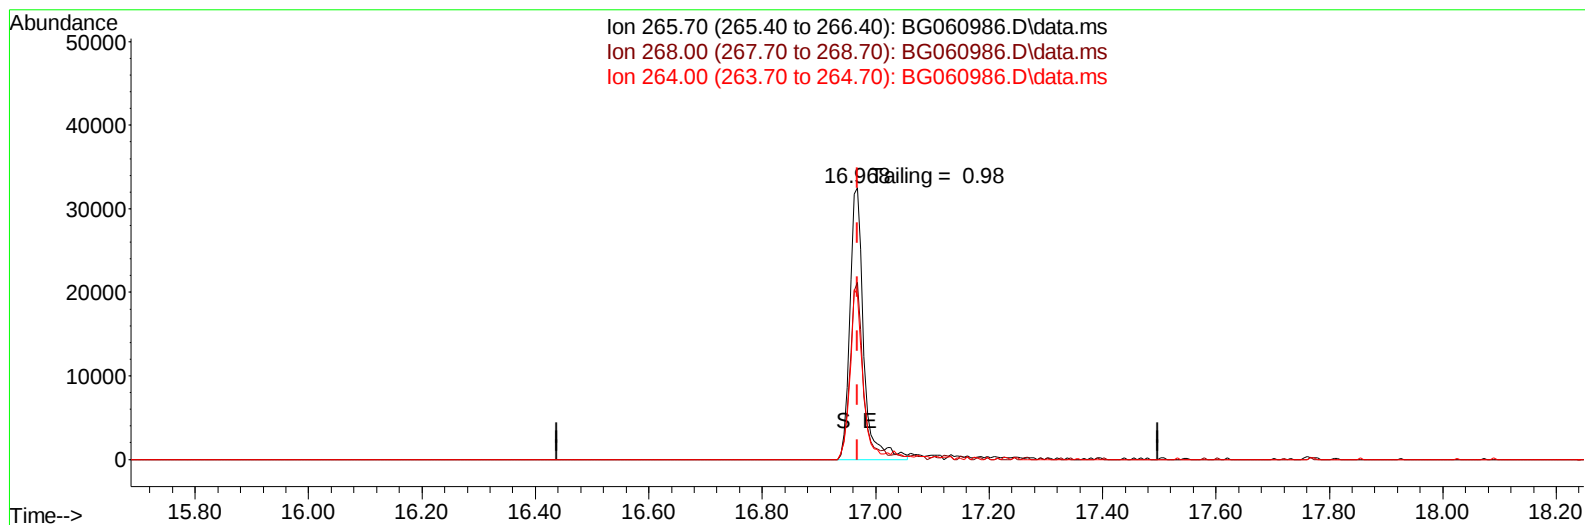

TIC: BG060986.D\data.ms

(70) Pentachlorophenol (C)

16.968min (-0.000) 26276.92 ng




response 54506

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	65.11
264.00	65.20	60.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042224\
Data File : BG060986.D
Acq On : 22 Apr 2024 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 06:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

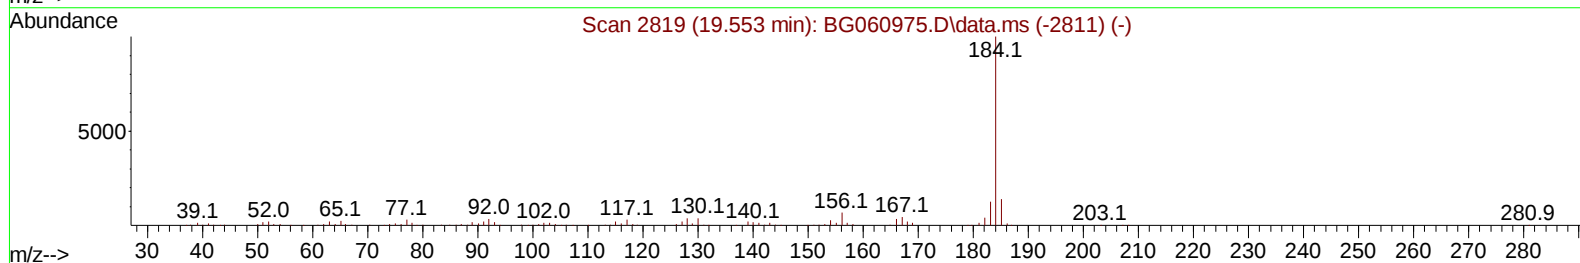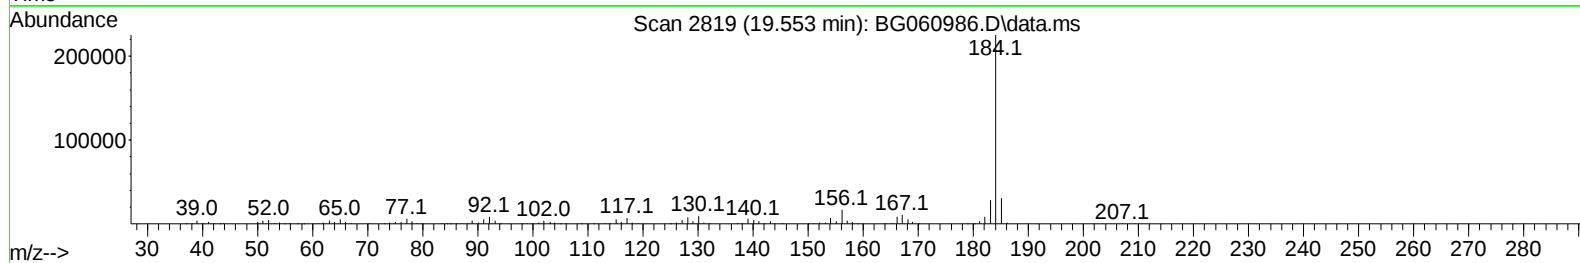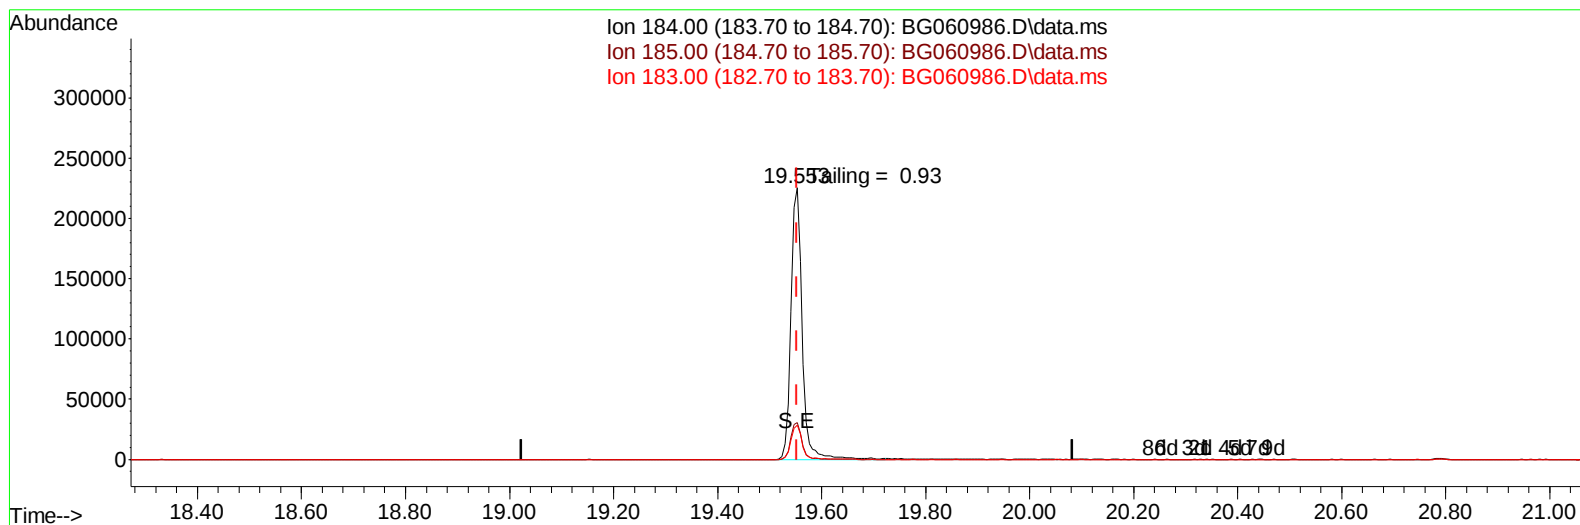

TIC: BG060986.D\data.ms

(77) Benzidine

19.553min (-0.000) 338888.95 ng m

response 345358

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.53
183.00	12.70	12.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/22/2024	BNA_G	<u>BG060986.D</u>
Compound Name	Response	Retention Time
DDT	186604	20.793
DDD	16475	20.352
DDE	2905	19.847
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19380	205984	9.41

Instrument :
BNA_G
ClientSampleId :
DFTPP