

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG042320\  
 Data File : BG045150.D  
 Acq On : 23 Apr 2020 20:29  
 Operator : CG/JU  
 Sample : L2350-08 10X  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 TP-5-D

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG041520.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.581       | 417           | 424         | 436          | rBV      | 196899         | 337058        | 23.49%          | 3.204%        |
| 2         | 7.173       | 687           | 695         | 706          | rBV2     | 216722         | 397802        | 27.73%          | 3.782%        |
| 3         | 8.007       | 830           | 837         | 847          | rVB      | 362335         | 627268        | 43.72%          | 5.963%        |
| 4         | 8.331       | 885           | 892         | 900          | rBV      | 188528         | 338082        | 23.56%          | 3.214%        |
| 5         | 9.165       | 1025          | 1034        | 1041         | rBV2     | 142840         | 269025        | 18.75%          | 2.557%        |
| 6         | 10.815      | 1307          | 1315        | 1325         | rVB      | 491301         | 912893        | 63.63%          | 8.678%        |
| 7         | 13.265      | 1722          | 1732        | 1741         | rBV      | 431018         | 685978        | 47.81%          | 6.521%        |
| 8         | 14.093      | 1866          | 1873        | 1880         | rBV      | 63881          | 101892        | 7.10%           | 0.969%        |
| 9         | 14.645      | 1959          | 1967        | 1978         | rBV      | 825798         | 1302134       | 90.76%          | 12.378%       |
| 10        | 16.132      | 2213          | 2220        | 2227         | rBV      | 329249         | 489489        | 34.12%          | 4.653%        |
| 11        | 17.389      | 2428          | 2434        | 2440         | rBV      | 874258         | 1434726       | 100.00%         | 13.639%       |
| 12        | 19.439      | 2779          | 2783        | 2789         | rBV      | 124762         | 181395        | 12.64%          | 1.724%        |
| 13        | 19.803      | 2841          | 2845        | 2850         | rVB      | 105844         | 151023        | 10.53%          | 1.436%        |
| 14        | 19.997      | 2873          | 2878        | 2884         | rBV      | 585880         | 809022        | 56.39%          | 7.691%        |
| 15        | 21.654      | 3153          | 3160        | 3166         | rBV      | 813859         | 1395990       | 97.30%          | 13.270%       |
| 16        | 24.838      | 3695          | 3702        | 3711         | rBV      | 416320         | 1085873       | 75.69%          | 10.322%       |


Sum of corrected areas: 10519650

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG042320\  
Data File : BG045150.D  
Acq On : 23 Apr 2020 20:29  
Operator : CG/JU  
Sample : L2350-08 10X  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
TP-5-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG041520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

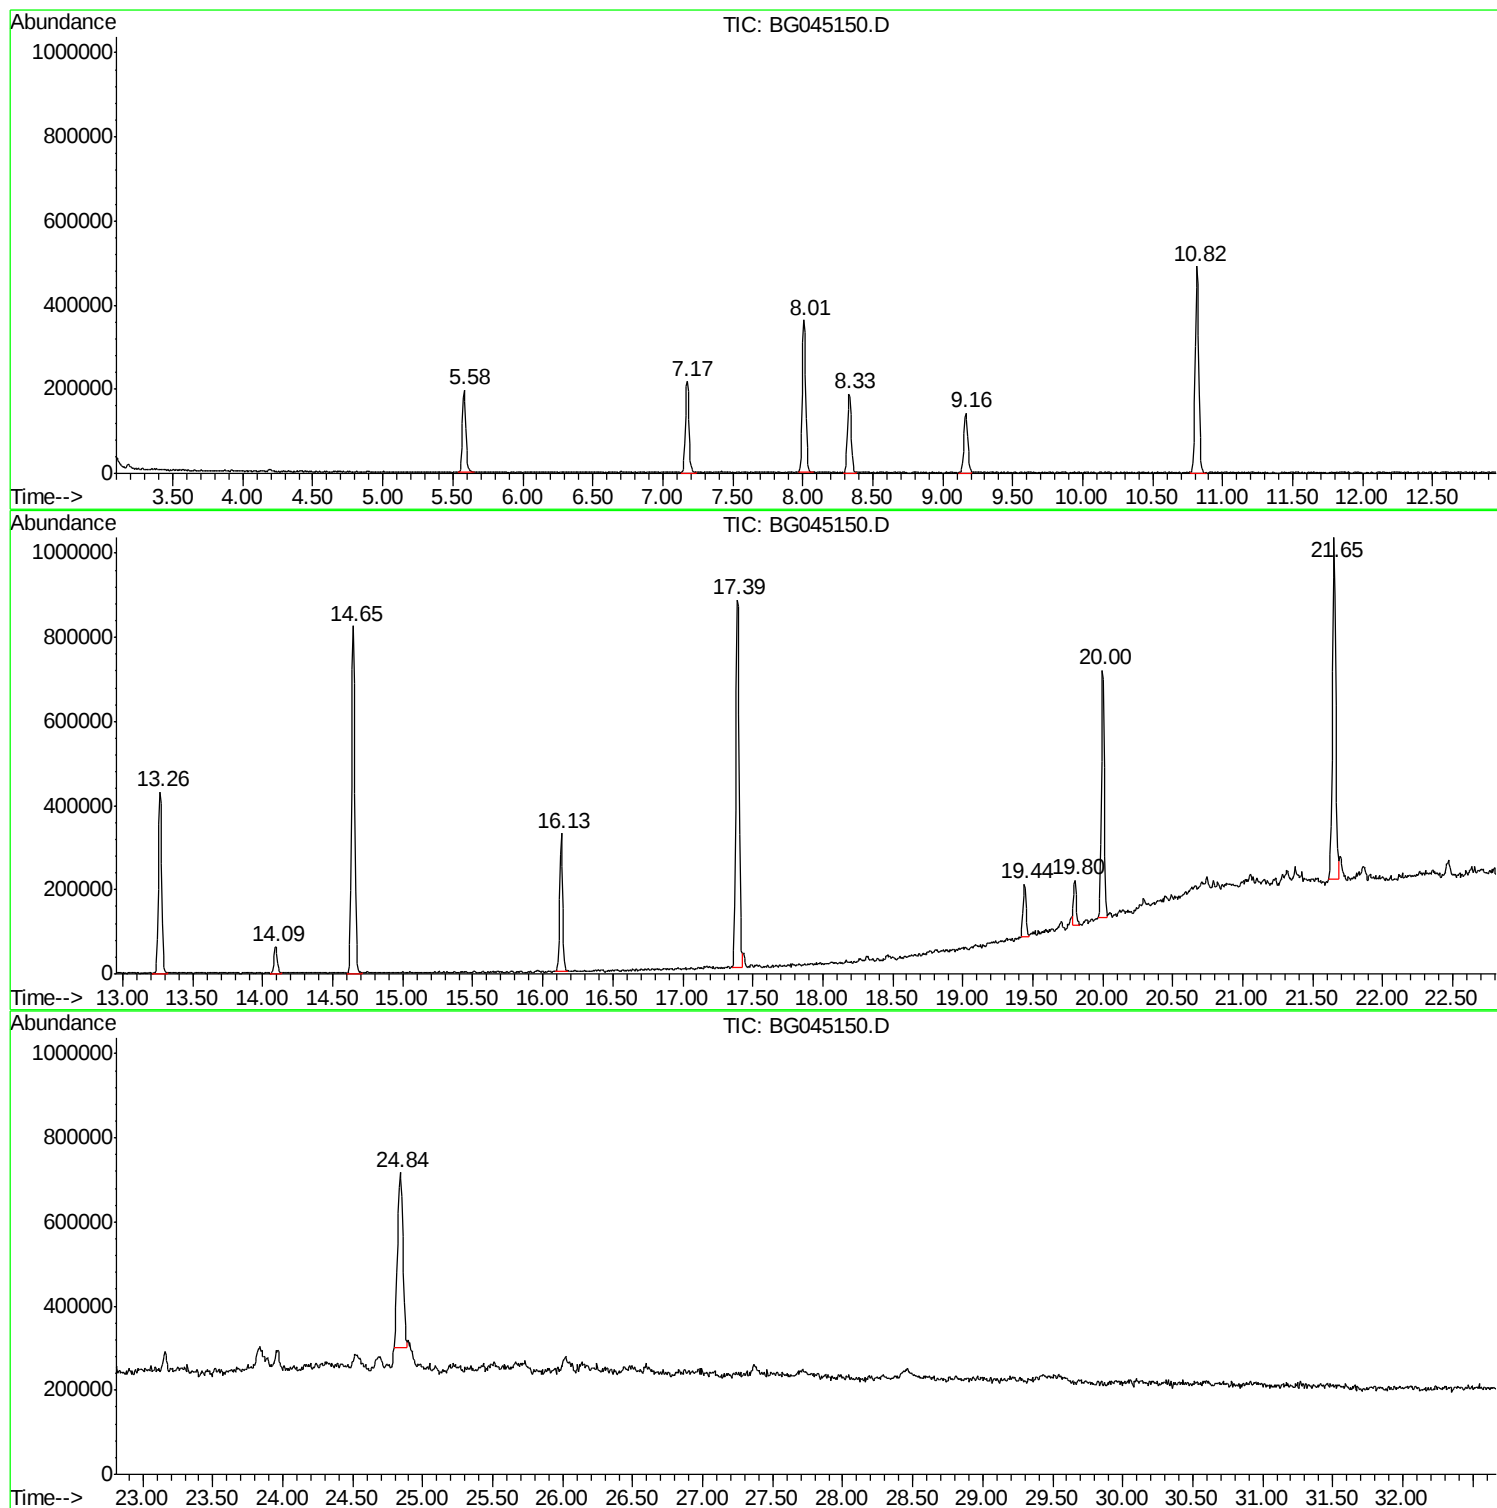

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG042320\  
Data File : BG045150.D  
Acq On : 23 Apr 2020 20:29  
Operator : CG/JU  
Sample : L2350-08 10X  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
TP-5-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG041520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG042320\  
Data File : BG045150.D  
Acq On : 23 Apr 2020 20:29  
Operator : CG/JU  
Sample : L2350-08 10X  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
TP-5-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG041520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |