
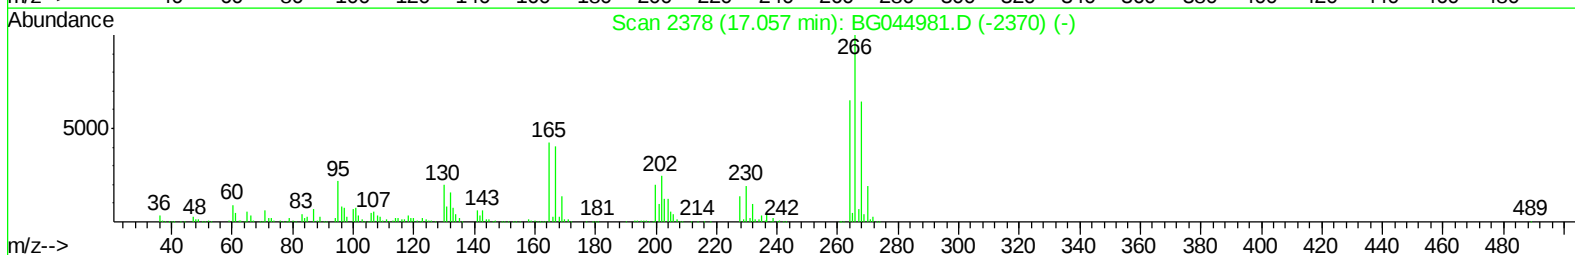
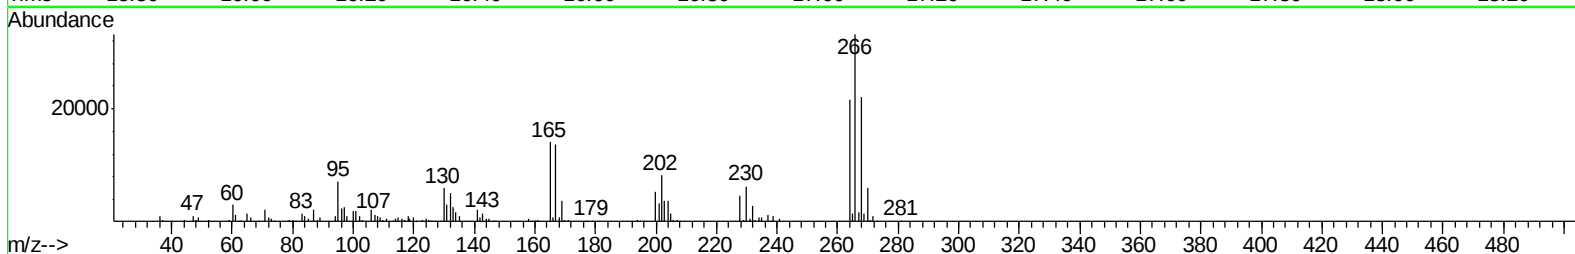


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG042420\
Data File : BG045156.D
Acq On : 24 Apr 2020 11:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 01:45:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 13:58:55 2020
Response via : Initial Calibration

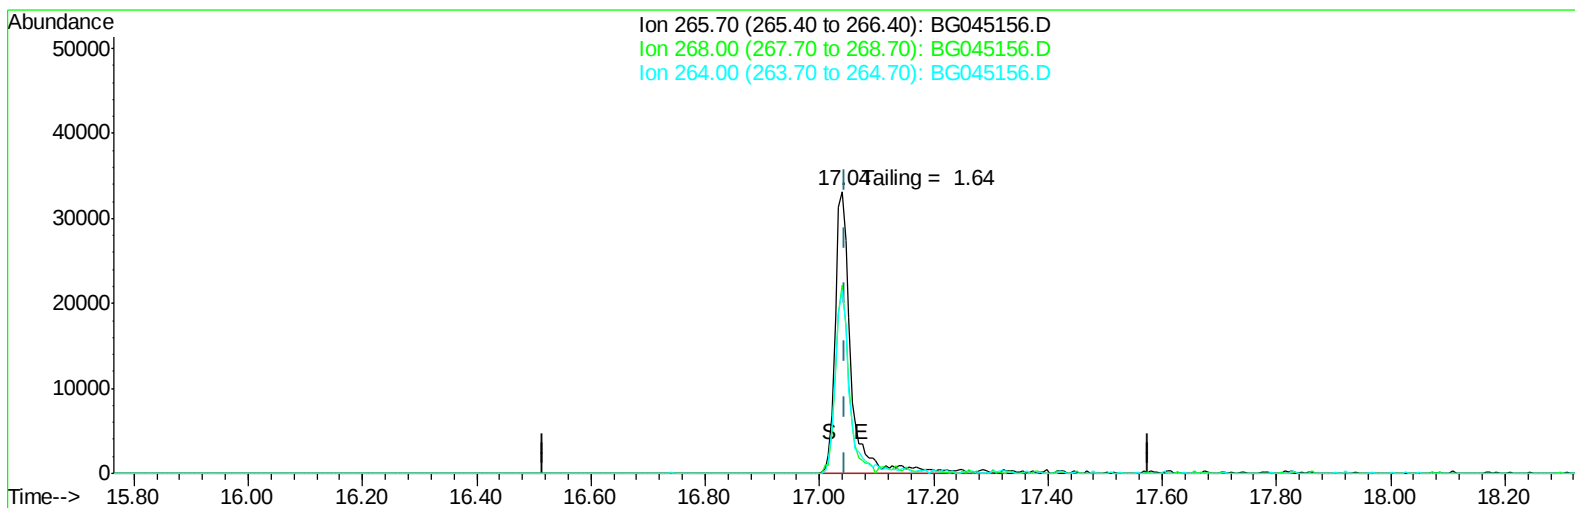

TIC: BG045156.D

(70) Pentachlorophenol (C)




17.039min (-0.006) 52014.98ng

response 59344

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	66.83
264.00	65.30	65.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG042420\
 Data File : BG045156.D
 Acq On : 24 Apr 2020 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 01:45:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 23 13:58:55 2020
 Response via : Initial Calibration

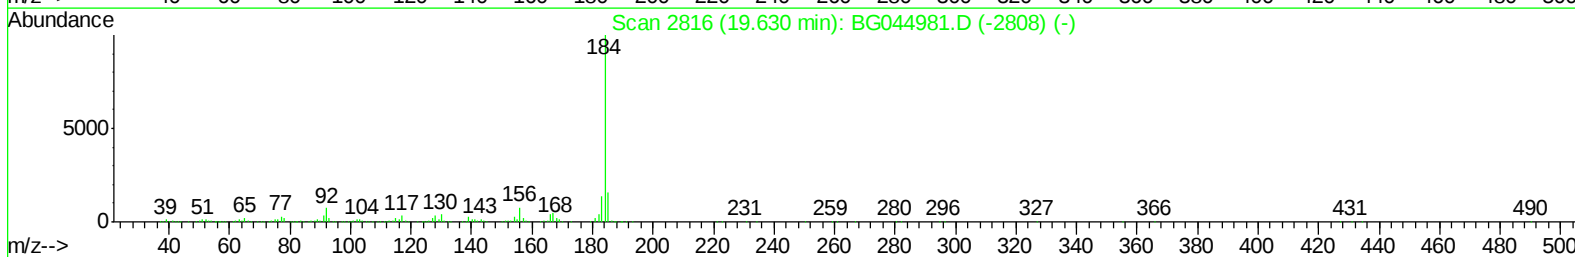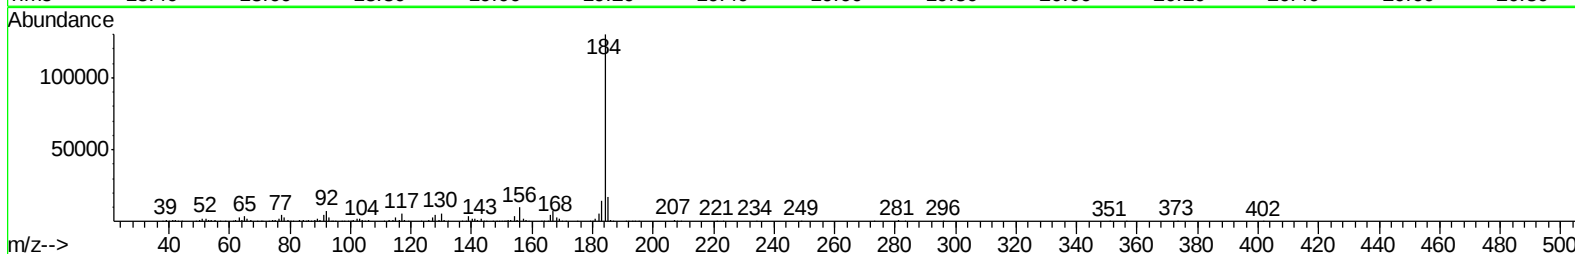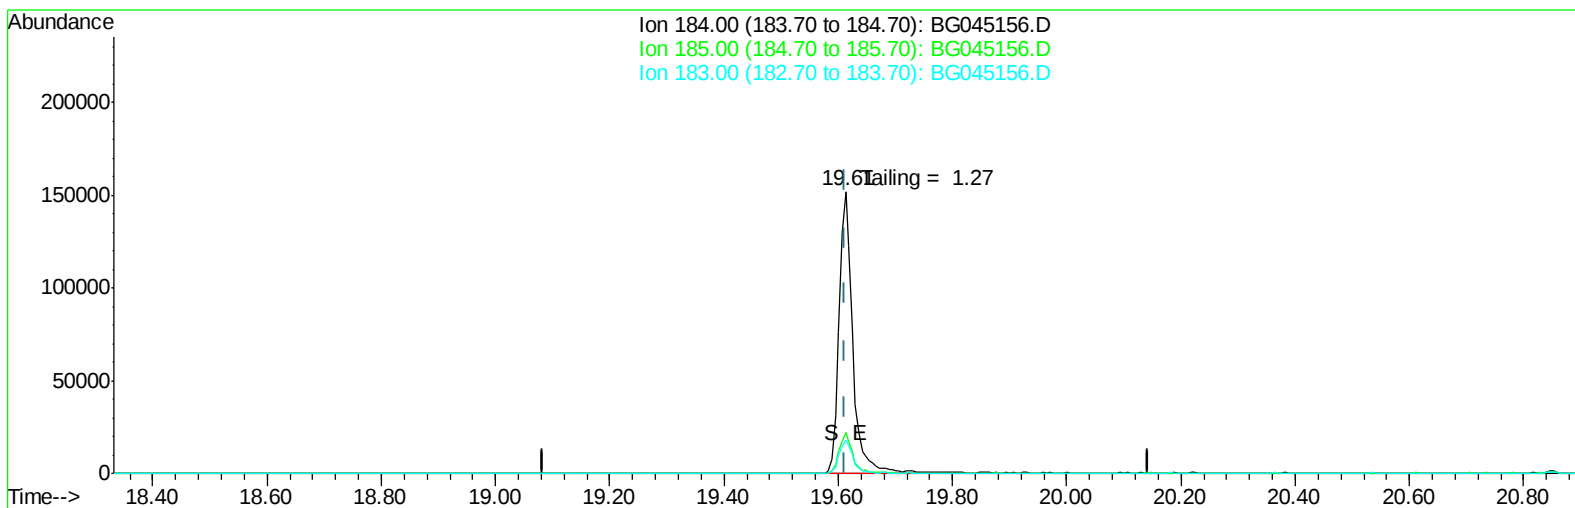

TIC: BG045156.D

(77) Benzidine

19.612min (-0.000) 144946.90ng

response 251354

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.53
183.00	14.10	12.01
0.00	0.00	0.00