


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042420\
 Data File : BG045156.D
 Acq On : 24 Apr 2020 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 13:58:55 2020

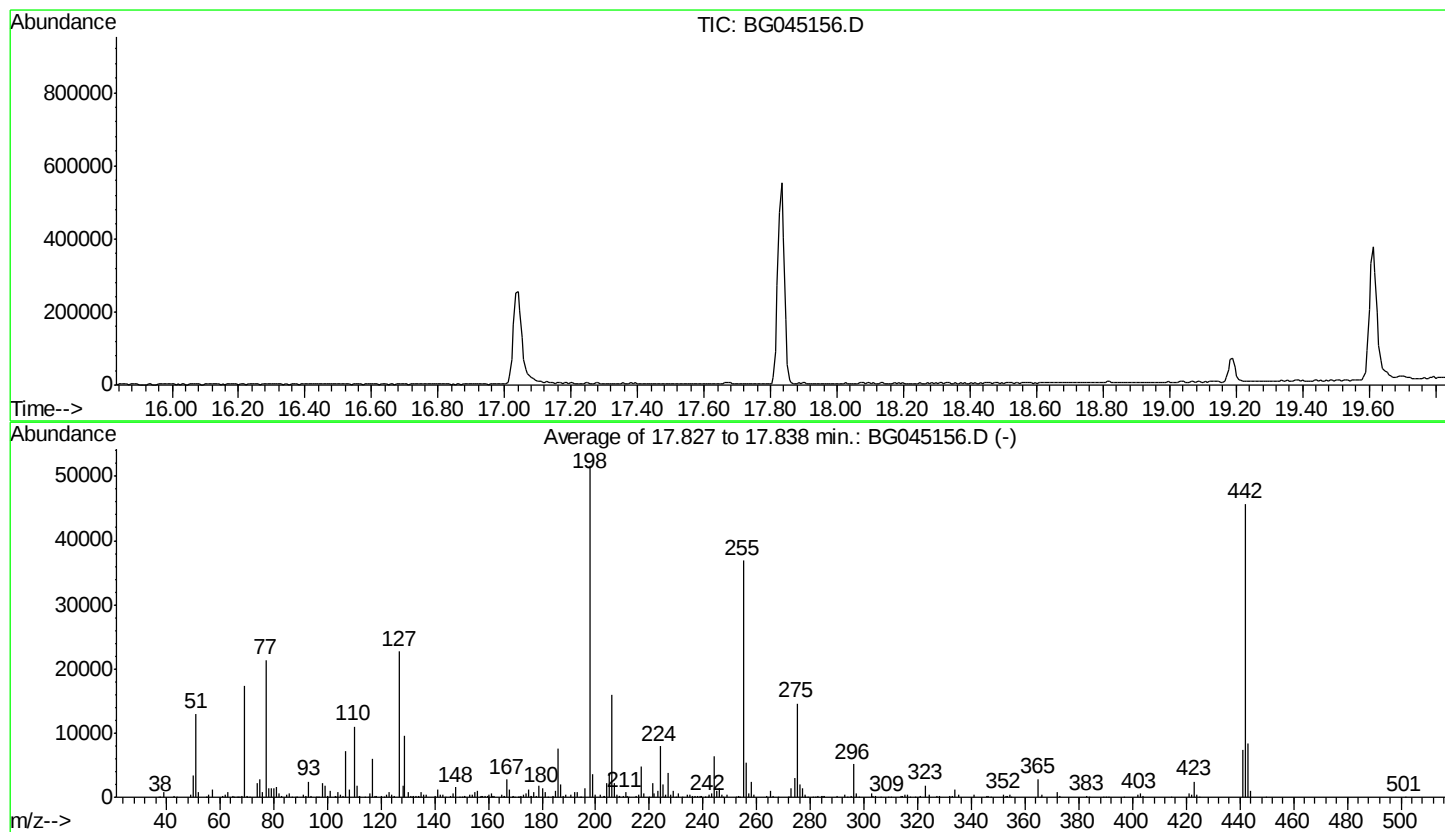

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	13039	PASS
68	69	0.00	2	0.9	164	PASS
69	198	0.00	100	33.8	17445	PASS
70	69	0.00	2	0.6	109	PASS
127	198	10	80	43.9	22709	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51672	PASS
199	198	5	9	6.9	3561	PASS
275	198	10	60	28.3	14641	PASS
365	198	1	100	5.4	2814	PASS
441	198	0.01	100	14.2	7343	PASS
442	198	50	100	88.4	45682	PASS
443	442	15	24	18.3	8362	PASS