
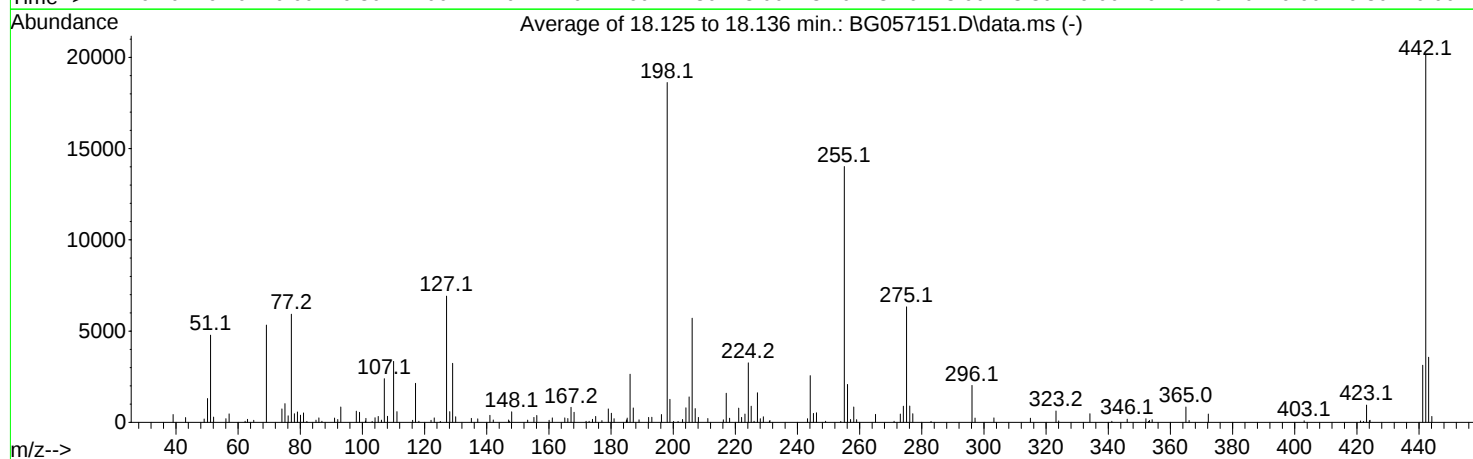


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042423\
Data File : BG057151.D
Acq On : 24 Apr 2023 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 25 04:59:02 2023

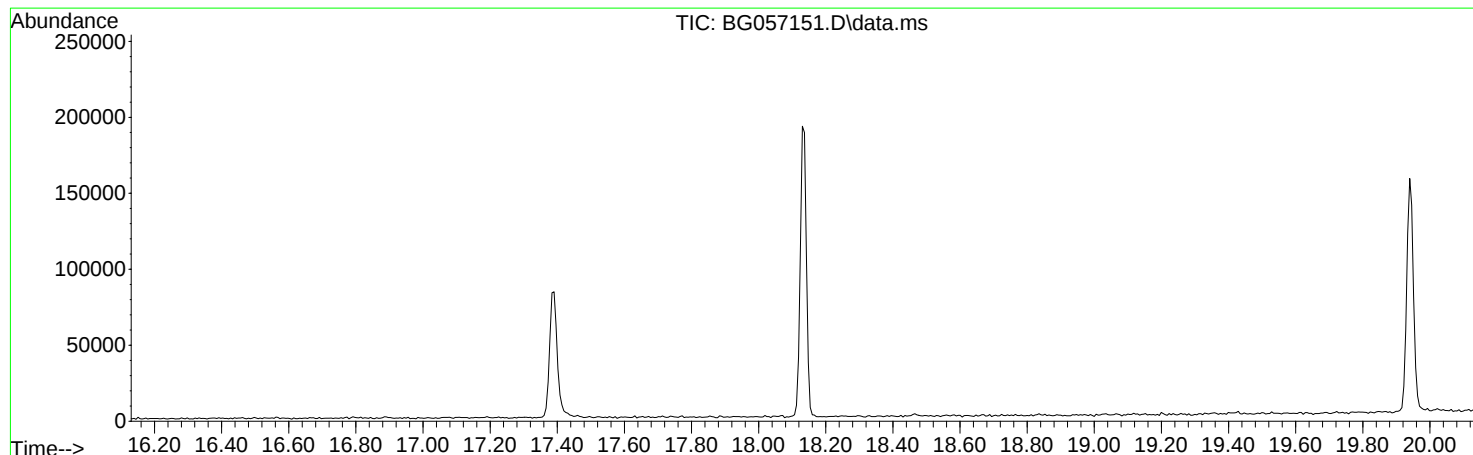

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	4781	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.6	5327	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.1	6914	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18622	PASS
199	198	5	9	6.8	1260	PASS
275	198	10	60	34.0	6330	PASS
365	198	1	100	4.5	844	PASS
441	198	0.01	100	16.8	3126	PASS
442	442	50	100	100.0	20156	PASS
443	442	15	24	17.7	3566	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/24/2023	BNA_G	<u>BG057151.D</u>
Compound Name	Response	Retention Time
DDT	54973	21.179
DDD	2157	20.721
DDE	0	20.217
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2157	57130	3.78

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042423\
Data File : BG057151.D
Acq On : 24 Apr 2023 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 25 05:48:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 04:59:02 2023
Response via : Initial Calibration

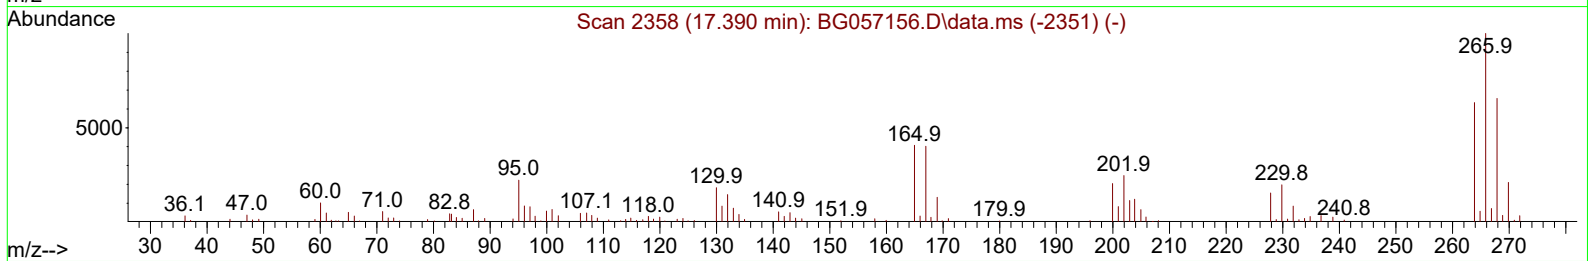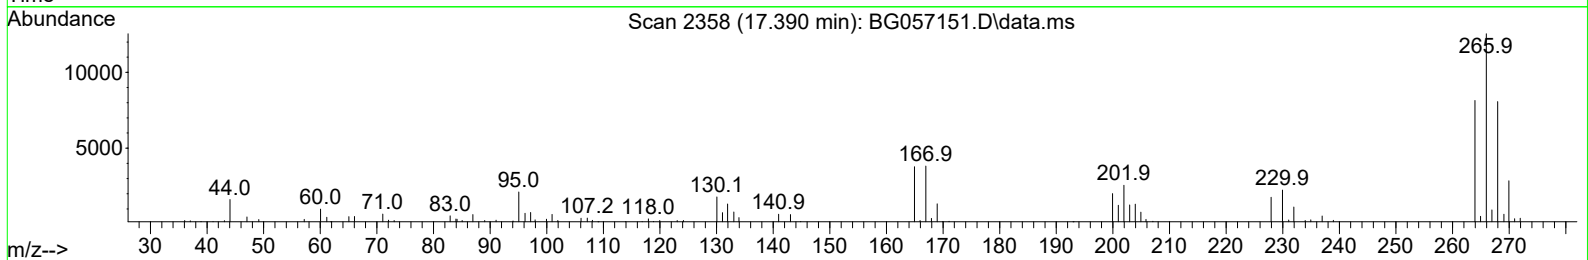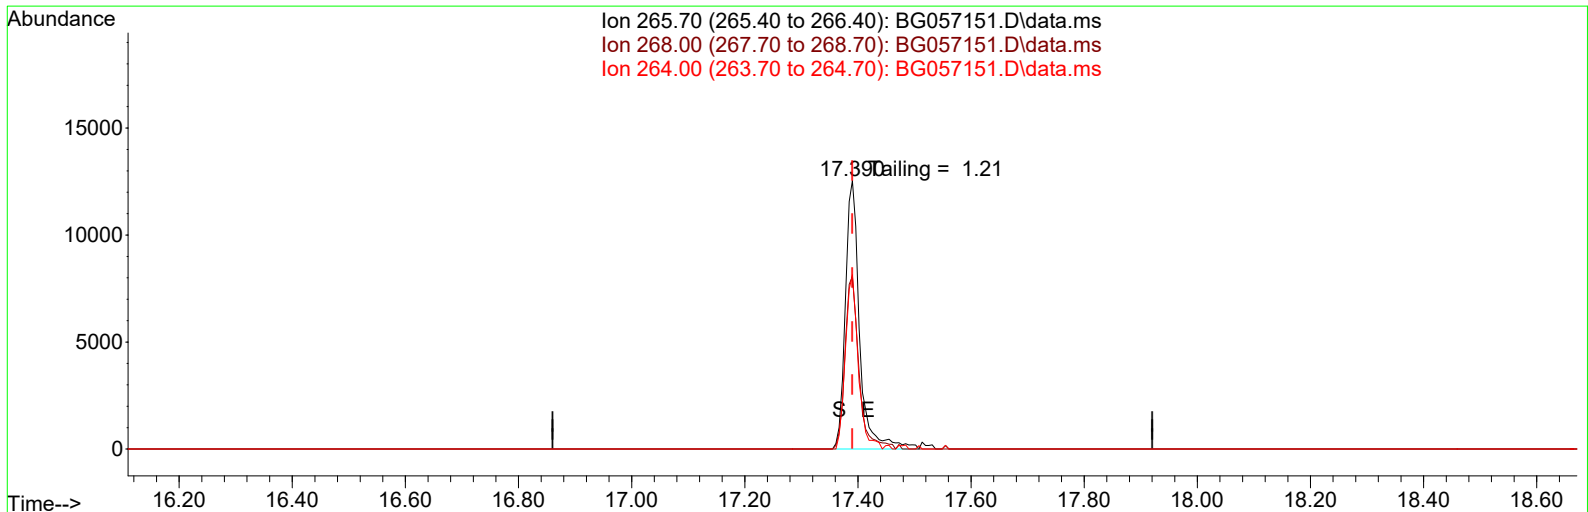

TIC: BG057151.D\data.ms

(70) Pentachlorophenol (C)

17.390min (+ 0.000) 0.00 ng




response 21087

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	64.34
264.00	63.40	64.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042423\
Data File : BG057151.D
Acq On : 24 Apr 2023 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 25 05:48:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 04:59:02 2023
Response via : Initial Calibration

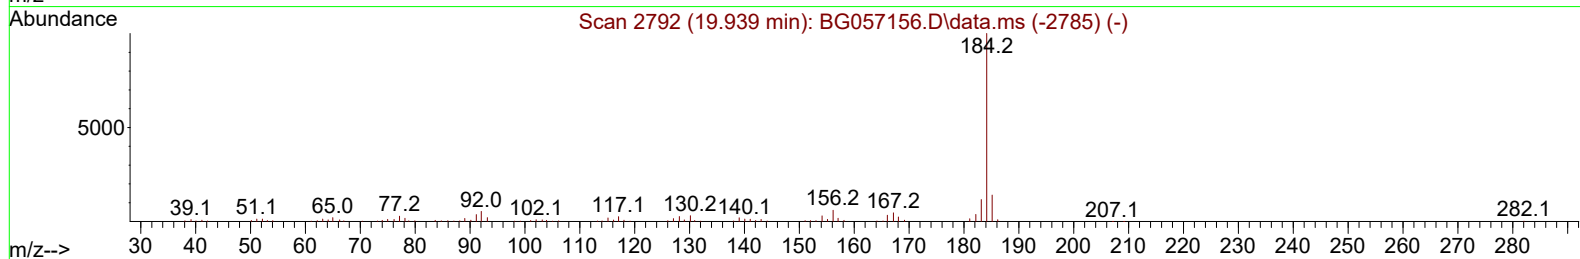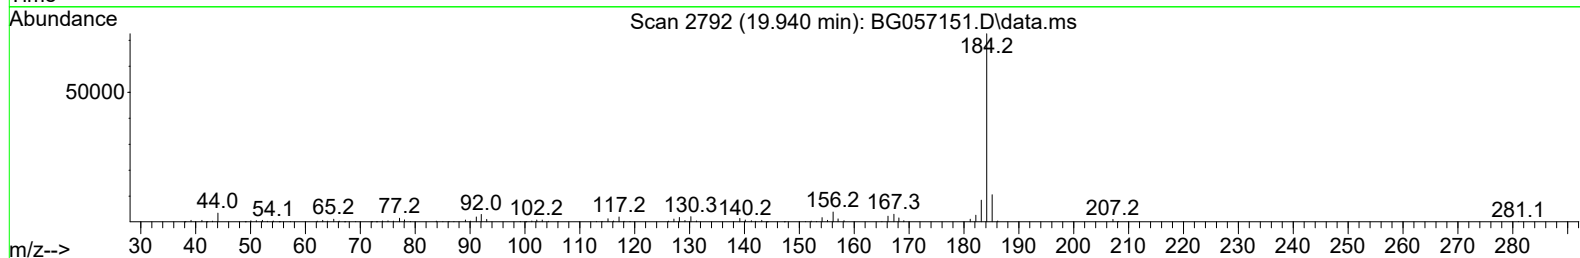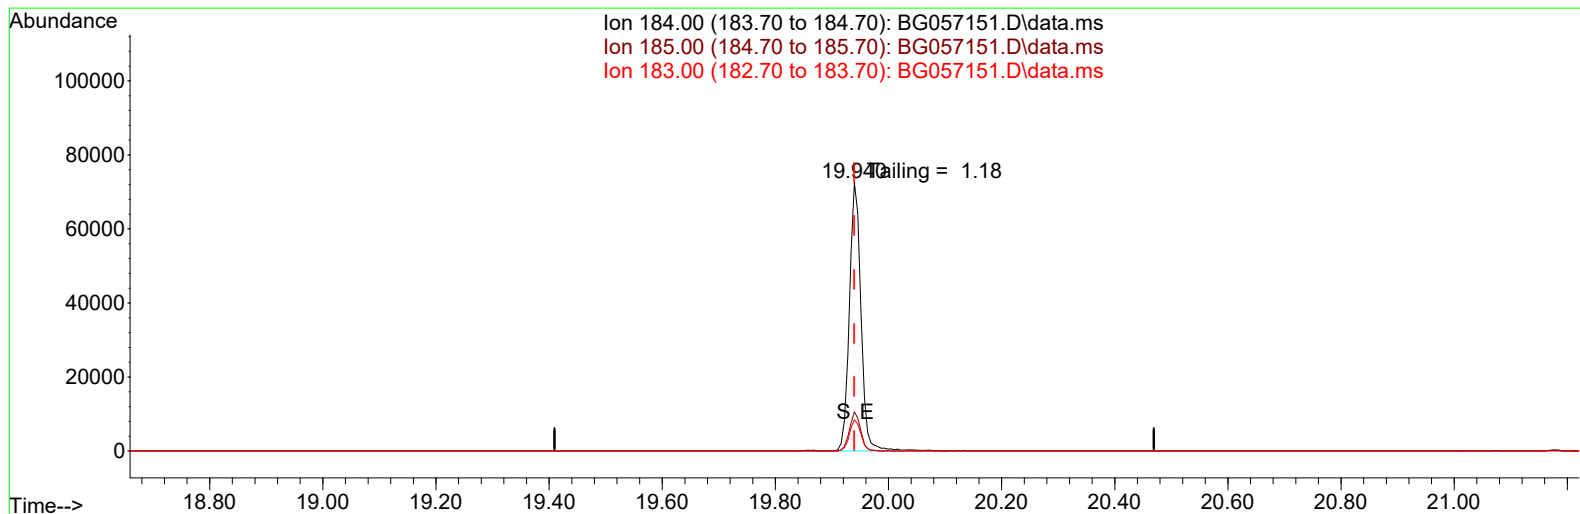

TIC: BG057151.D\data.ms

(77) Benzidine

19.940min (+ 0.000) 0.00 ng

response 103177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.59
183.00	11.70	11.66
0.00	0.00	0.00