


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042424\
Data File : BG061018.D
Acq On : 24 Apr 2024 9:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 22 04:22:00 2024

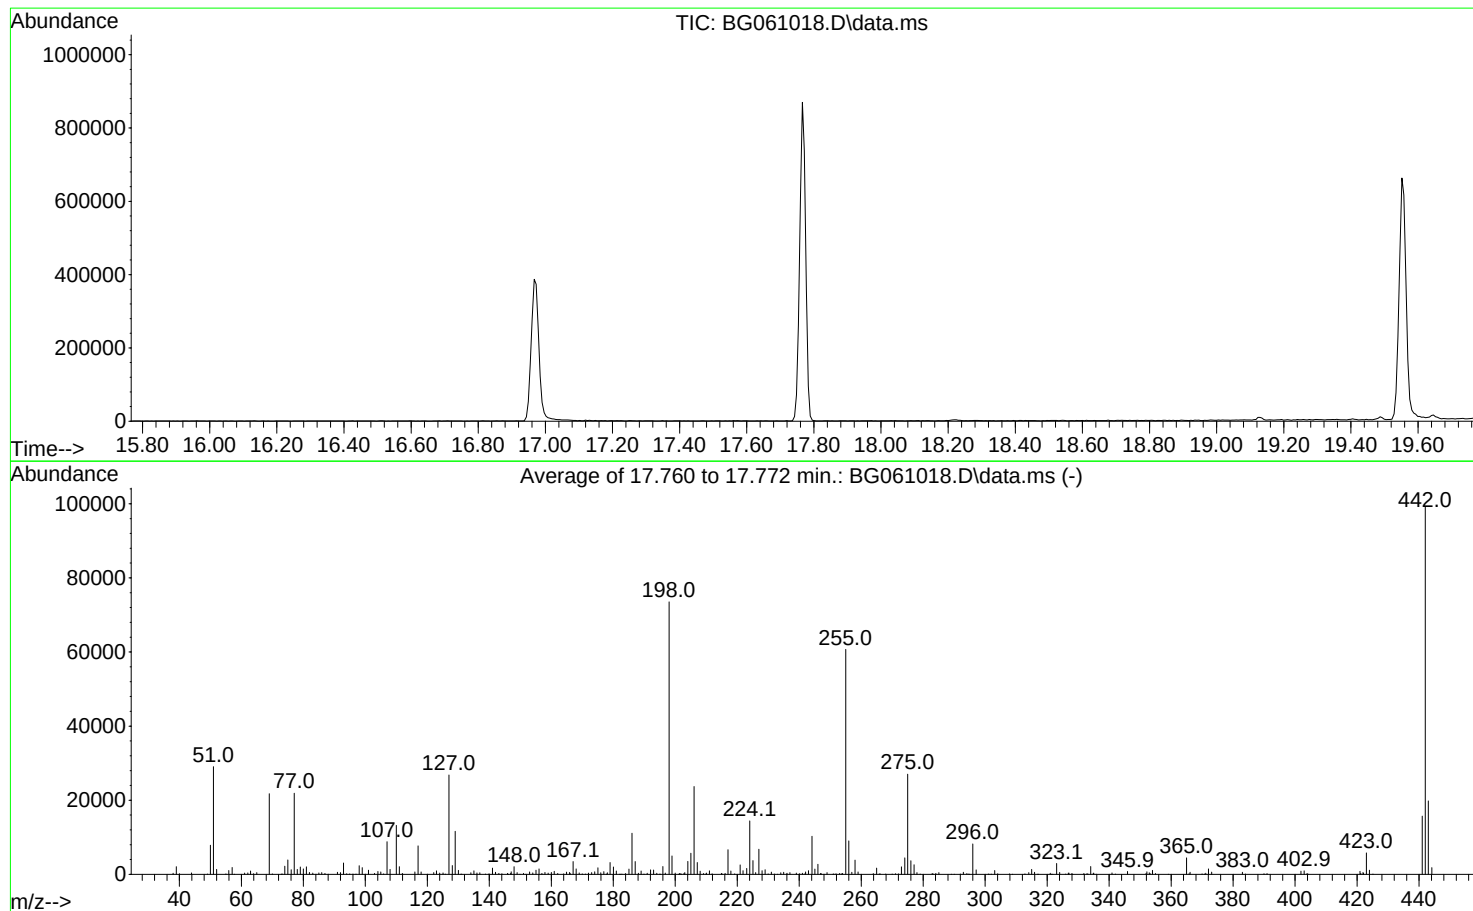




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	29077	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.6	21781	PASS
70	69	0.00	2	0.6	123	PASS
127	198	10	80	36.5	26821	PASS
197	198	0.00	2	0.5	335	PASS
198	198	100	100	100.0	73523	PASS
199	198	5	9	6.8	4989	PASS
275	198	10	60	36.8	27051	PASS
365	198	1	100	6.1	4463	PASS
441	198	0.01	100	21.4	15698	PASS
442	442	50	100	100.0	99264	PASS
443	442	15	24	20.0	19808	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042424\
Data File : BG061018.D
Acq On : 24 Apr 2024 9:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 24 11:36:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

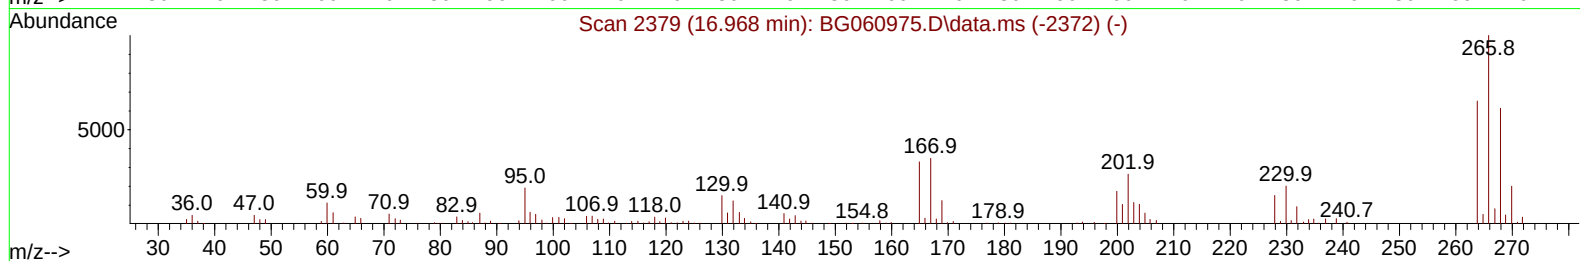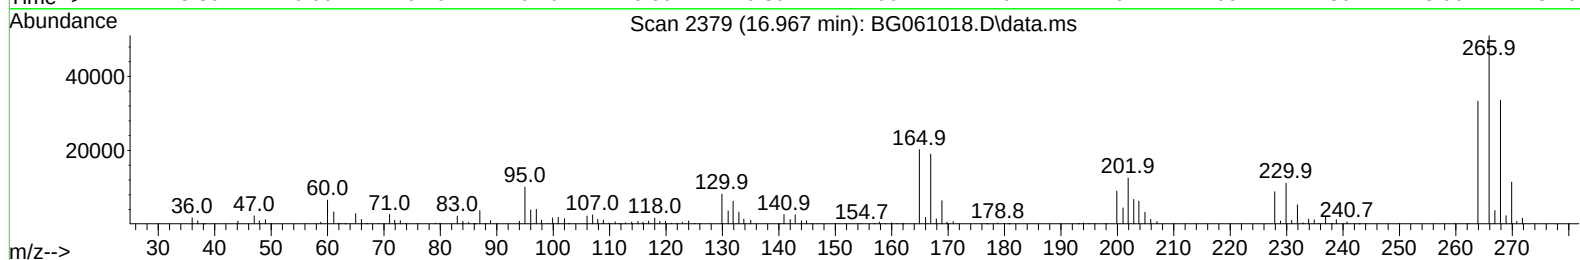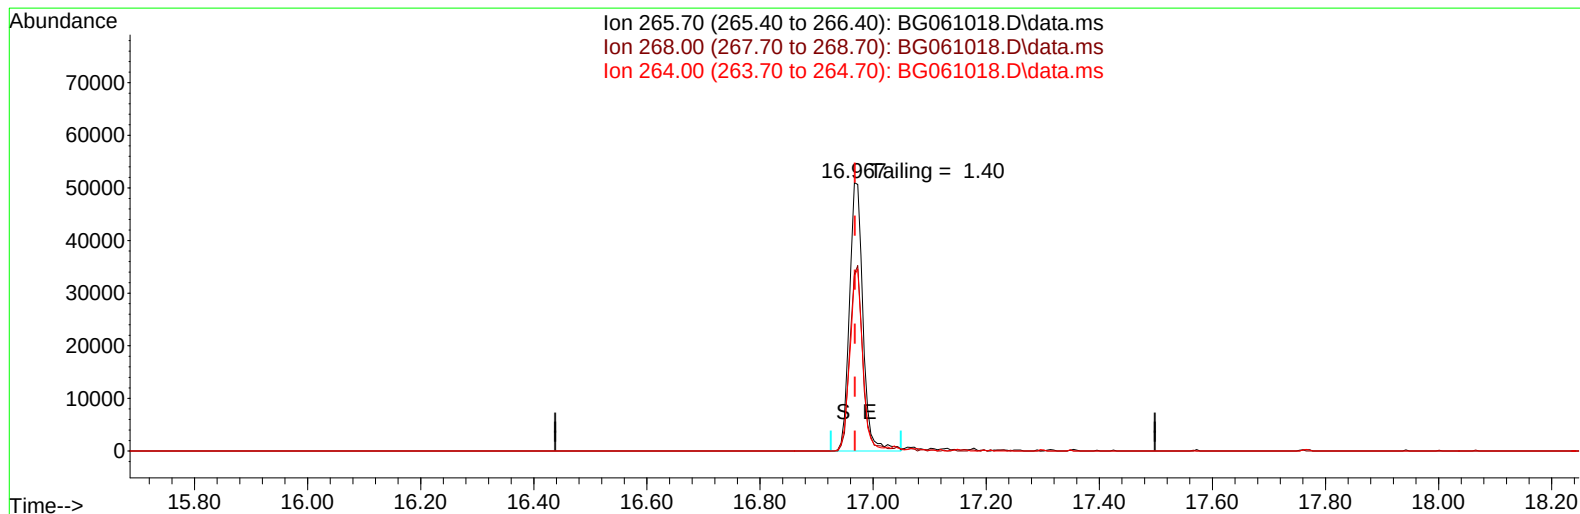

TIC: BG061018.D\data.ms

(70) Pentachlorophenol (C)

16.967min (-0.001) 164714.79 ng




response 85023

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	65.84
264.00	65.20	65.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042424\
Data File : BG061018.D
Acq On : 24 Apr 2024 9:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 24 11:36:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

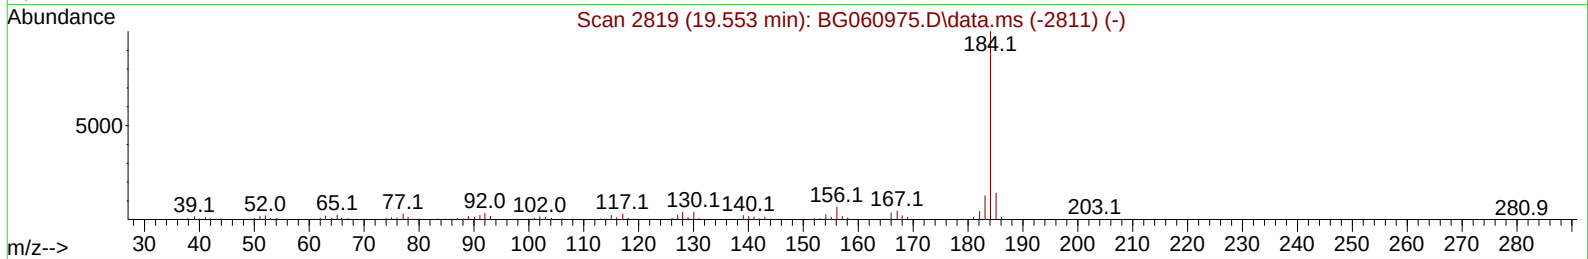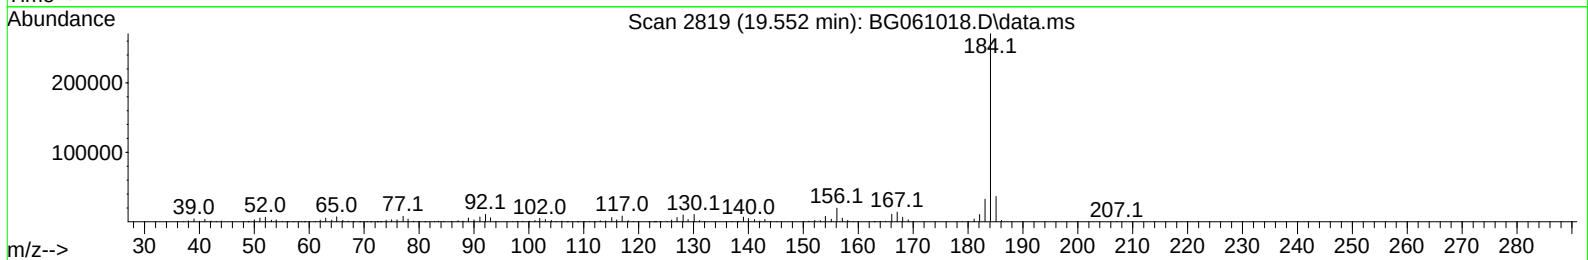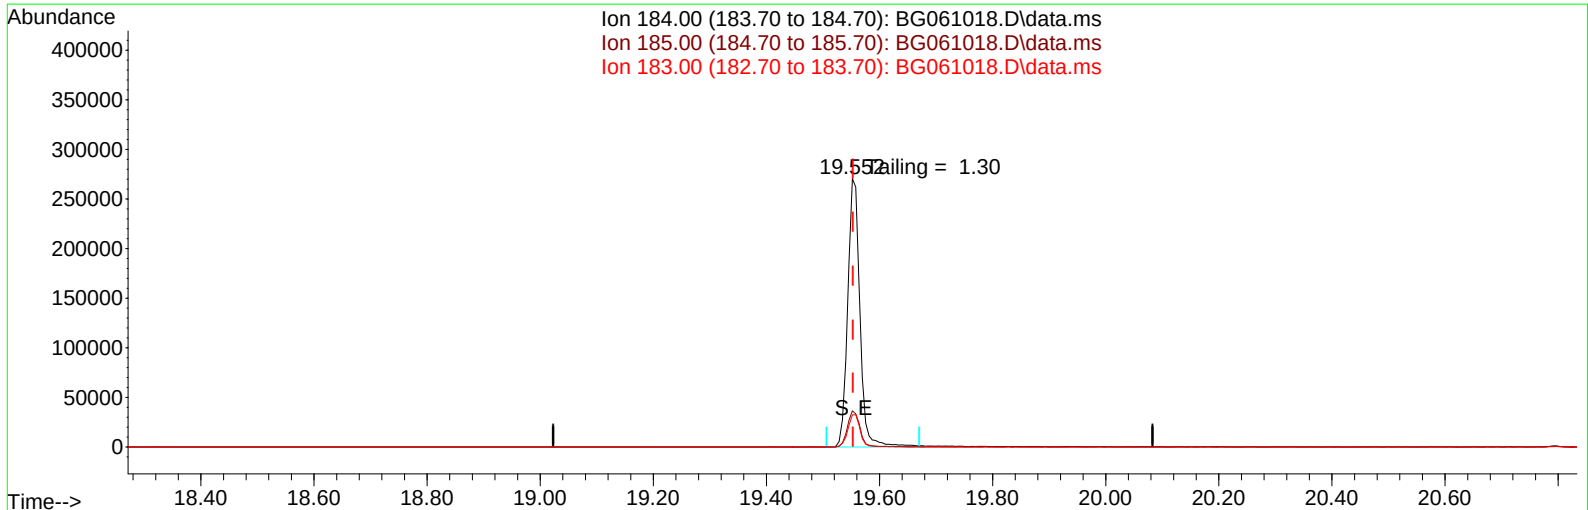

TIC: BG061018.D\data.ms

(77) Benzidine

19.552min (-0.001) 5727.58 ng m

response 406780

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.51
183.00	12.70	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/24/2024	BNA_G	<u>BG061018.D</u>
Compound Name	Response	Retention Time
DDT	257328	20.792
DDD	14513	20.351
DDE	1139	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15652	272980	5.73

Instrument :
BNA_G
ClientSampleId :
DFTPP